

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
 Data File : BM007442.D
 Acq On : 07 Sep 2016 16:29
 Operator : UM/SJ
 Sample : H4666-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	737	744	755	rBV	454968	802812	13.27%	1.474%
2	7.128	766	772	780	rBV	362754	566436	9.36%	1.040%
3	7.328	794	806	814	rBV	468355	777604	12.85%	1.427%
4	7.792	878	885	895	rVB	688172	1100800	18.19%	2.021%
5	8.492	997	1004	1014	rBV2	643765	1043093	17.24%	1.915%
6	8.945	1074	1081	1094	rBV	497170	836618	13.83%	1.536%
7	9.663	1196	1203	1213	rBV	436467	731492	12.09%	1.343%
8	10.198	1287	1294	1312	rBV	660890	1172506	19.38%	2.152%
9	10.575	1350	1358	1366	rBV	1091685	1855434	30.66%	3.406%
10	10.716	1376	1382	1395	rBV	264475	491256	8.12%	0.902%
11	13.833	1905	1912	1916	rBV	1439464	2090306	34.54%	3.837%
12	13.880	1916	1920	1927	rVB	865359	1235151	20.41%	2.267%
13	14.116	1949	1960	1971	rBV	1677250	2548687	42.12%	4.678%
14	14.421	2003	2012	2021	rBV2	2026993	3149801	52.05%	5.782%
15	14.627	2041	2047	2063	rBV	491539	903745	14.93%	1.659%
16	15.274	2152	2157	2161	rVB	61570	78836	1.30%	0.145%
17	15.415	2174	2181	2191	rVB	2377779	3430987	56.70%	6.298%
18	15.539	2196	2202	2217	rBV	586820	845108	13.97%	1.551%
19	15.657	2217	2222	2229	rBV5	38430	81494	1.35%	0.150%
20	16.133	2298	2303	2311	rBV	94876	164250	2.71%	0.301%
21	16.921	2433	2437	2442	rBV	64550	95206	1.57%	0.175%
22	17.168	2472	2479	2486	rBV	3052812	4393928	72.61%	8.065%
23	17.262	2488	2495	2505	rVB	2732231	4085711	67.52%	7.500%
24	18.051	2625	2629	2634	rBV3	43411	60529	1.00%	0.111%
25	19.556	2879	2885	2898	rBV	3614627	5199823	85.93%	9.545%
26	21.050	3135	3139	3149	rBV5	105539	216544	3.58%	0.397%
27	21.344	3183	3189	3200	rBV	4643930	6051391	100.00%	11.108%
28	22.391	3365	3367	3372	rVB3	62898	74054	1.22%	0.136%
29	22.903	3451	3454	3460	rVB3	67168	98082	1.62%	0.180%
30	23.468	3543	3550	3561	rBV2	2421641	4649601	76.84%	8.535%
31	23.615	3567	3575	3586	rBV	2674940	5138125	84.91%	9.432%
32	24.127	3657	3662	3668	rVB2	134426	237653	3.93%	0.436%
33	24.880	3785	3790	3801	rVB2	120241	271013	4.48%	0.497%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007442.D
Acq On : 07 Sep 2016 16:29
Operator : UM/SJ
Sample : H4666-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Title : SVOA CALIBRATION


Sum of corrected areas: 54478076

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007442.D
Acq On : 07 Sep 2016 16:29
Operator : UM/SJ
Sample : H4666-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

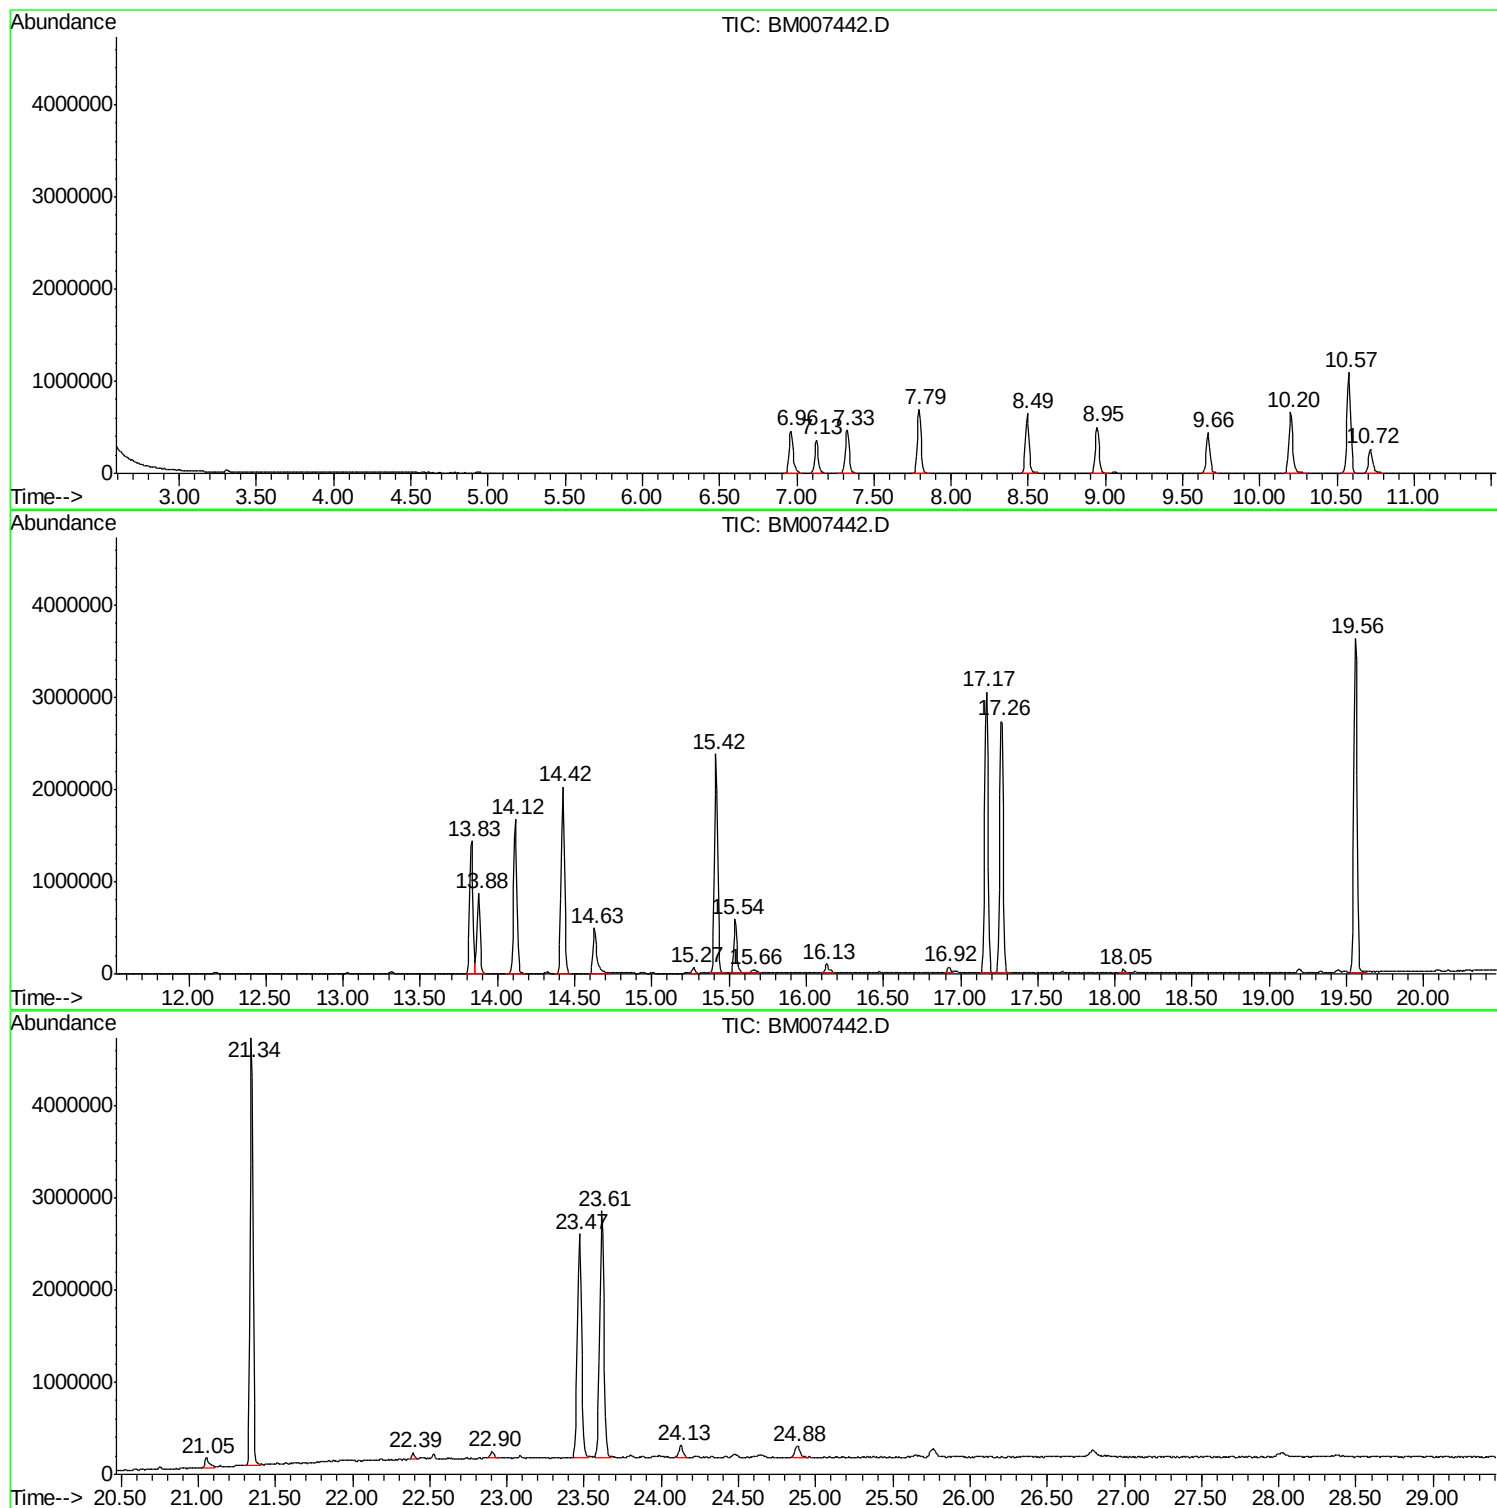

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007442.D
Acq On : 07 Sep 2016 16:29
Operator : UM/SJ
Sample : H4666-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007442.D
Acq On : 07 Sep 2016 16:29
Operator : UM/SJ
Sample : H4666-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc