

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
 Data File : BM007444.D
 Acq On : 07 Sep 2016 18:17
 Operator : UM/SJ
 Sample : H4666-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3A6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	735	744	759	rVB	770950	1337089	16.07%	1.739%
2	7.128	762	772	782	rBV	603615	959407	11.53%	1.248%
3	7.328	799	806	817	rBV	776717	1287007	15.46%	1.674%
4	7.792	878	885	899	rVB	707874	1143546	13.74%	1.487%
5	8.492	997	1004	1014	rBV	1089200	1788992	21.49%	2.327%
6	8.945	1073	1081	1095	rBV	845528	1428363	17.16%	1.858%
7	9.663	1196	1203	1216	rBV	751377	1275243	15.32%	1.659%
8	10.198	1287	1294	1305	rBV	1137030	1961543	23.57%	2.552%
9	10.575	1349	1358	1366	rBV	1148270	1928571	23.17%	

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007444.D
Acq On : 07 Sep 2016 18:17
Operator : UM/SJ
Sample : H4666-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Title : SVOA CALIBRATION


Sum of corrected areas: 76877171

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007444.D
Acq On : 07 Sep 2016 18:17
Operator : UM/SJ
Sample : H4666-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

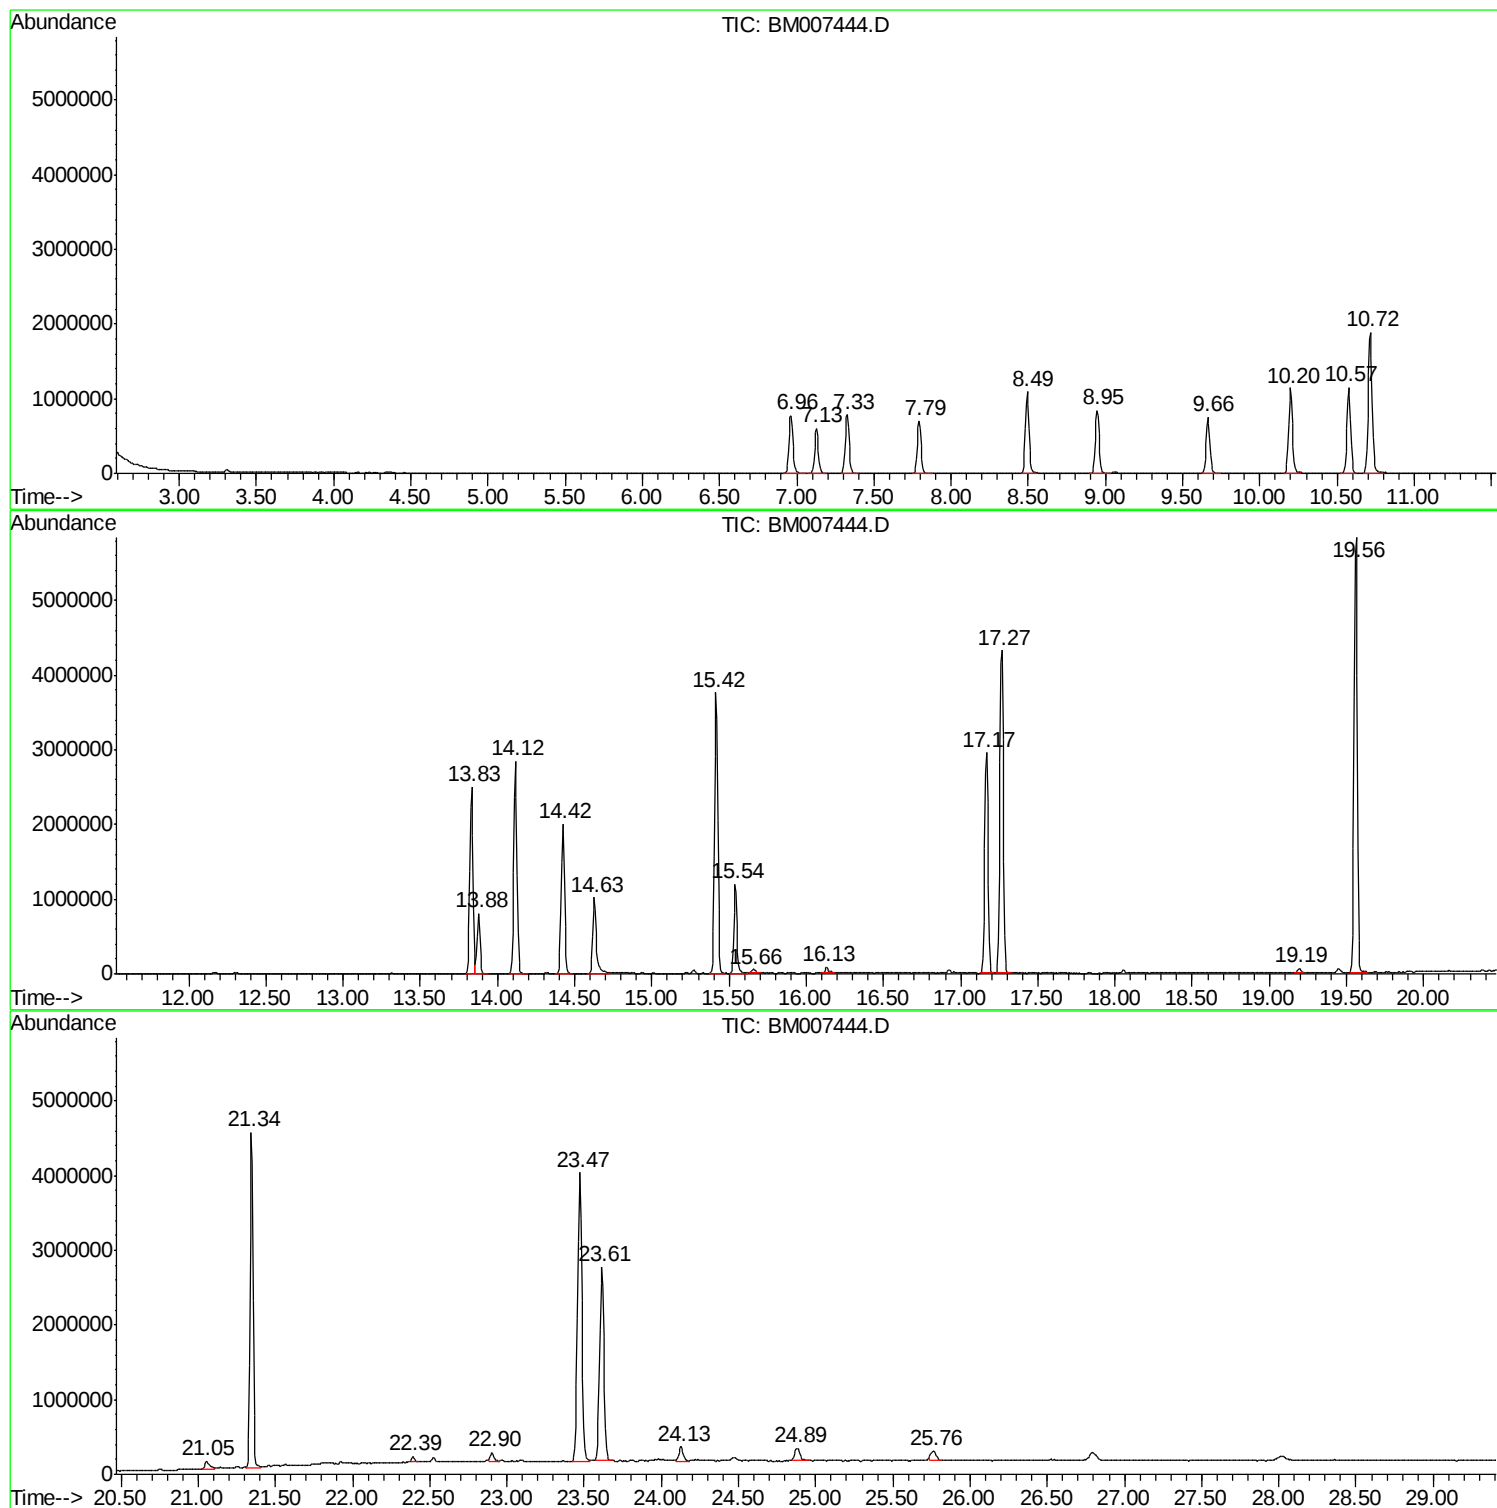

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007444.D
Acq On : 07 Sep 2016 18:17
Operator : UM/SJ
Sample : H4666-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090716\
Data File : BM007444.D
Acq On : 07 Sep 2016 18:17
Operator : UM/SJ
Sample : H4666-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc