
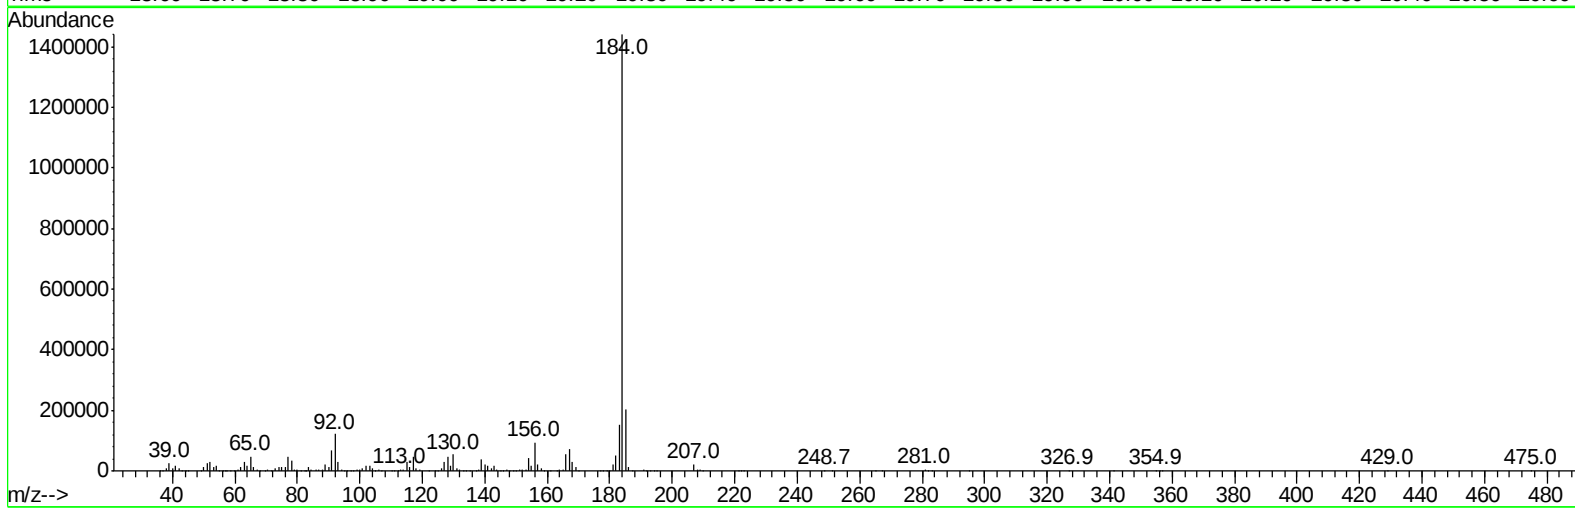


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090717\
Data File : BM011454.D
Acq On : 07 Sep 2017 14:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 08:45:27 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

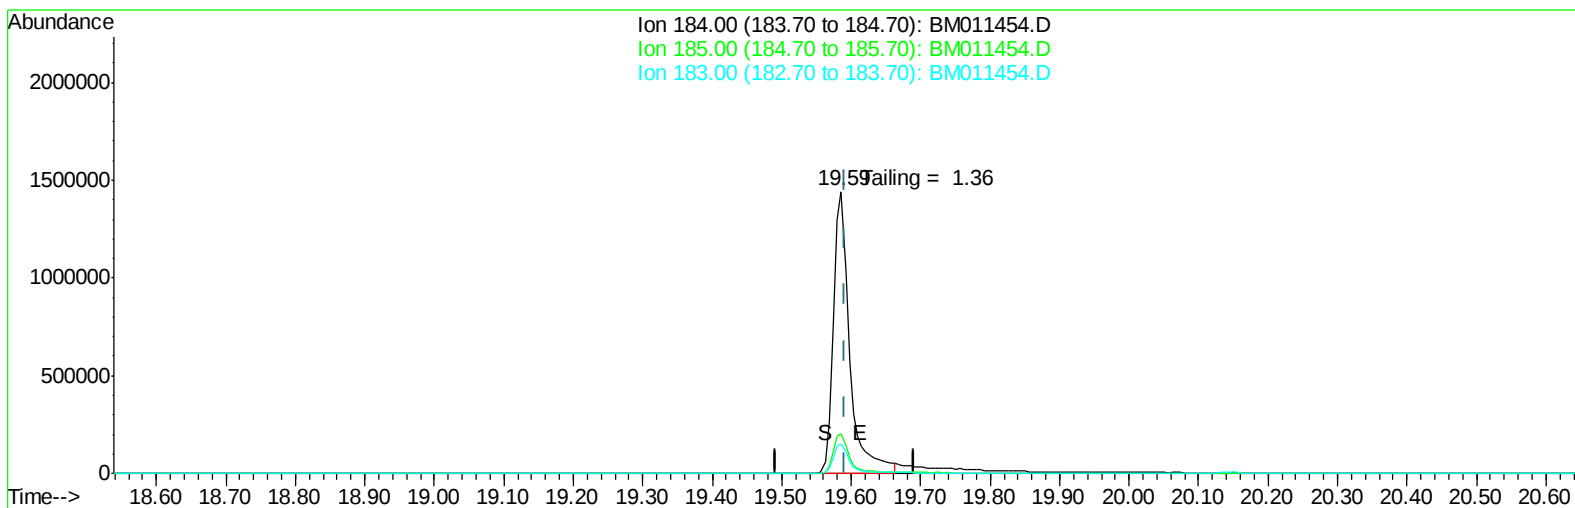

TIC: BM011454.D

(76) Benzidine



19.586min (-0.006) 3320.41ng

response 2288947

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.09
183.00	11.10	10.61
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM090717\
Data File : BM011454.D
Acq On : 07 Sep 2017 14:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 08 08:45:27 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM083117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 18:39:59 2017
Response via : Initial Calibration

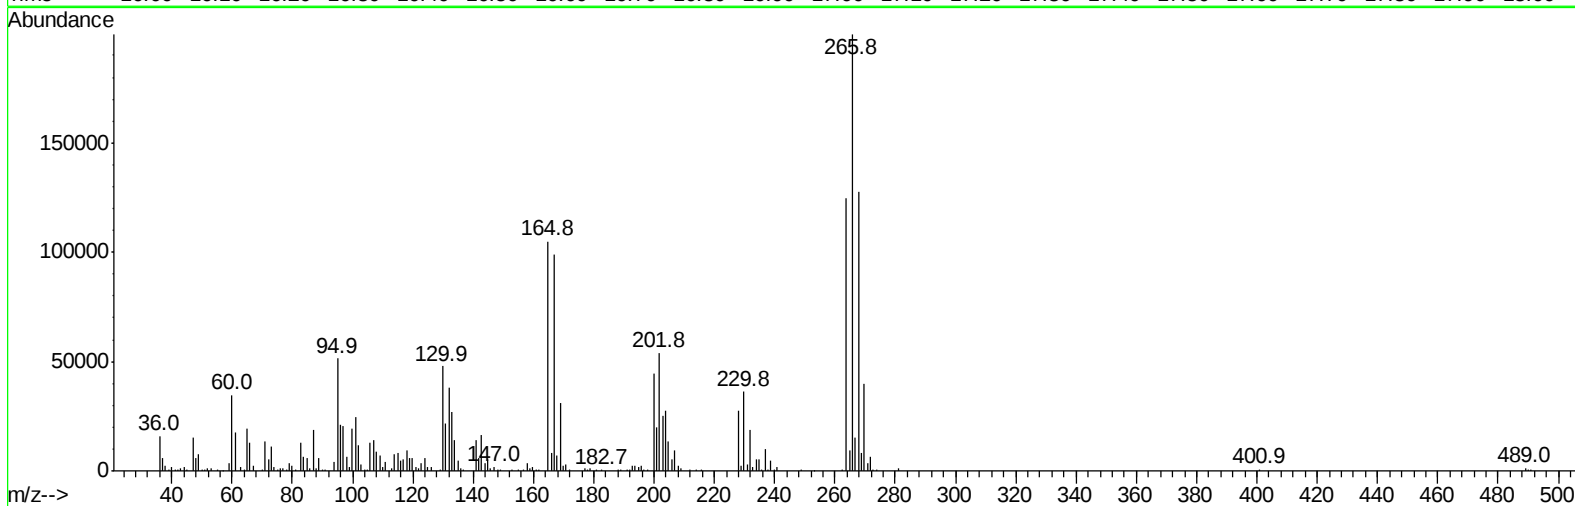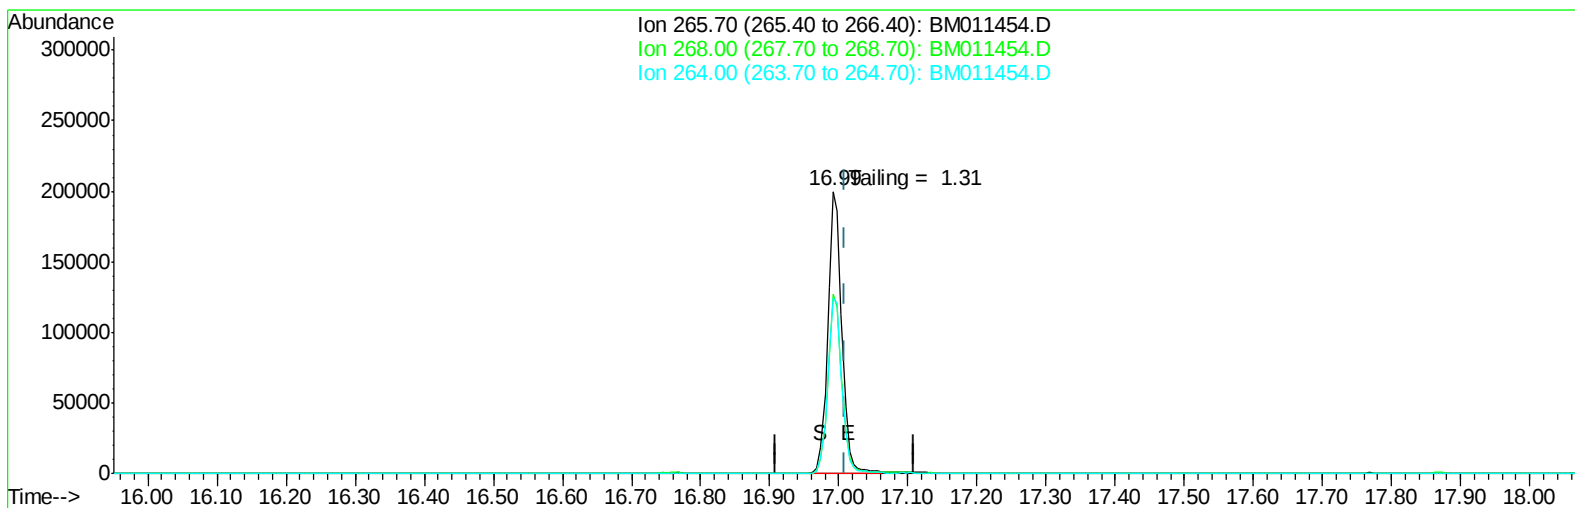

TIC: BM011454.D

(69) Pentachlorophenol (C)

16.992min (-0.018) 53887.65ng

response 279725

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.83
264.00	61.20	62.33
0.00	0.00	0.00