


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM090717\
 Data File : BM011454.D
 Acq On : 07 Sep 2017 14:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM083117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 18:39:59 2017

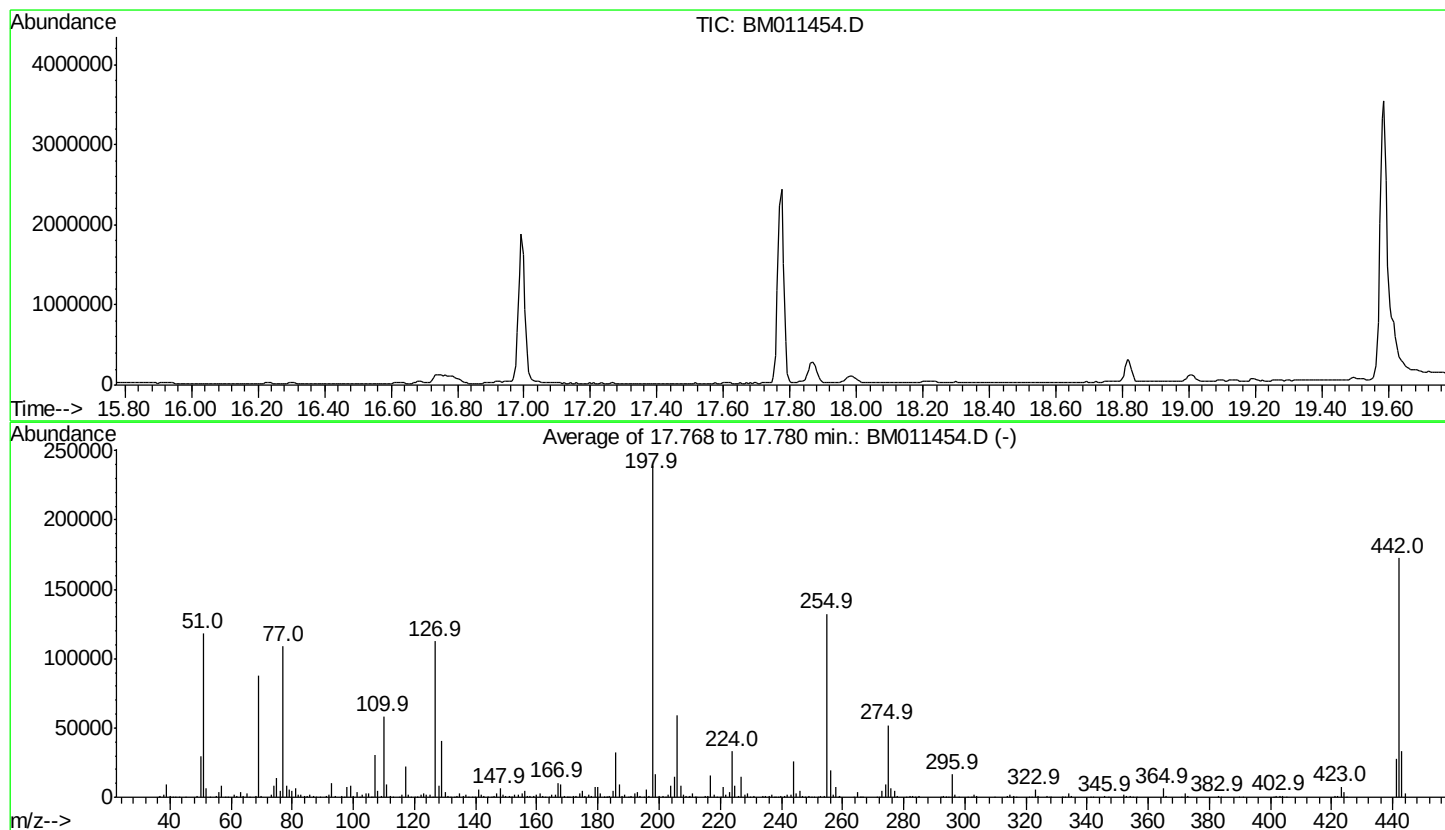

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	117906	PASS
68	69	0.00	2	1.4	1262	PASS
69	198	0.00	100	36.6	87482	PASS
70	69	0.00	2	0.6	541	PASS
127	198	10	80	46.9	112314	PASS
197	198	0.00	2	0.3	707	PASS
198	198	100	100	100.0	239232	PASS
199	198	5	9	6.8	16344	PASS
275	198	10	60	21.8	52138	PASS
365	198	1	100	2.7	6454	PASS
441	443	0.01	100	82.4	27696	PASS
442	198	50	100	72.1	172586	PASS
443	442	15	24	19.5	33632	PASS