

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090816\
 Data File : BM007461.D
 Acq On : 08 Sep 2016 19:16
 Operator : UM/SJ
 Sample : H4692-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C4

Quant Time: Sep 09 03:04:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 09 03:02:55 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	225739	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	1045305	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.42	164	727223	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	1903122	20.00	ng/ul	0.00
75) Chrysene-d12	21.34	240	2685239	20.00	ng/ul	0.00
83) Perylene-d12	23.62	264	2844401	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	5147	1.17	ng/uL	0.00
5) Phenol-d5	6.96	99	107722	5.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	289574	25.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	311330	19.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	219936	11.83	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	208699	27.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	251795	28.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	408846	22.92	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	14433	0.65	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	1732666	27.62	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	2001849	27.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	58674	4.95	ng/ul	0.00
57) Fluorene-d10	15.42	176	1485271	27.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	311071	25.99	ng/ul	0.00
70) Anthracene-d10	17.26	188	2533558	28.50	ng/ul	0.00
76) Pyrene-d10	19.56	212	3196388	28.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.47	264	3718928	28.39	ng/ul	0.00


Target Compounds					Qvalue
56) Diethylphthalate	15.24	149	71501	1.10 ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090816\
Data File : BM007461.D
Acq On : 08 Sep 2016 19:16
Operator : UM/SJ
Sample : H4692-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C4

Quant Time: Sep 09 03:04:05 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 09 03:02:55 2016
Response via : Initial Calibration

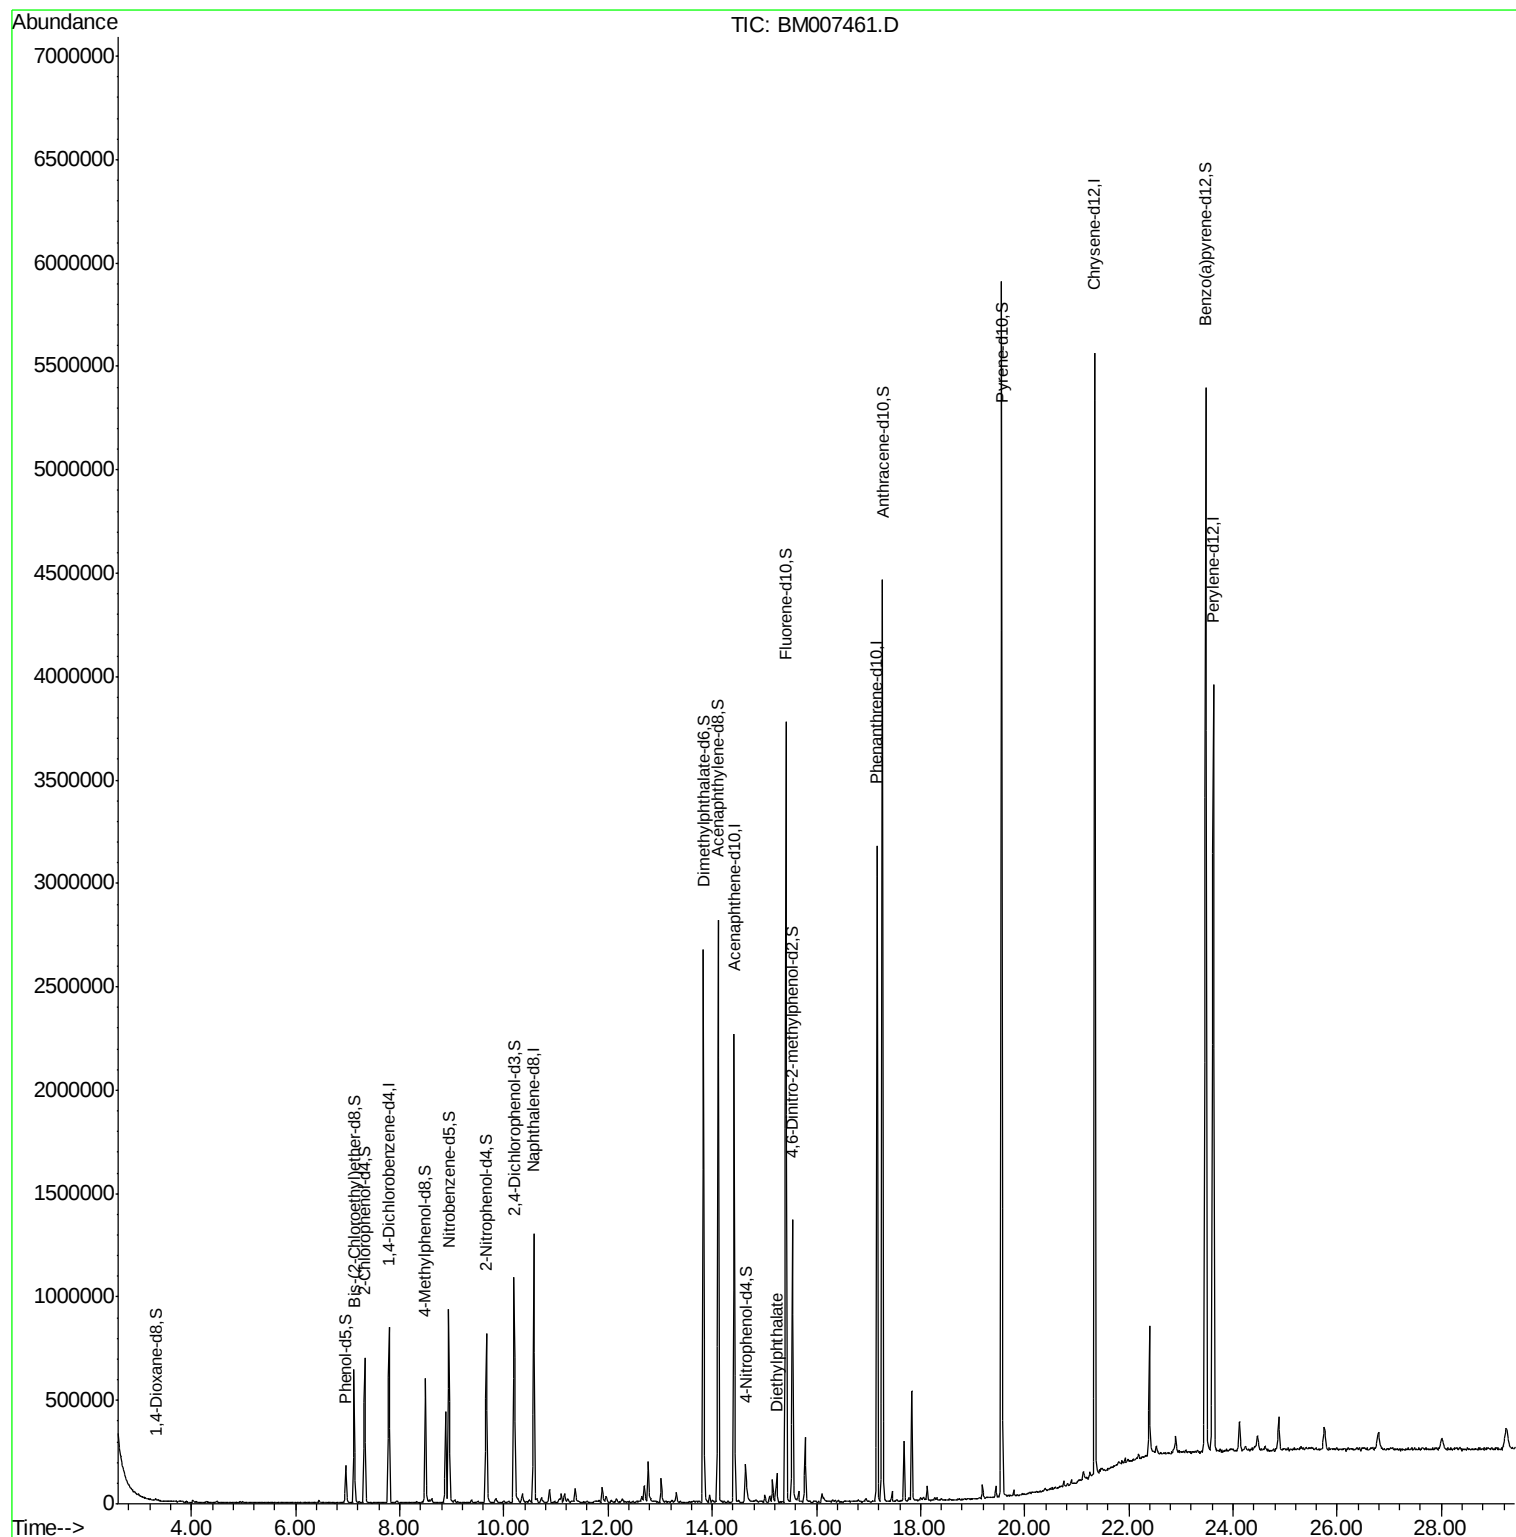


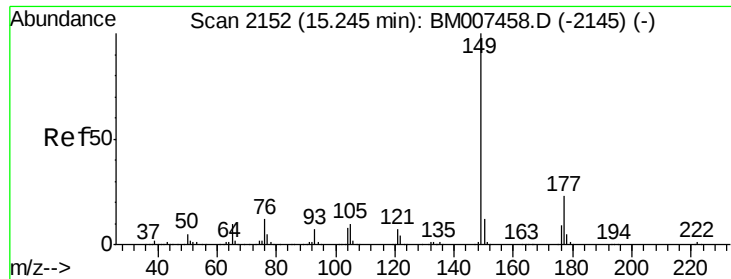

#56
 Diethylphthalate
 Concen: 1.10 ng/ul
 RT: 15.24 min Scan# 2151
 Delta R.T. -0.01 min
 Lab File: BM007461.D
 Acq: 08 Sep 2016 19:16

Instrument :
 BNA_M
 ClientSampleId :
 BD3C4

Tgt Ion	Ratio	Lower	Upper
149	100		
177	20.5	18.6	28.0
150	12.0	10.0	15.0

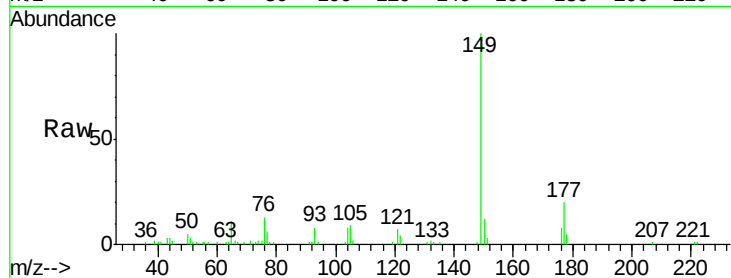

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

