

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090816\
 Data File : BM007459.D
 Acq On : 08 Sep 2016 18:04
 Operator : UM/SJ
 Sample : PB93299BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK99

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	732	744	755	rBV	782301	1303302	14.29%	1.831%
2	7.128	765	772	781	rBV	614922	989800	10.86%	1.390%
3	7.322	799	805	820	rBV	809776	1359066	14.91%	1.909%
4	7.792	876	885	892	rBV	626053	1035867	11.36%	1.455%
5	8.492	997	1004	1017	rBV	1047189	1744955	19.14%	2.451%
6	8.945	1073	1081	1095	rBV	861184	1418466	15.56%	1.993%
7	9.663	1196	1203	1216	rBV	758224	1281419	14.05%	1.800%
8	10.198	1287	1294	1311	rBV	1031306	1834302	20.12%	2.577%
9	10.575	1351	1358	1366	rBV	944453	1596670	17.51%	2.243%
10	10.716	1374	1382	1400	rBV	1098691	2031570	22.28%	2.854%
11	13.833	1905	1912	1924	rVB	2522007	3625245	39.76%	5.093%
12	14.115	1952	1960	1972	rBV	2556850	3875306	42.50%	5.444%
13	14.421	2005	2012	2023	rVB2	1610490	2520369	27.64%	3.541%
14	14.633	2039	2048	2065	rBV	1018144	1952999	21.42%	2.744%
15	15.415	2174	2181	2190	rBV	3595024	5124520	56.21%	7.199%
16	15.545	2196	2203	2218	rBV	1234134	1867024	20.48%	2.623%
17	17.168	2472	2479	2486	rBV	2385380	3461867	37.97%	4.863%
18	17.262	2489	2495	2505	rBV2	4084745	6218198	68.20%	8.735%
19	19.556	2879	2885	2896	rBV	5534996	7989001	87.62%	11.223%
20	21.344	3184	3189	3199	rBV	4030505	5211312	57.16%	7.321%
21	22.903	3451	3454	3463	rVB3	87841	143457	1.57%	0.202%
22	23.474	3543	3551	3563	rBV	4952069	9117419	100.00%	12.808%
23	23.615	3568	3575	3586	rVB2	2641441	5205699	57.10%	7.313%
24	24.127	3658	3662	3671	rVB2	140754	277790	3.05%	0.390%


Sum of corrected areas: 71185623

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090816\
Data File : BM007459.D
Acq On : 08 Sep 2016 18:04
Operator : UM/SJ
Sample : PB93299BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK99

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

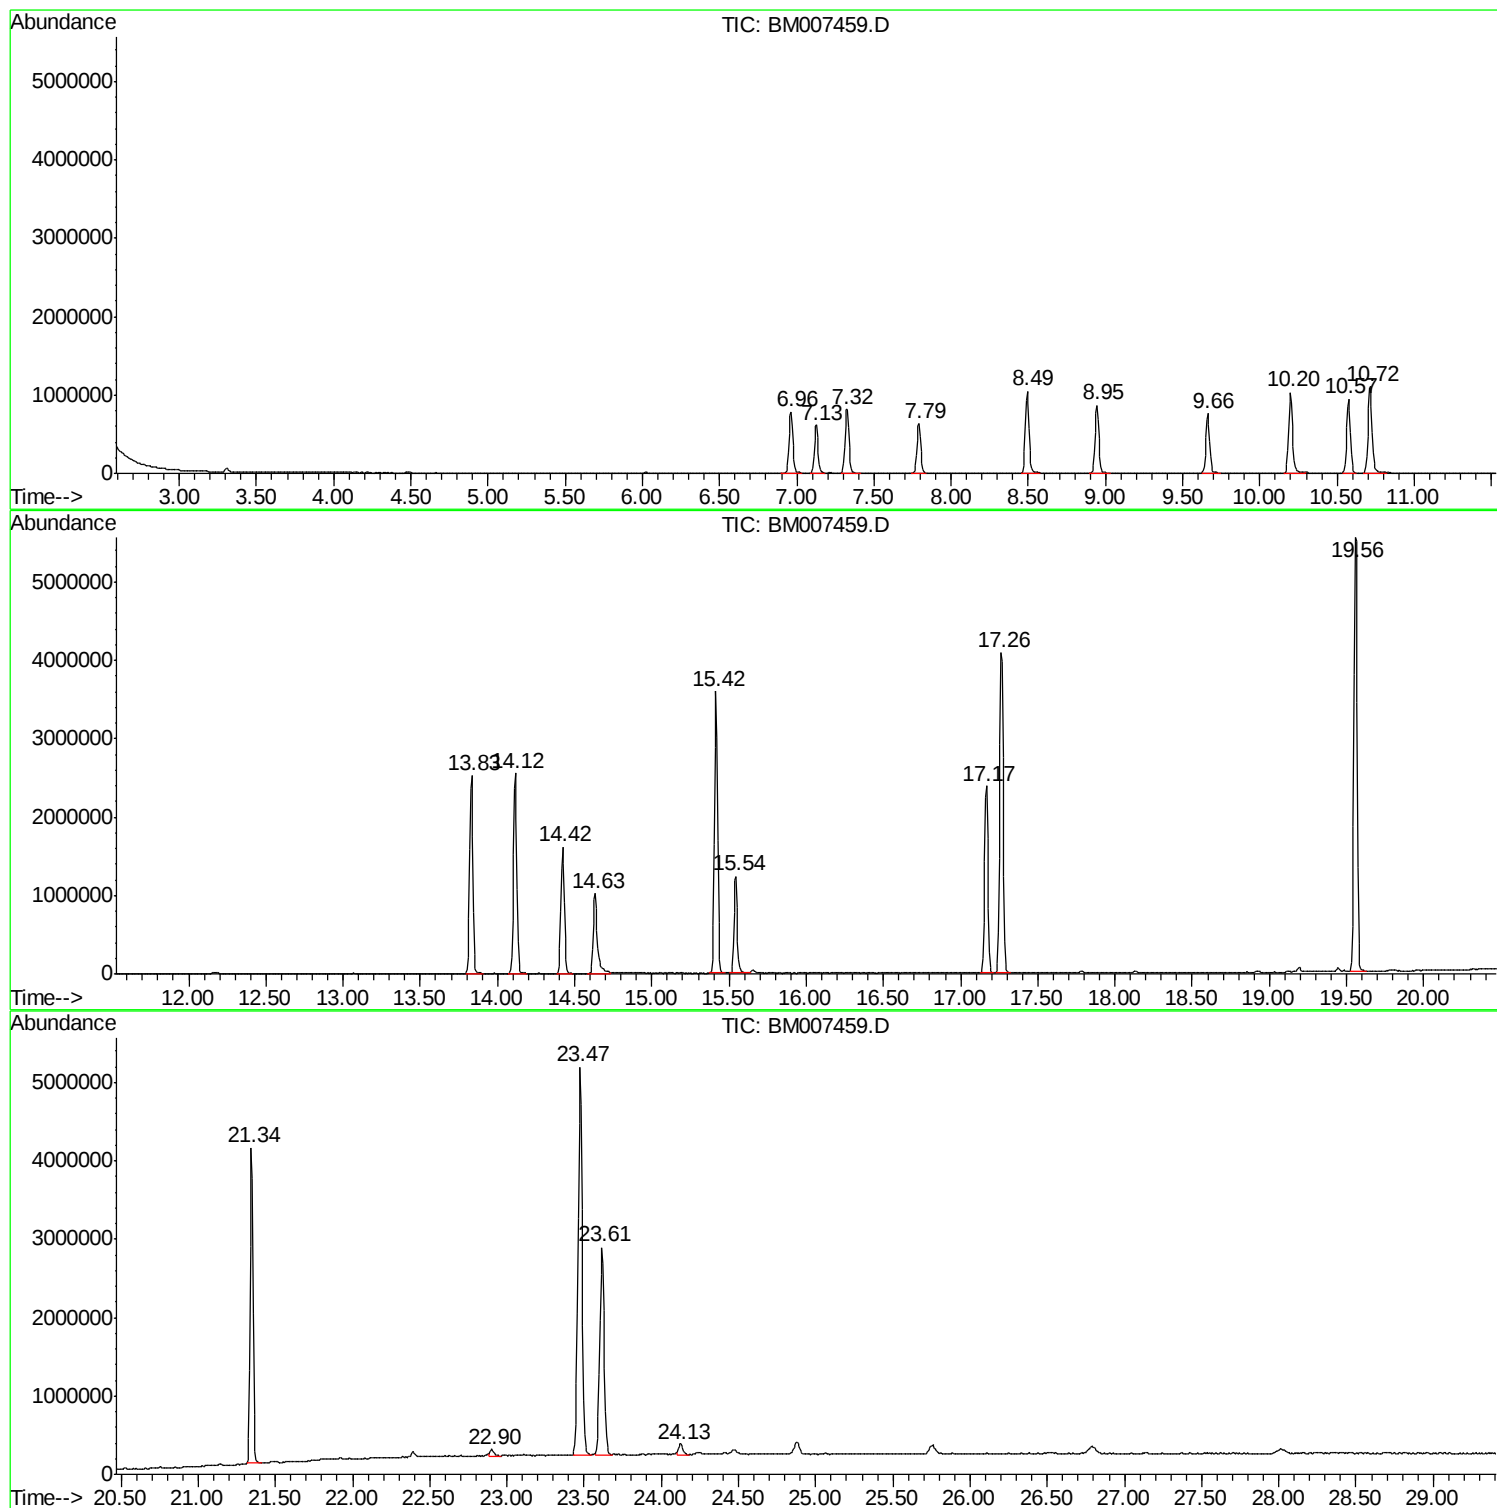

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090816\
Data File : BM007459.D
Acq On : 08 Sep 2016 18:04
Operator : UM/SJ
Sample : PB93299BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK99

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090816\
Data File : BM007459.D
Acq On : 08 Sep 2016 18:04
Operator : UM/SJ
Sample : PB93299BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK99

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc