

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
 Data File : BM027353.D
 Acq On : 08 Sep 2020 11:50
 Operator : JU/CG
 Sample : L3891-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW289

Quant Time: Sep 08 12:21:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 08 10:18:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	103949	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	402329	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	304516	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	732546	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	911009	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	966504	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	14698	6.29	ng/uL	0.00
5) Phenol-d5	6.76	99	50006	5.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	162536	28.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	152976	24.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	97760	13.99	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	92221	30.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	105778	31.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	195770	27.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	27713	3.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	829585	34.24	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	922473	33.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	17552	4.11	ng/ul	0.00
58) Fluorene-d10	15.21	176	732825	33.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	137224	29.27	ng/ul	0.00
71) Anthracene-d10	17.06	188	1311786	37.87	ng/ul	0.00
79) Pyrene-d10	19.36	212	1637248	40.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	1874990	36.17	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	100990	3.955	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
Data File : BM027353.D
Acq On : 08 Sep 2020 11:50
Operator : JU/CG
Sample : L3891-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW289

Quant Time: Sep 08 12:21:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 08 10:18:28 2020
Response via : Initial Calibration

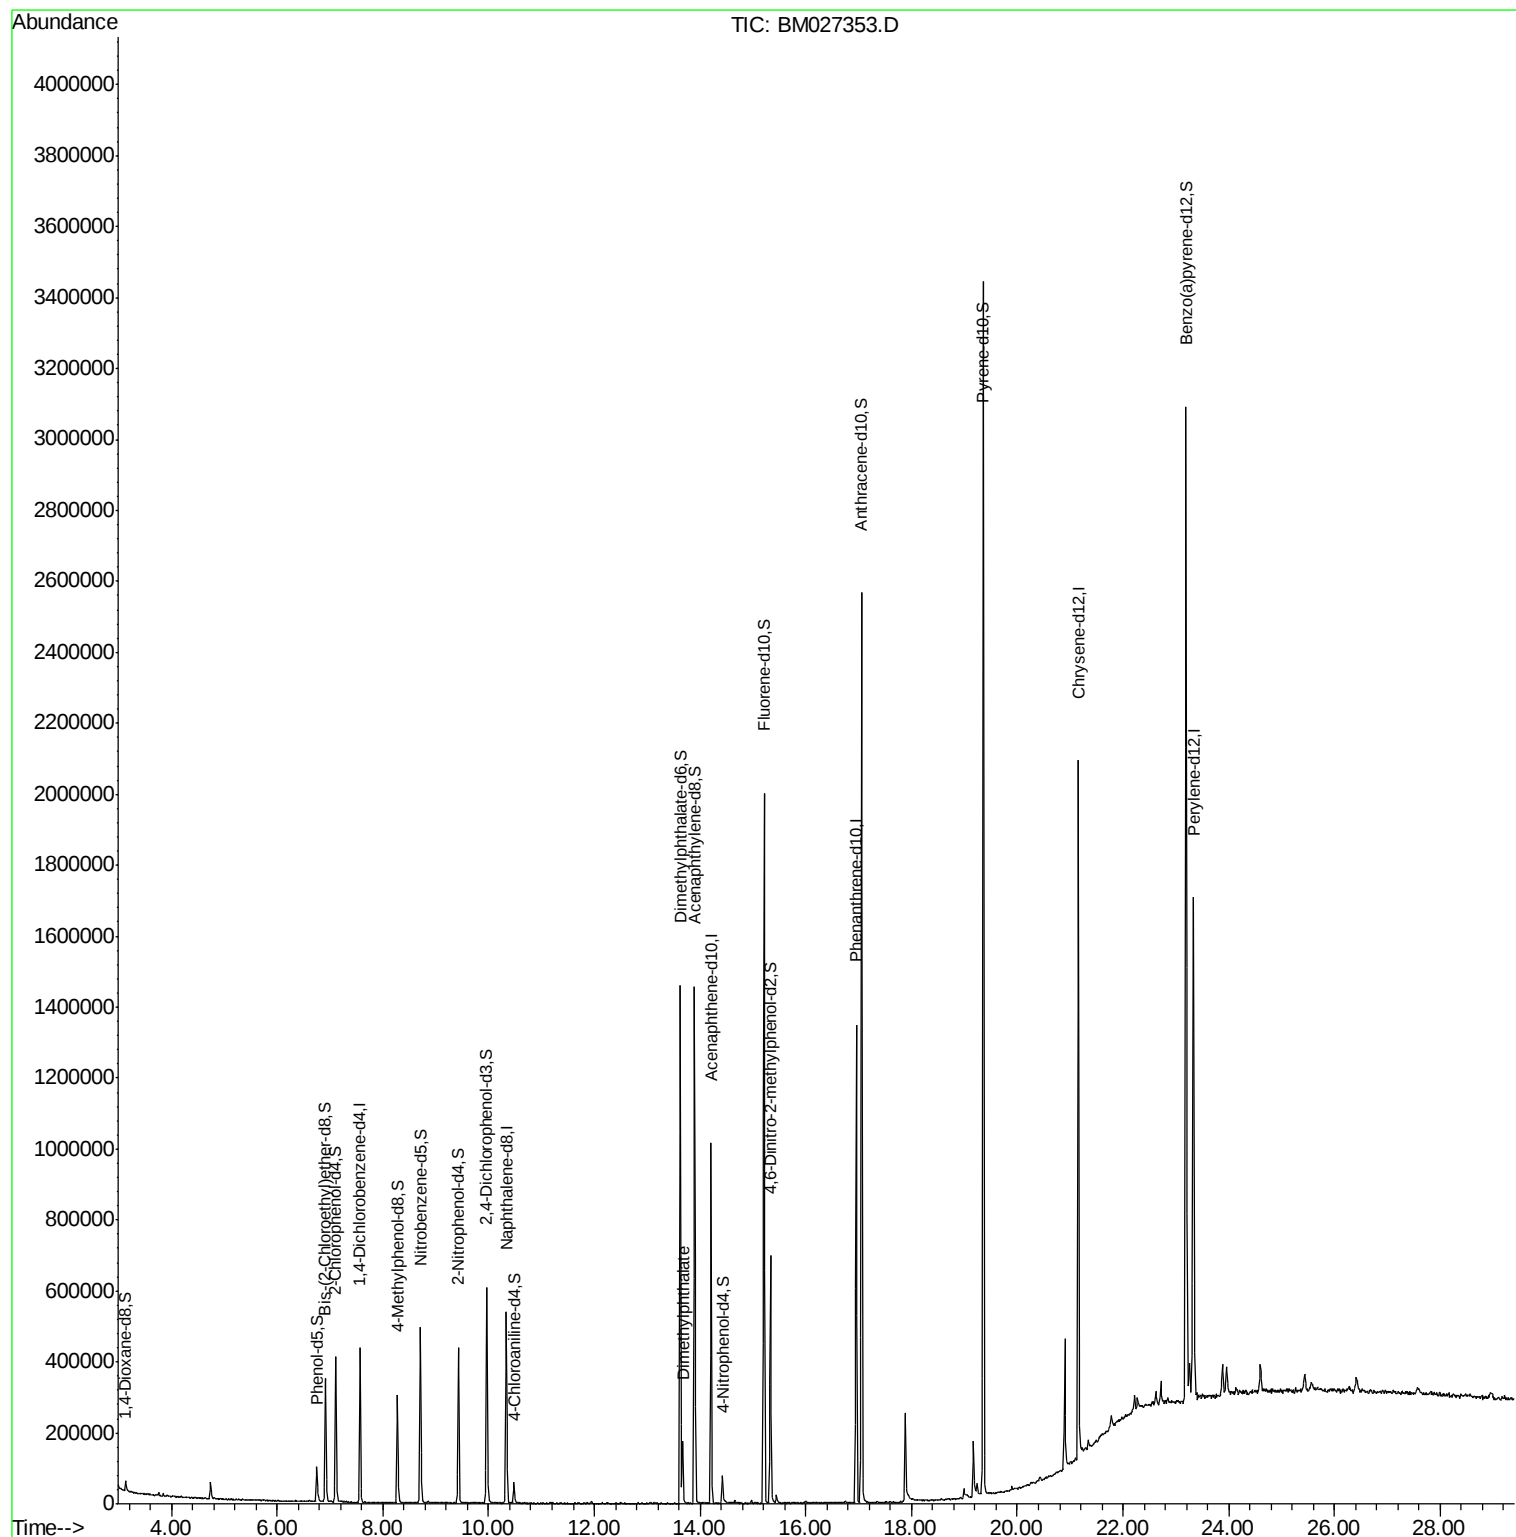

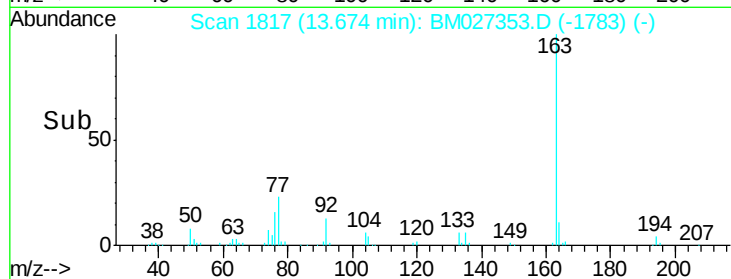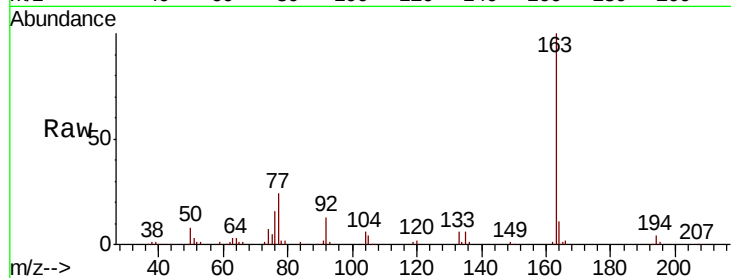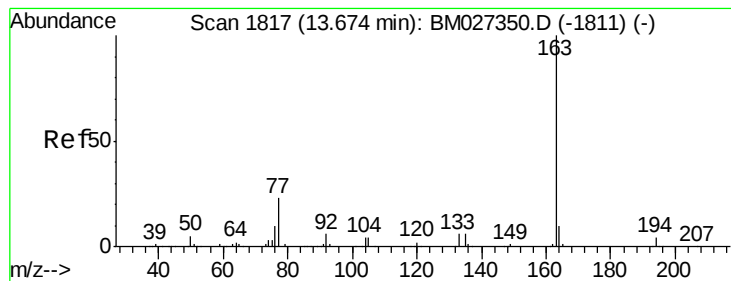

#45
 Dimethylphthalate
 Concen: 3.955 ng/ul
 RT: 13.67 min Scan# 1817
 Delta R.T. 0.00 min
 Lab File: BM027353.D
 Acq: 08 Sep 2020 11:50

Instrument :
 BNA_M
 ClientSampleId :
 EW289

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.3	4.9
164	10.5	8.1	12.1

