

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
 Data File : BM027359.D
 Acq On : 08 Sep 2020 15:28
 Operator : JU/CG
 Sample : L3891-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW290

Quant Time: Sep 08 16:00:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 08 10:18:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	101149	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	399350	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	302323	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	736136	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	940460	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	974305	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	15957	7.02	ng/uL	0.00
5) Phenol-d5	6.75	99	71458	8.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	177088	31.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	177066	29.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	129304	19.02	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	104890	34.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	117931	35.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	229424	32.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	37038	4.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	920609	38.27	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	995293	36.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	32002	7.55	ng/ul	0.00
58) Fluorene-d10	15.21	176	805483	37.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	162313	34.45	ng/ul	0.00
71) Anthracene-d10	17.06	188	1432587	41.15	ng/ul	0.00
79) Pyrene-d10	19.36	212	1863267	44.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2148776	41.12	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	93309	3.681	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
Data File : BM027359.D
Acq On : 08 Sep 2020 15:28
Operator : JU/CG
Sample : L3891-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW290

Quant Time: Sep 08 16:00:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 08 10:18:28 2020
Response via : Initial Calibration

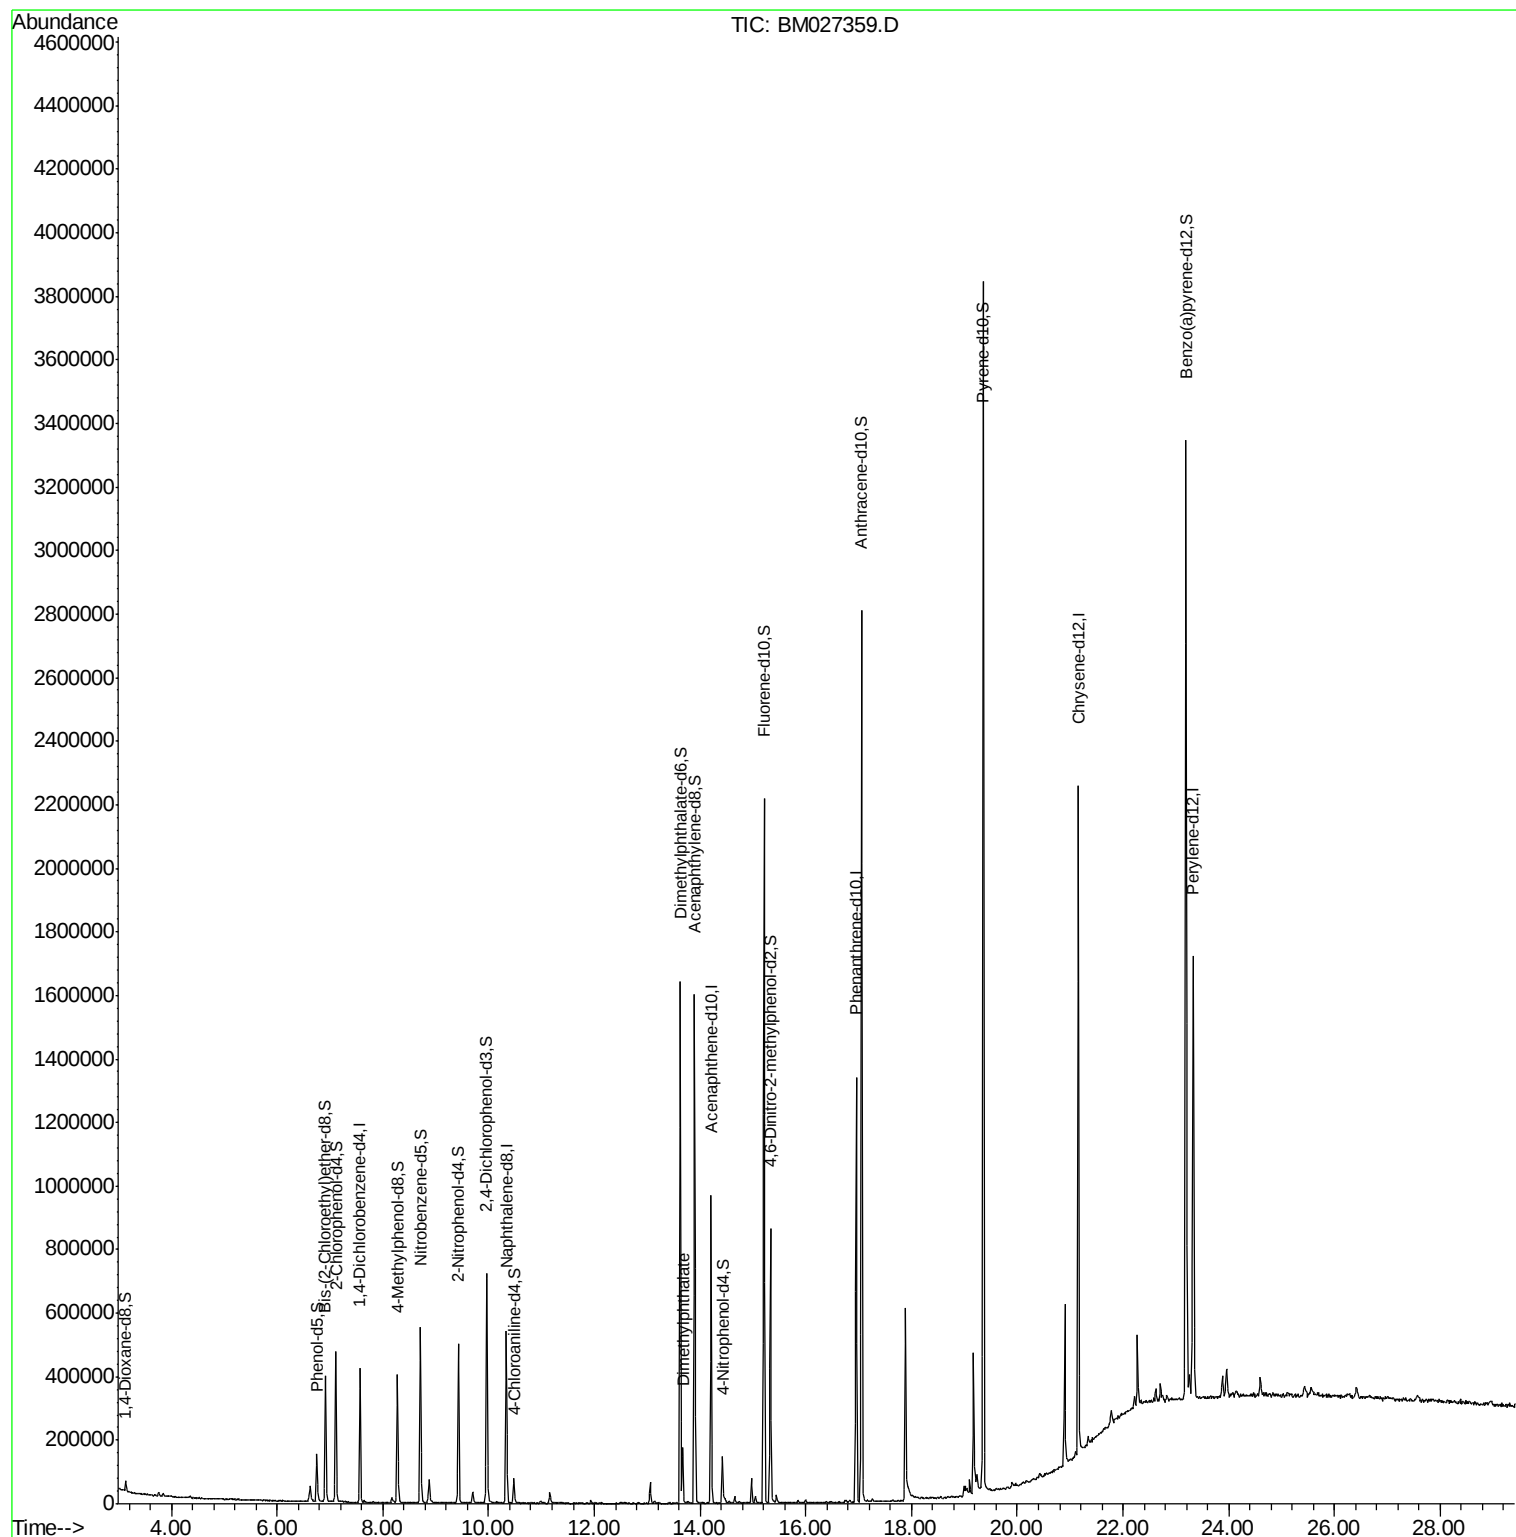


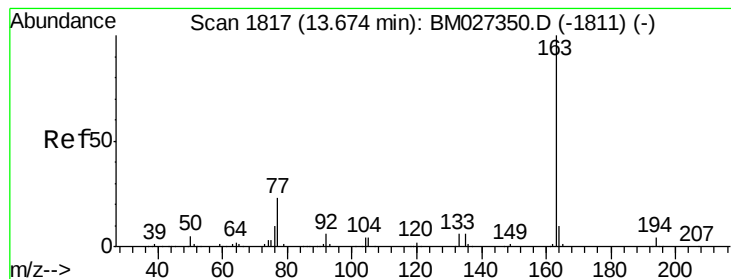

#45
 Dimethylphthalate
 Concen: 3.681 ng/ul
 RT: 13.67 min Scan# 1817
 Delta R.T. 0.00 min
 Lab File: BM027359.D
 Acq: 08 Sep 2020 15:28

Instrument :
 BNA_M
 ClientSampleId :
 EW290

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.3	4.9
164	10.9	8.1	12.1

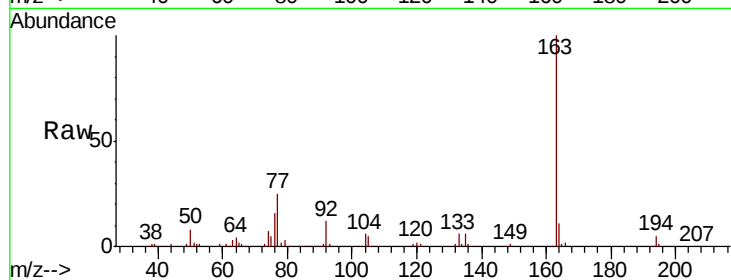

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

