

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
 Data File : BM027360.D
 Acq On : 08 Sep 2020 16:05
 Operator : JU/CG
 Sample : L3891-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW295

Quant Time: Sep 08 16:45:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 08 10:18:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	87993	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	352195	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	274794	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	649059	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	776292	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	822503	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	14919	7.54	ng/uL	0.00
5) Phenol-d5	6.75	99	52001	7.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	158312	32.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	147230	27.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	101173	17.10	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	94283	35.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	107881	37.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	199825	31.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	23228	3.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	910267	41.63	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1009748	40.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	21377	5.55	ng/ul	0.00
58) Fluorene-d10	15.21	176	801734	40.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	157166	37.84	ng/ul	0.00
71) Anthracene-d10	17.06	188	1478099	48.16	ng/ul	0.00
79) Pyrene-d10	19.36	212	1848521	53.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2089491	47.36	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.67	163	144154	6.256	ng/ul# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
Data File : BM027360.D
Acq On : 08 Sep 2020 16:05
Operator : JU/CG
Sample : L3891-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW295

Quant Time: Sep 08 16:45:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 08 10:18:28 2020
Response via : Initial Calibration

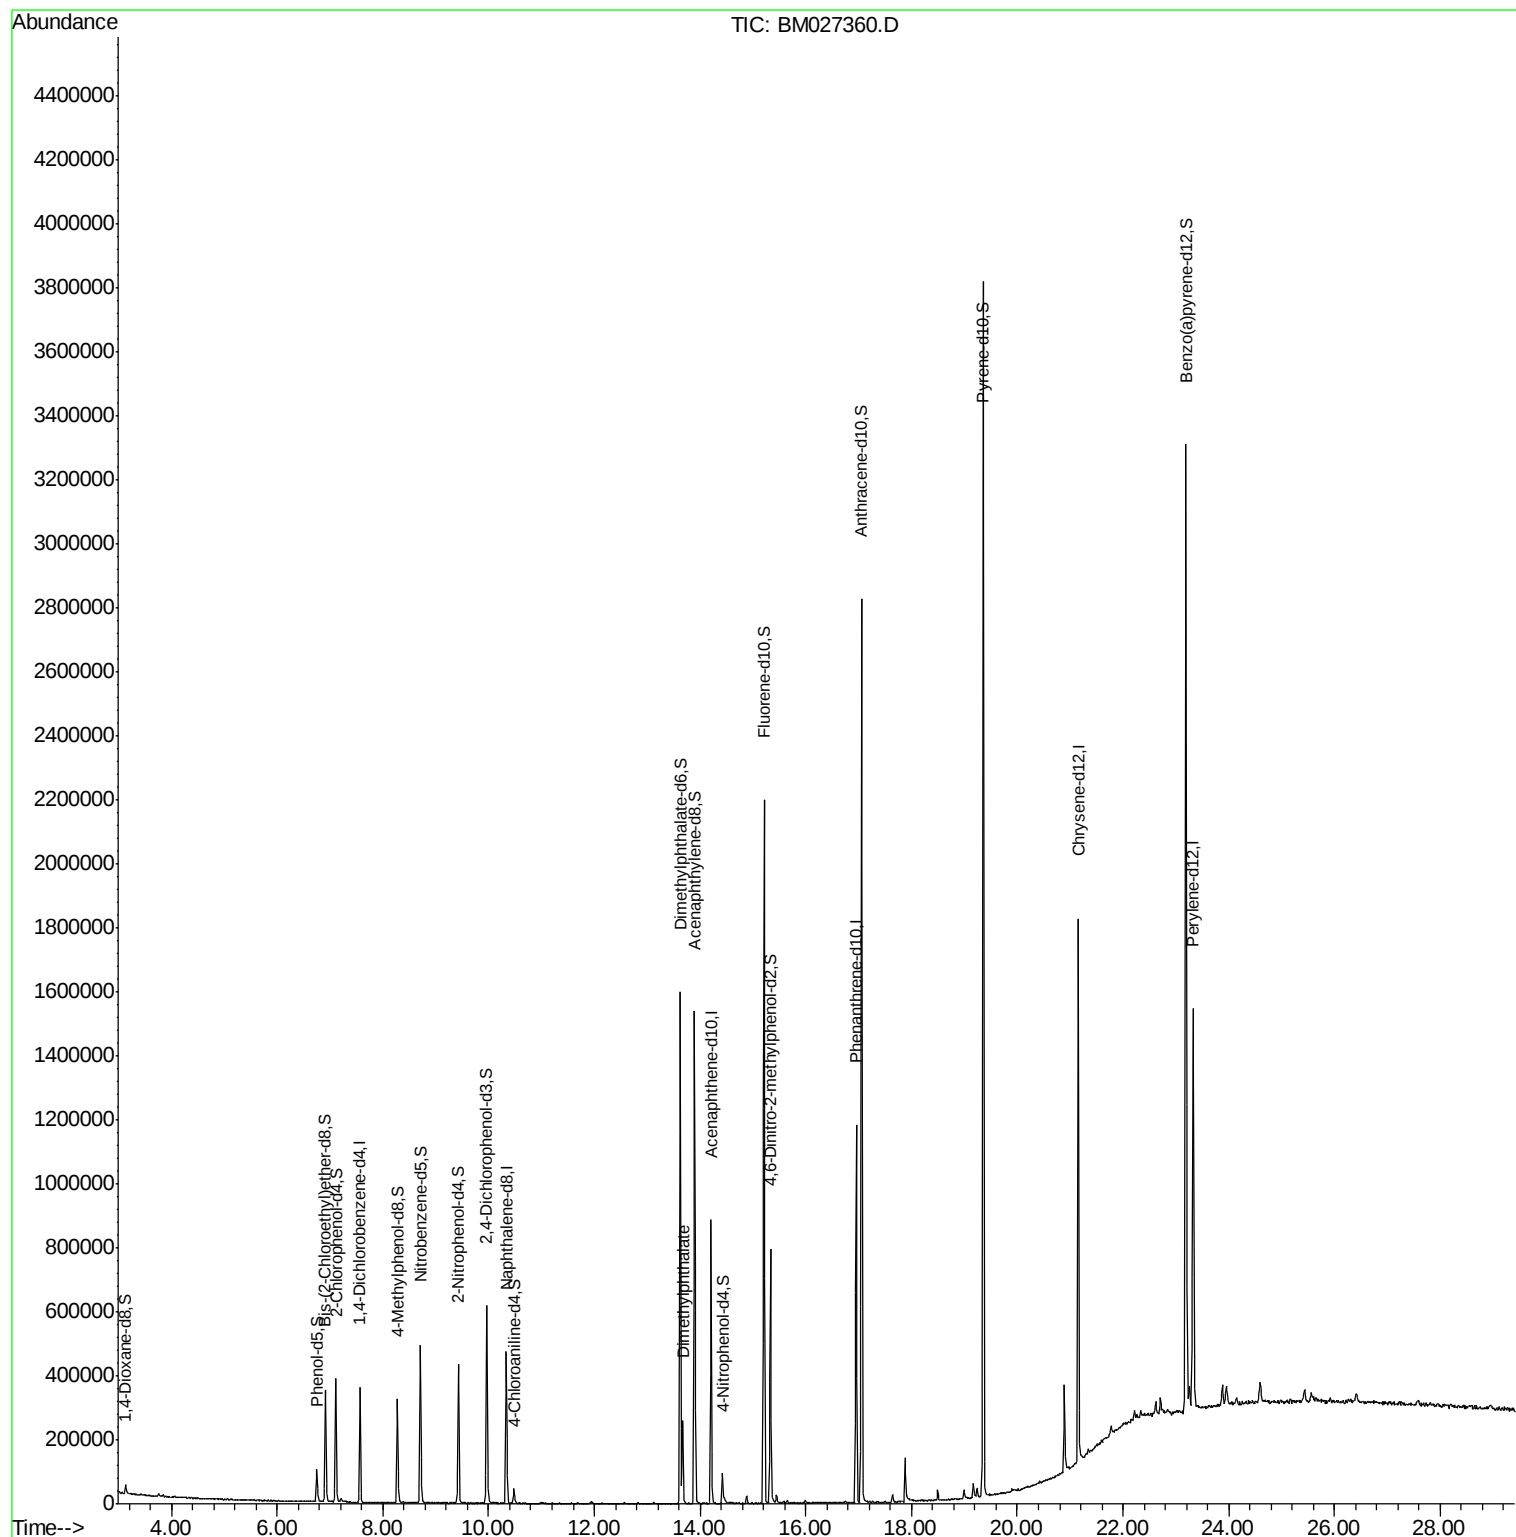

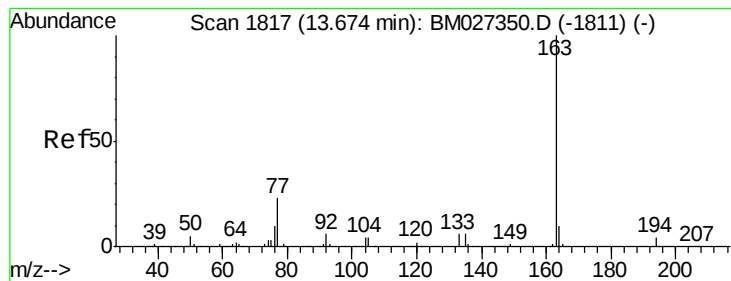

#45

Dimethylphthalate

Concen: 6.256 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. 0.00 min

Lab File: BM027360.D

Acq: 08 Sep 2020 16:05

Instrument :

BNA_M

ClientSampleId :

EW295


Tot Ion:163 Resp: 144154

Ion Ratio Lower Upper

163 100

194 5.0 3.3 4.9#

164 10.1 8.1 12.1

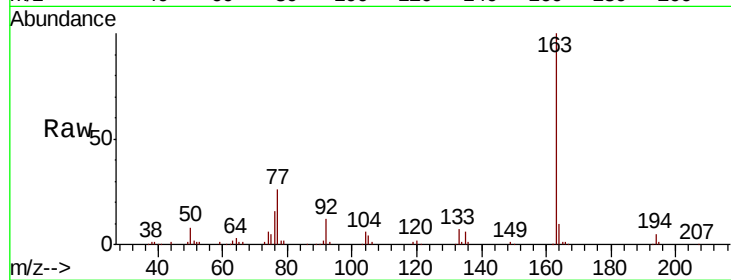

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

