

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
 Data File : BM027361.D
 Acq On : 08 Sep 2020 16:44
 Operator : JU/CG
 Sample : L3891-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW2A0

Quant Time: Sep 08 17:15:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Sep 08 10:18:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	91875	20.00	ng/ul	0.00
18) Naphthalene-d8	10.34	136	359484	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	278609	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	665603	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	800978	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	844899	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	9965	4.83	ng/uL	0.00
5) Phenol-d5	6.76	99	35469	4.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	107547	21.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	99544	17.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	68147	11.03	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	62070	22.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	69813	23.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	133929	20.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	15405	2.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	576432	26.00	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	638149	25.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	10048	2.57	ng/ul	0.00
58) Fluorene-d10	15.21	176	510013	25.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	92593	21.74	ng/ul	0.00
71) Anthracene-d10	17.06	188	958902	30.46	ng/ul	0.00
79) Pyrene-d10	19.36	212	1187675	33.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1332586	29.40	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	89267	3.821	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM090820\
Data File : BM027361.D
Acq On : 08 Sep 2020 16:44
Operator : JU/CG
Sample : L3891-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW2A0

Quant Time: Sep 08 17:15:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Sep 08 10:18:28 2020
Response via : Initial Calibration

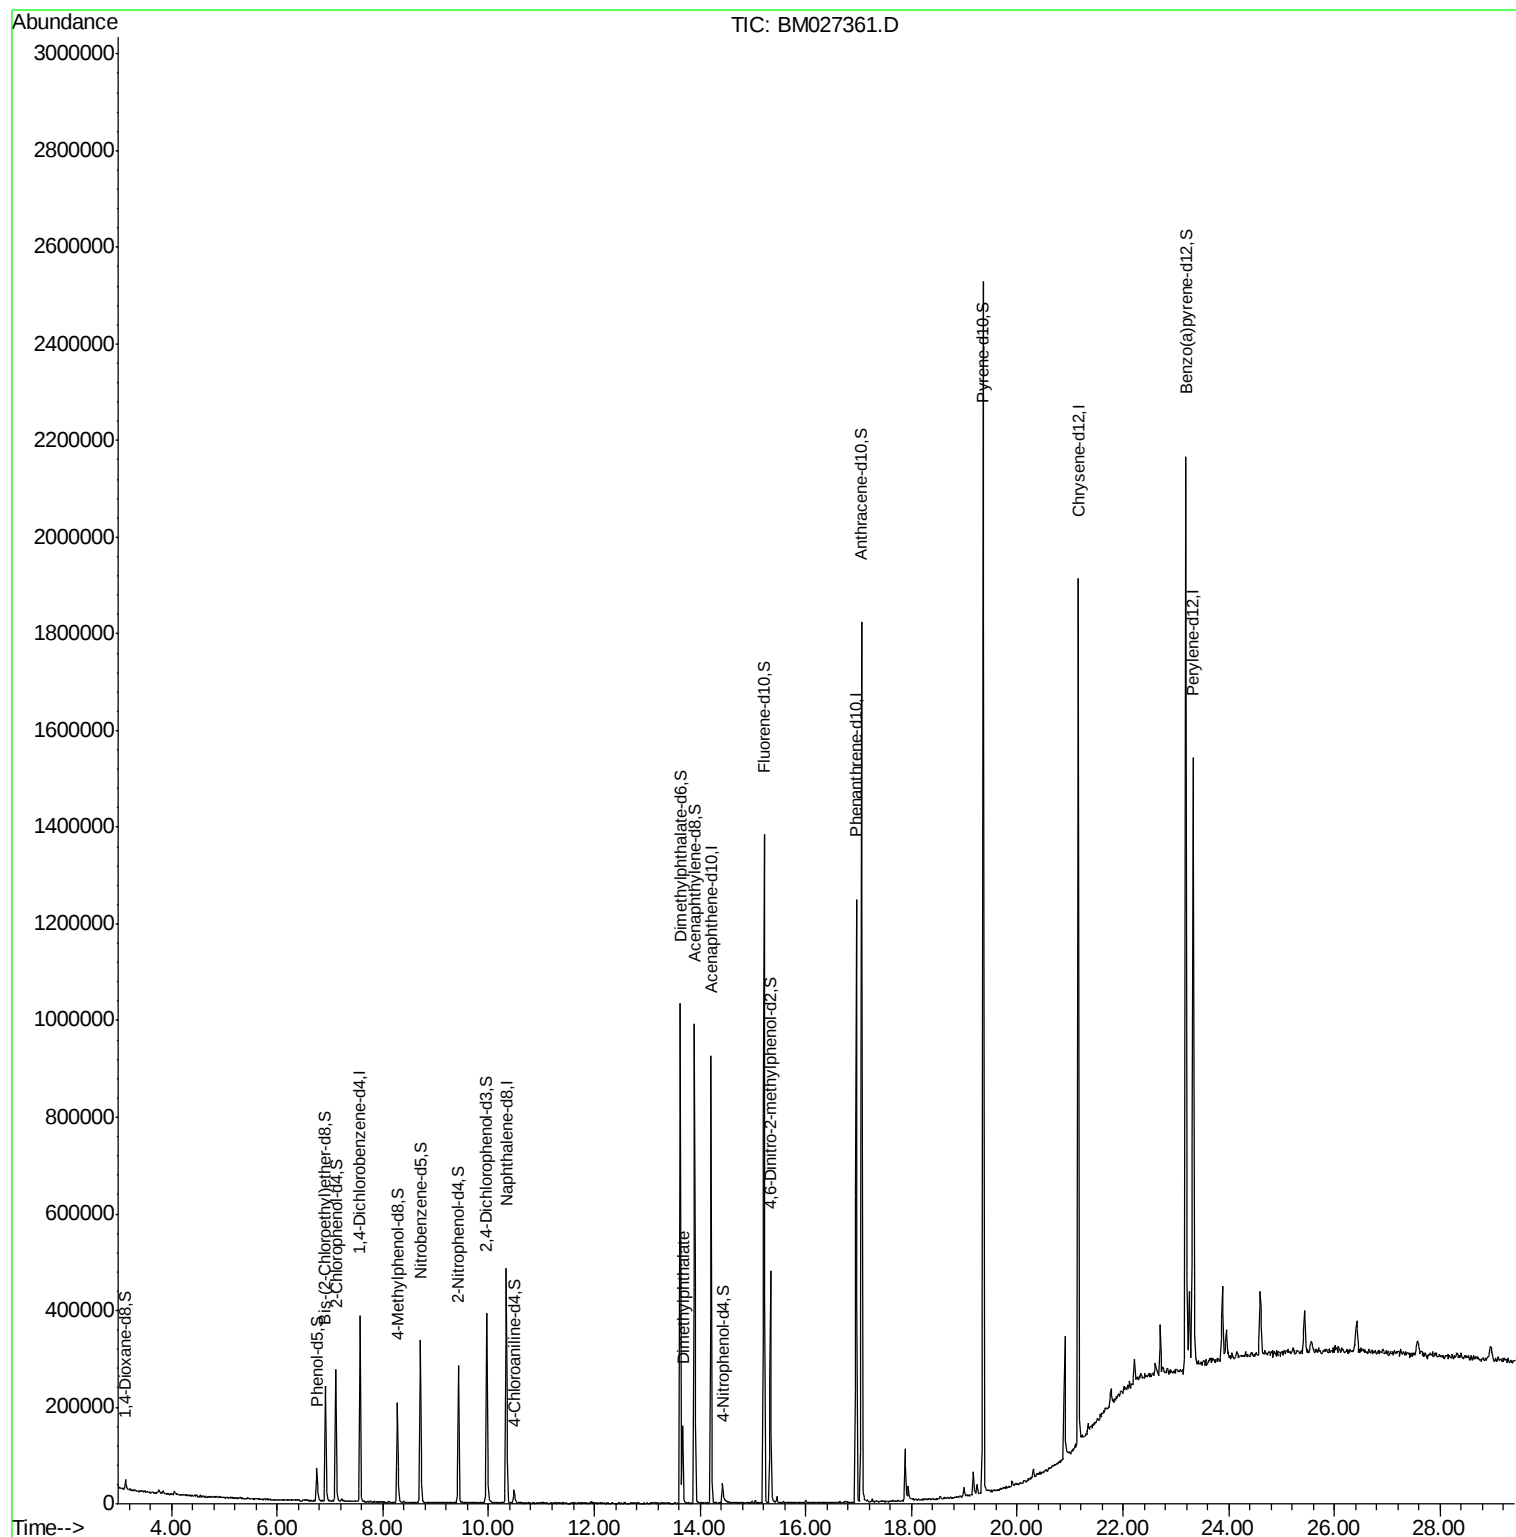

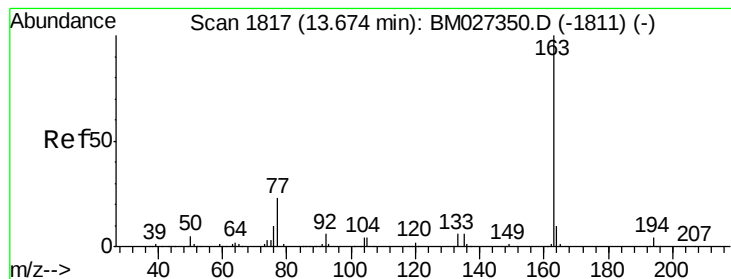

#45

Dimethylphthalate

Concen: 3.821 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. 0.00 min

Lab File: BM027361.D

Acq: 08 Sep 2020 16:44

Instrument :

BNA_M

ClientSampleId :

EW2A0


Tot Ion:163 Resp: 89267

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.1 8.1 12.1

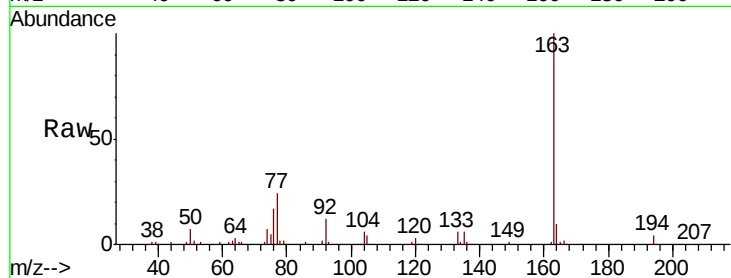

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

