


Benzaldehyde

Response Ratio

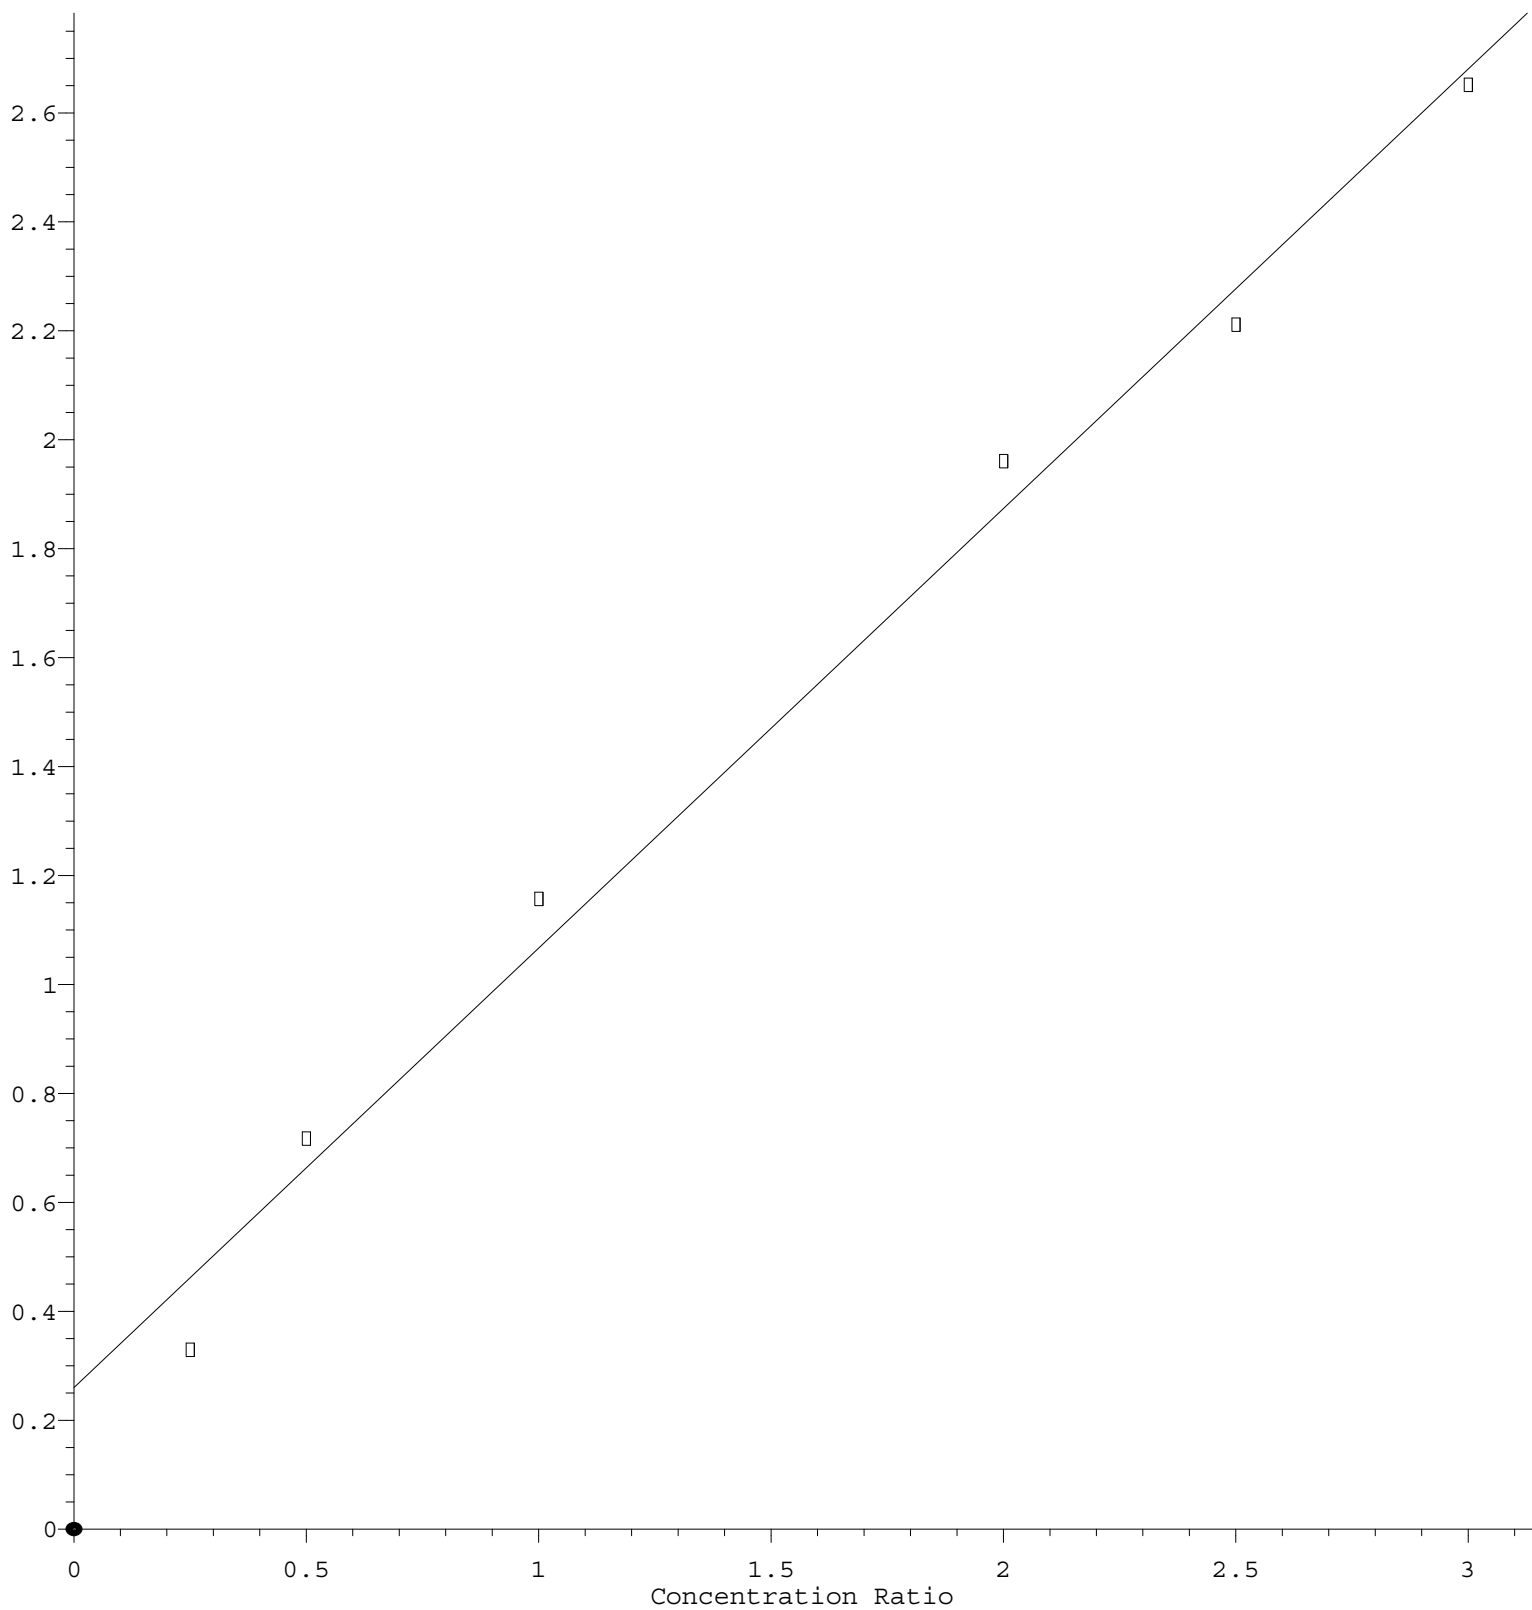

$$\text{Response} = 8.069\text{e-}001 * \text{Amt} + 2.604\text{e-}001$$


Coef of Det (r^2) = 0.990036 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021

Hexachlorocyclopentadiene

Response Ratio

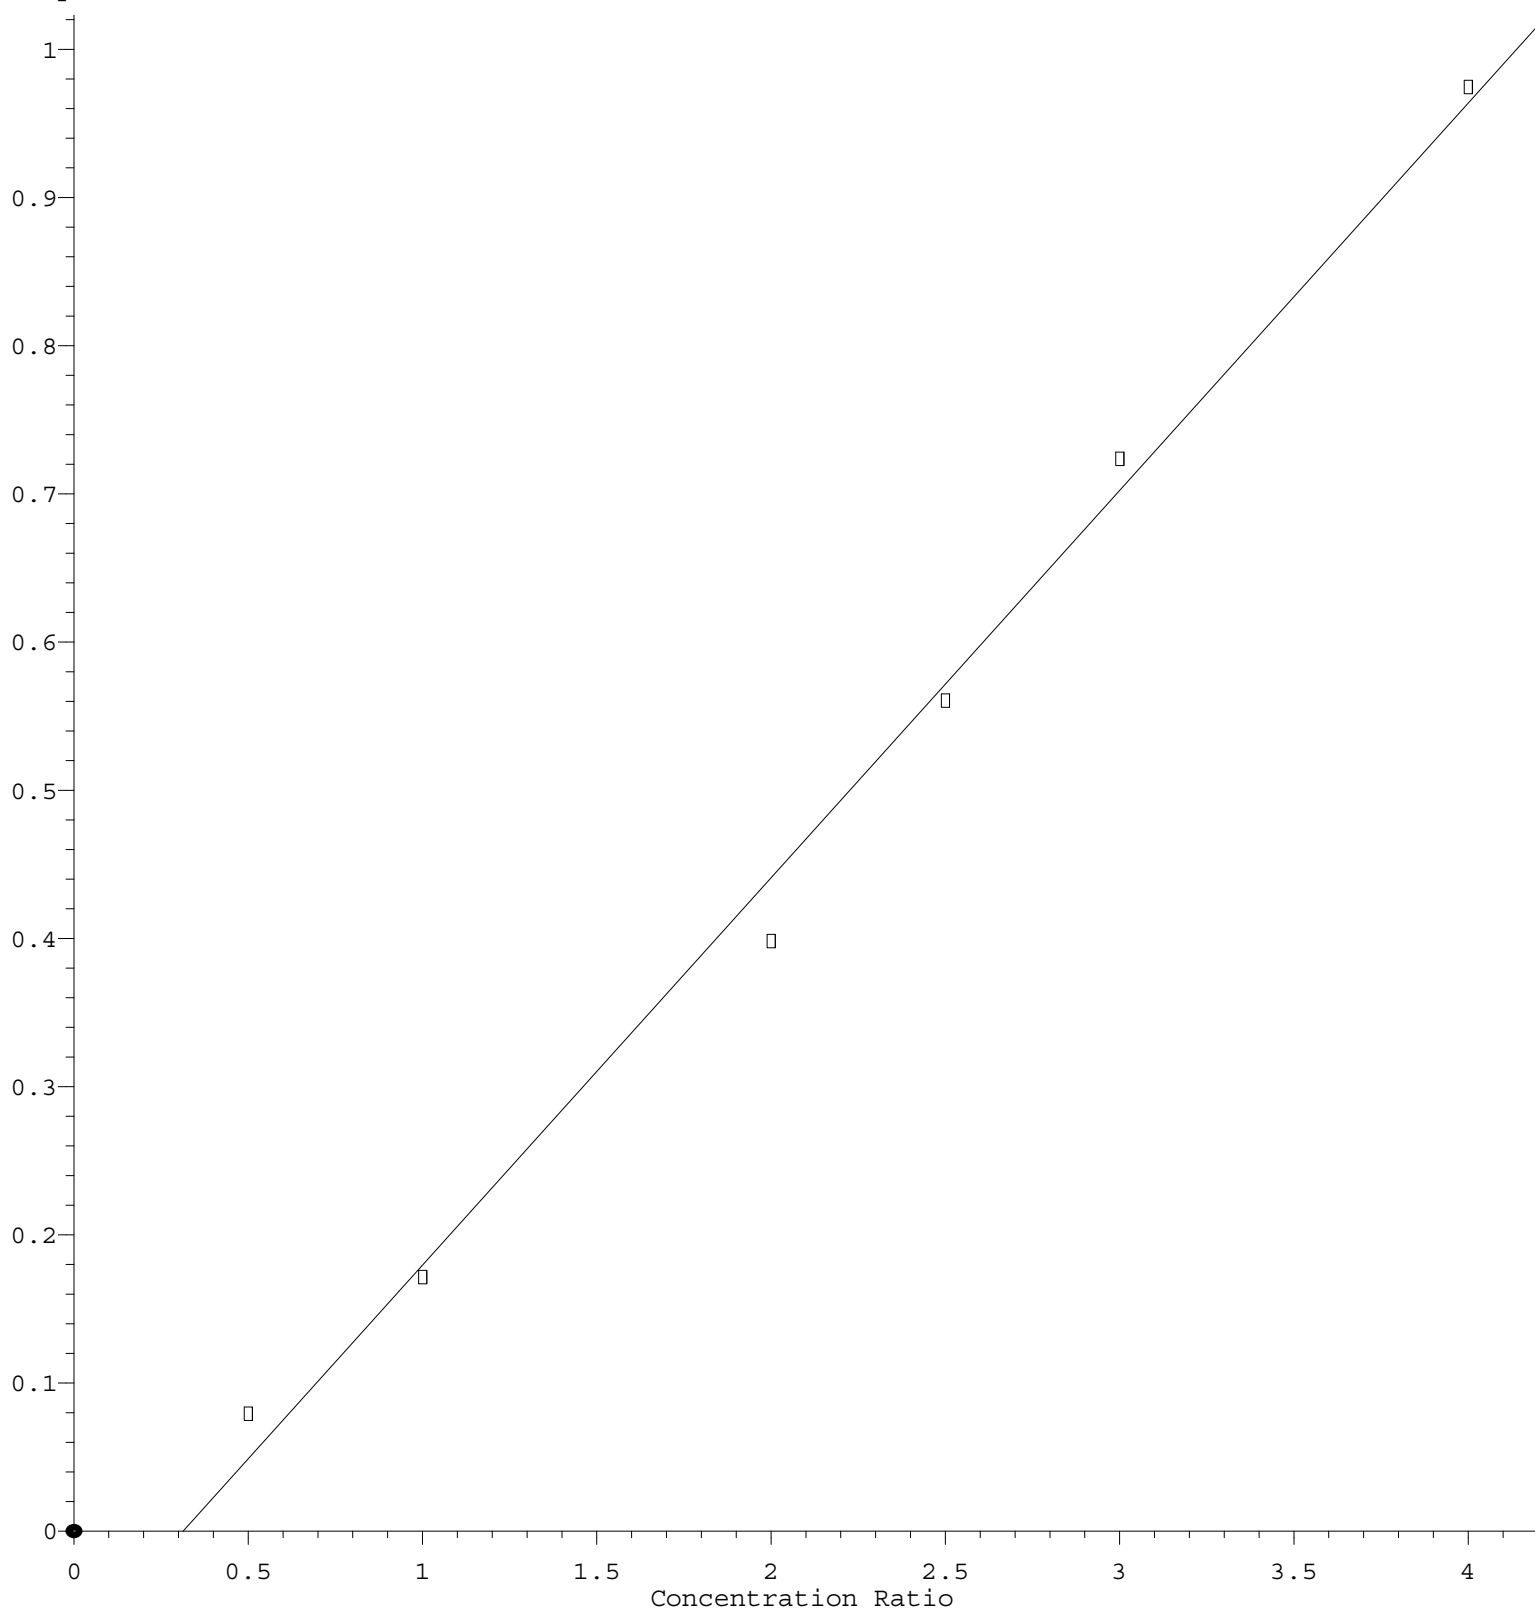

$$\text{Response} = 2.614\text{e-}001 * \text{Amt} - 8.172\text{e-}002$$


Coef of Det (r^2) = 0.993864 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021

2-Nitroaniline

Response Ratio

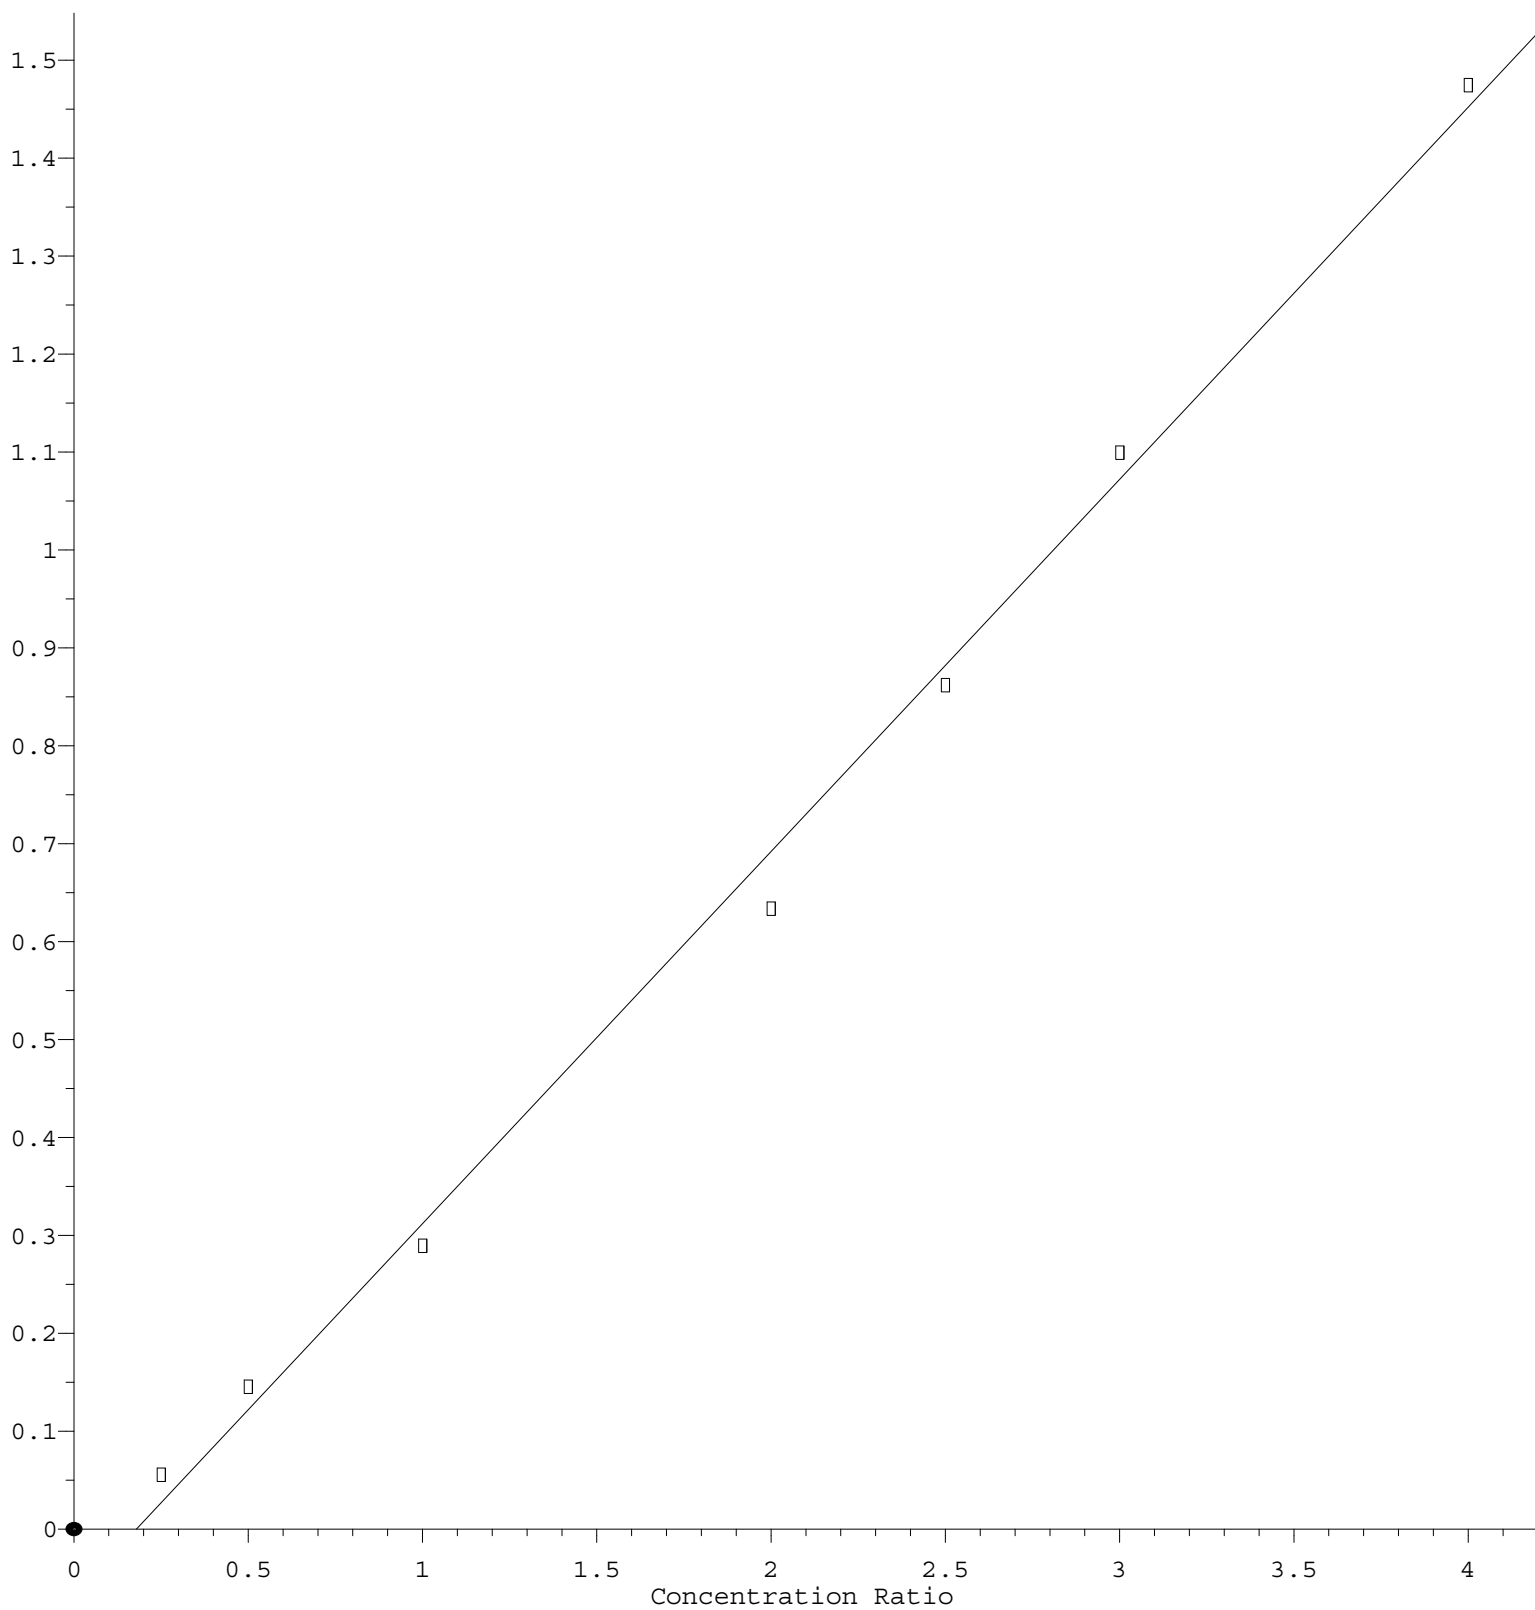


$$\text{Response} = 3.800\text{e-}001 * \text{Amt} - 6.786\text{e-}002$$

Coef of Det (r^2) = 0.995824 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021


2,4-Dinitrophenol

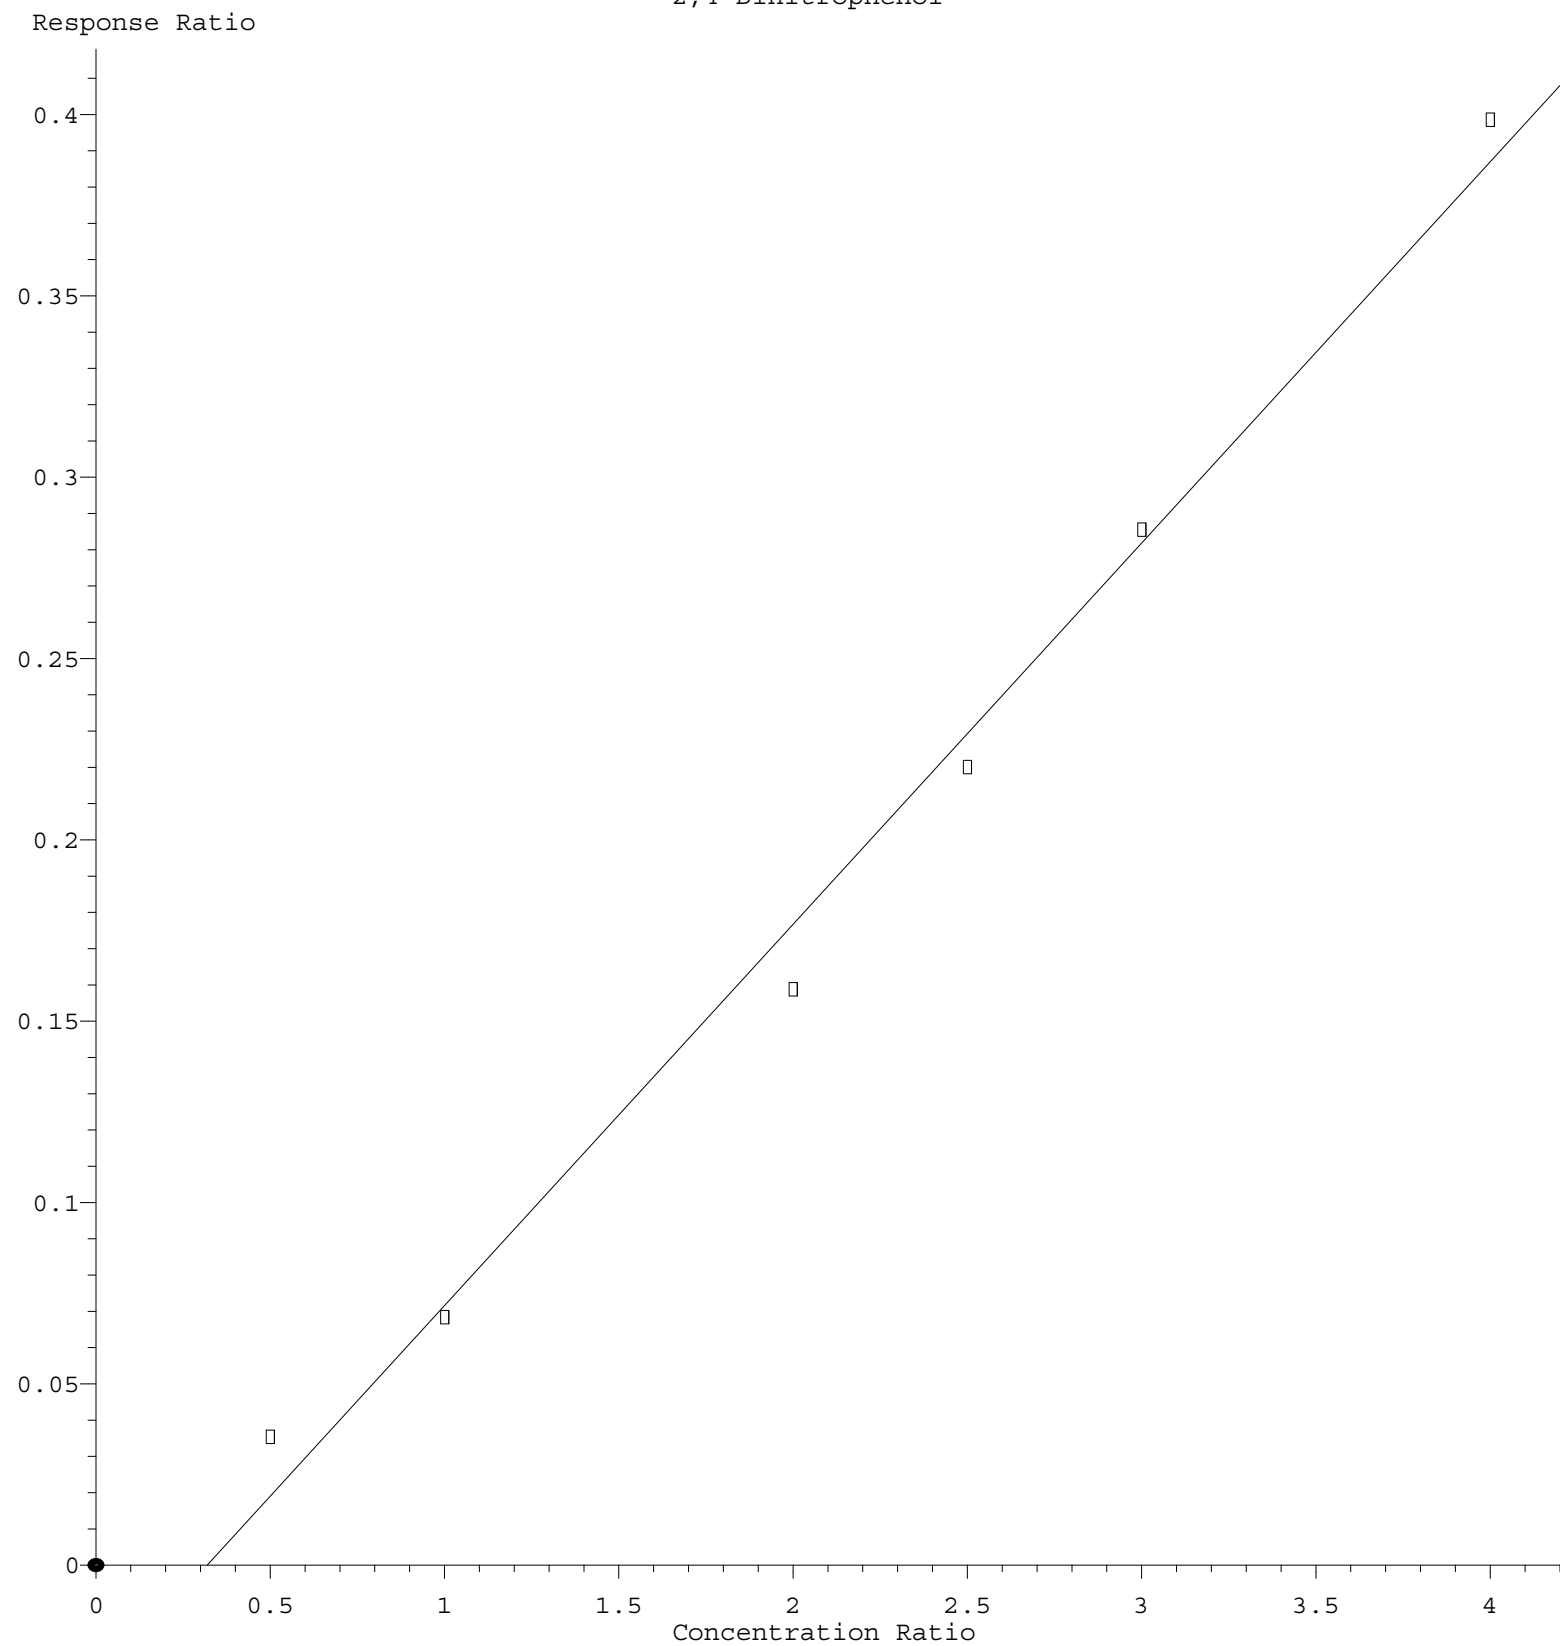

Response = 1.052e-001 * Amt - 3.353e-002
 Coef of Det (r^2) = 0.991060 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M
 Calibration Table Last Updated: Wed Sep 08 19:23:17 2021

2,4-Dinitrotoluene

Response Ratio

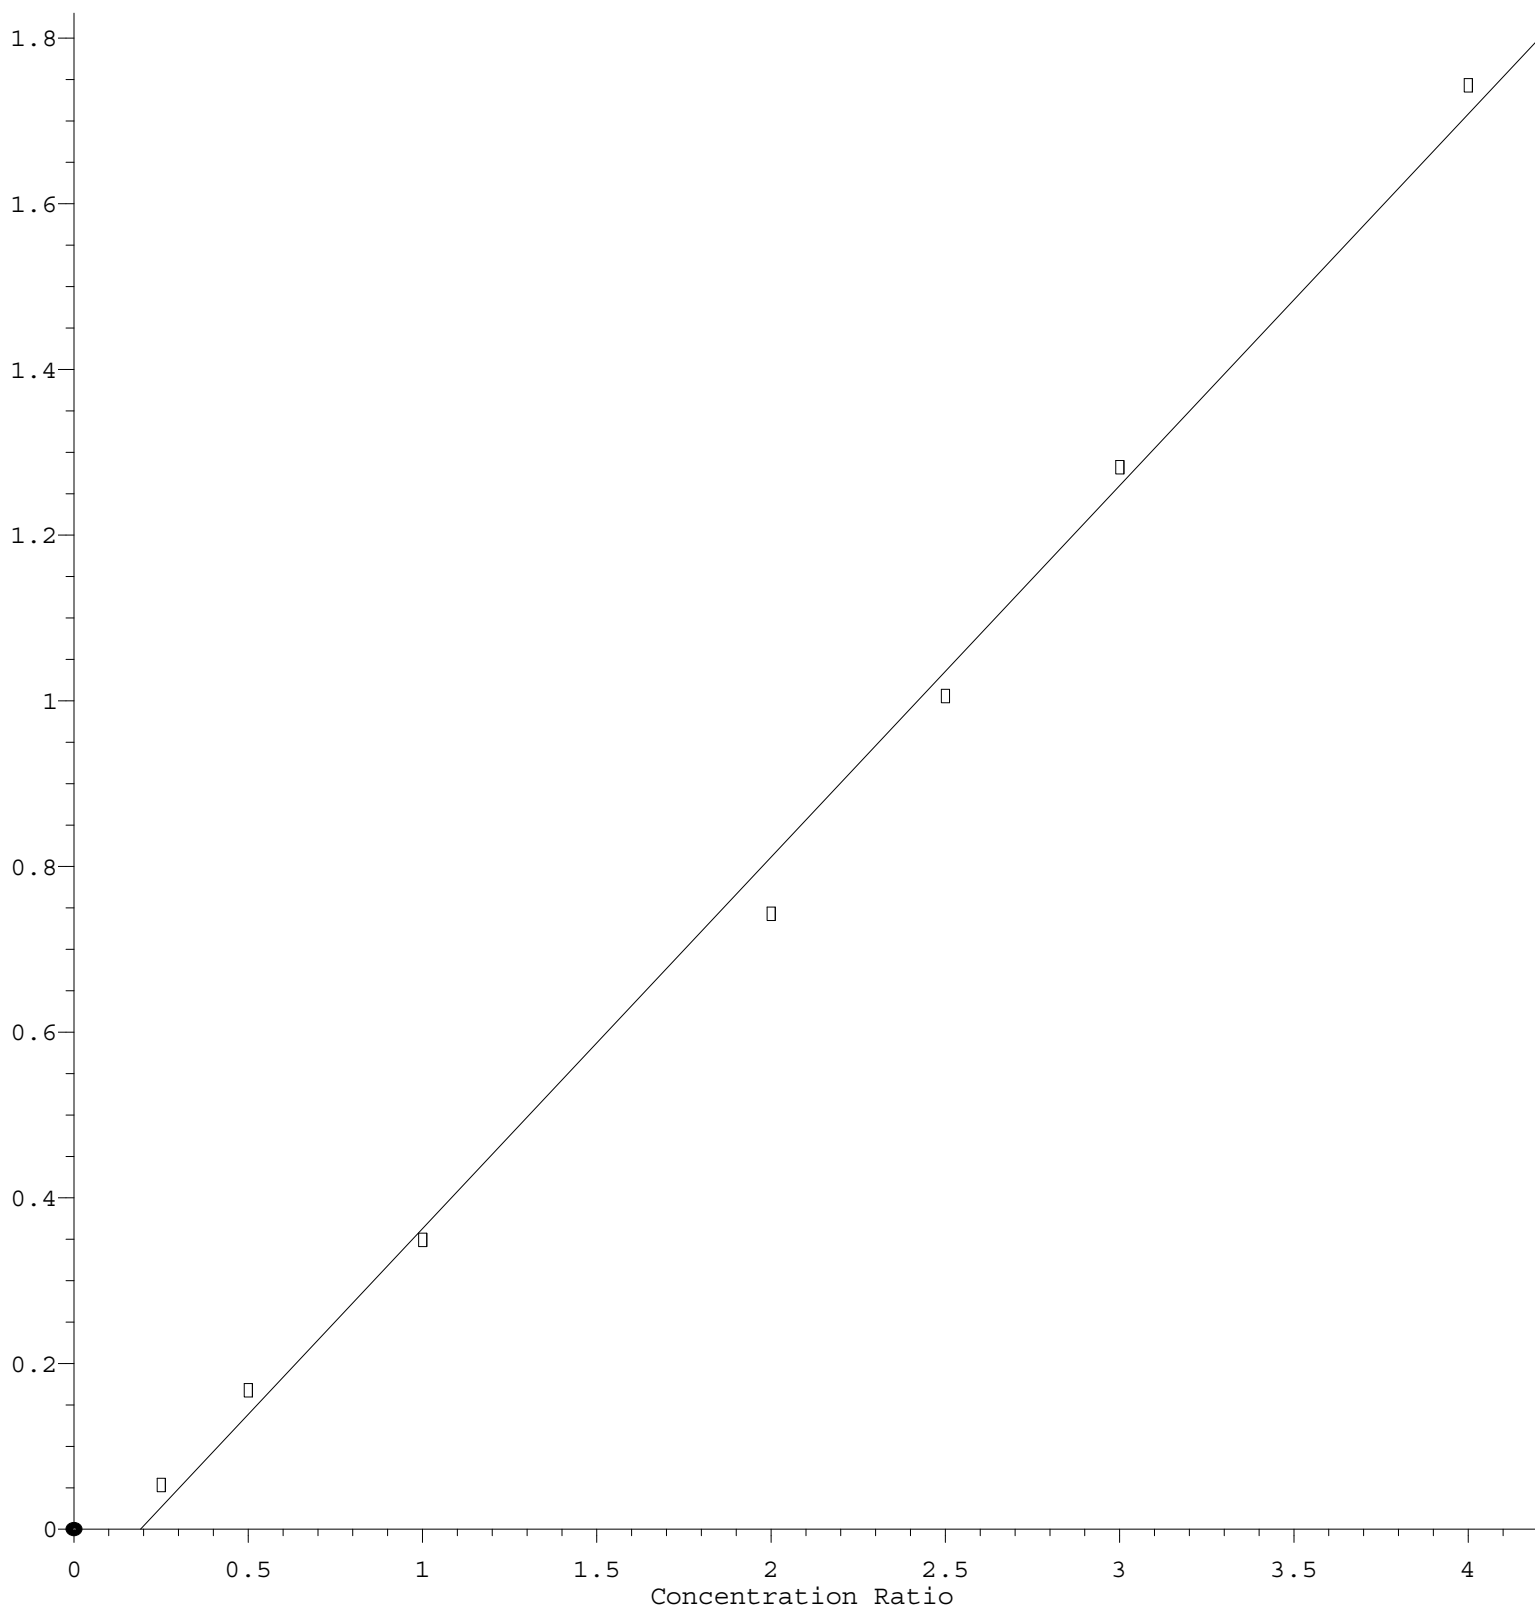

$$\text{Response} = 4.485\text{e-}001 * \text{Amt} - 8.549\text{e-}002$$


Coef of Det (r^2) = 0.996111 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021

4-Nitroaniline

Response Ratio

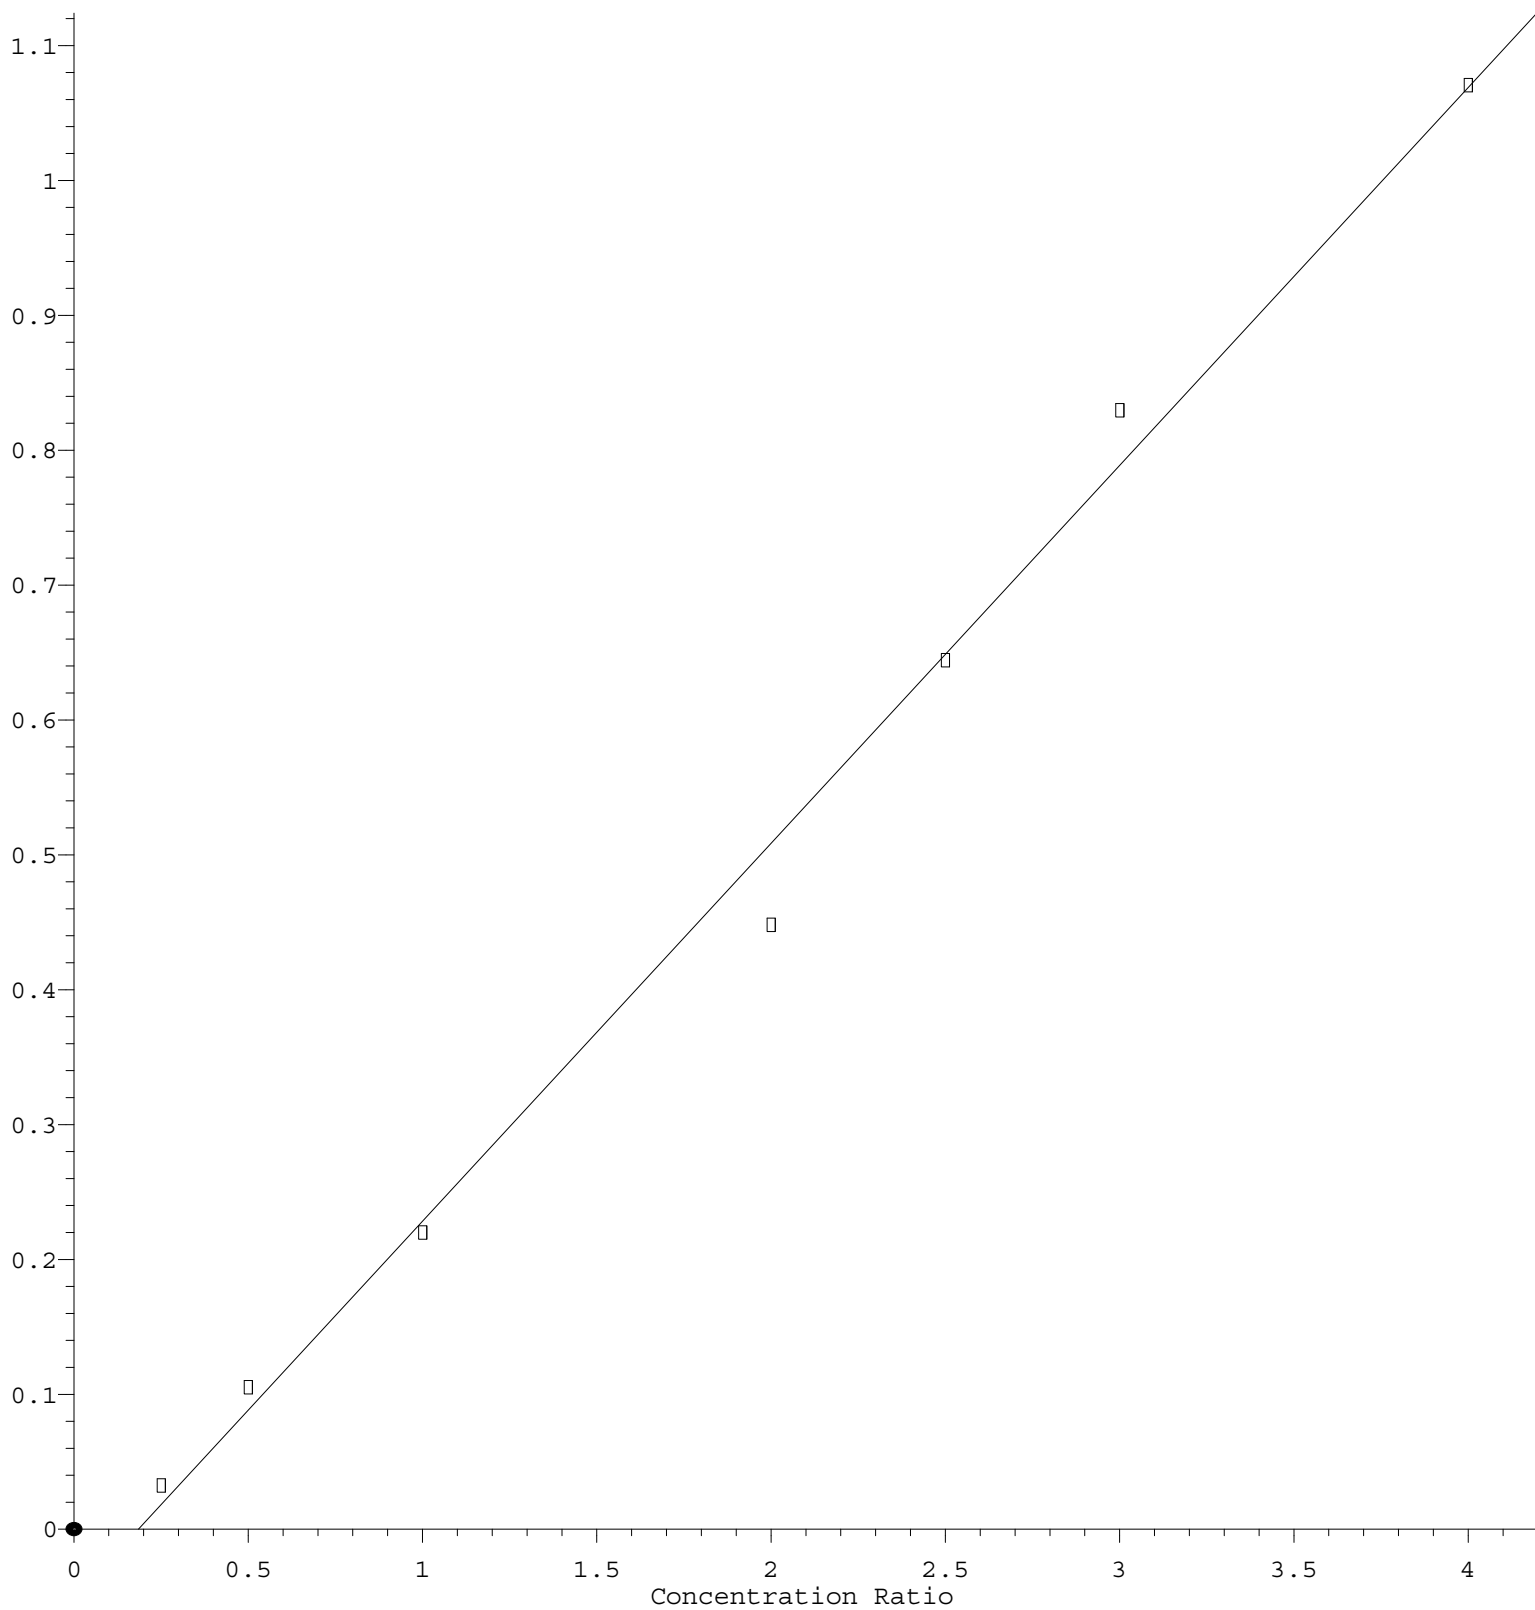

$$\text{Response} = 2.802\text{e-}001 * \text{Amt} - 5.182\text{e-}002$$


Coef of Det (r^2) = 0.993499 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021

Butylbenzylphthalate

Response Ratio

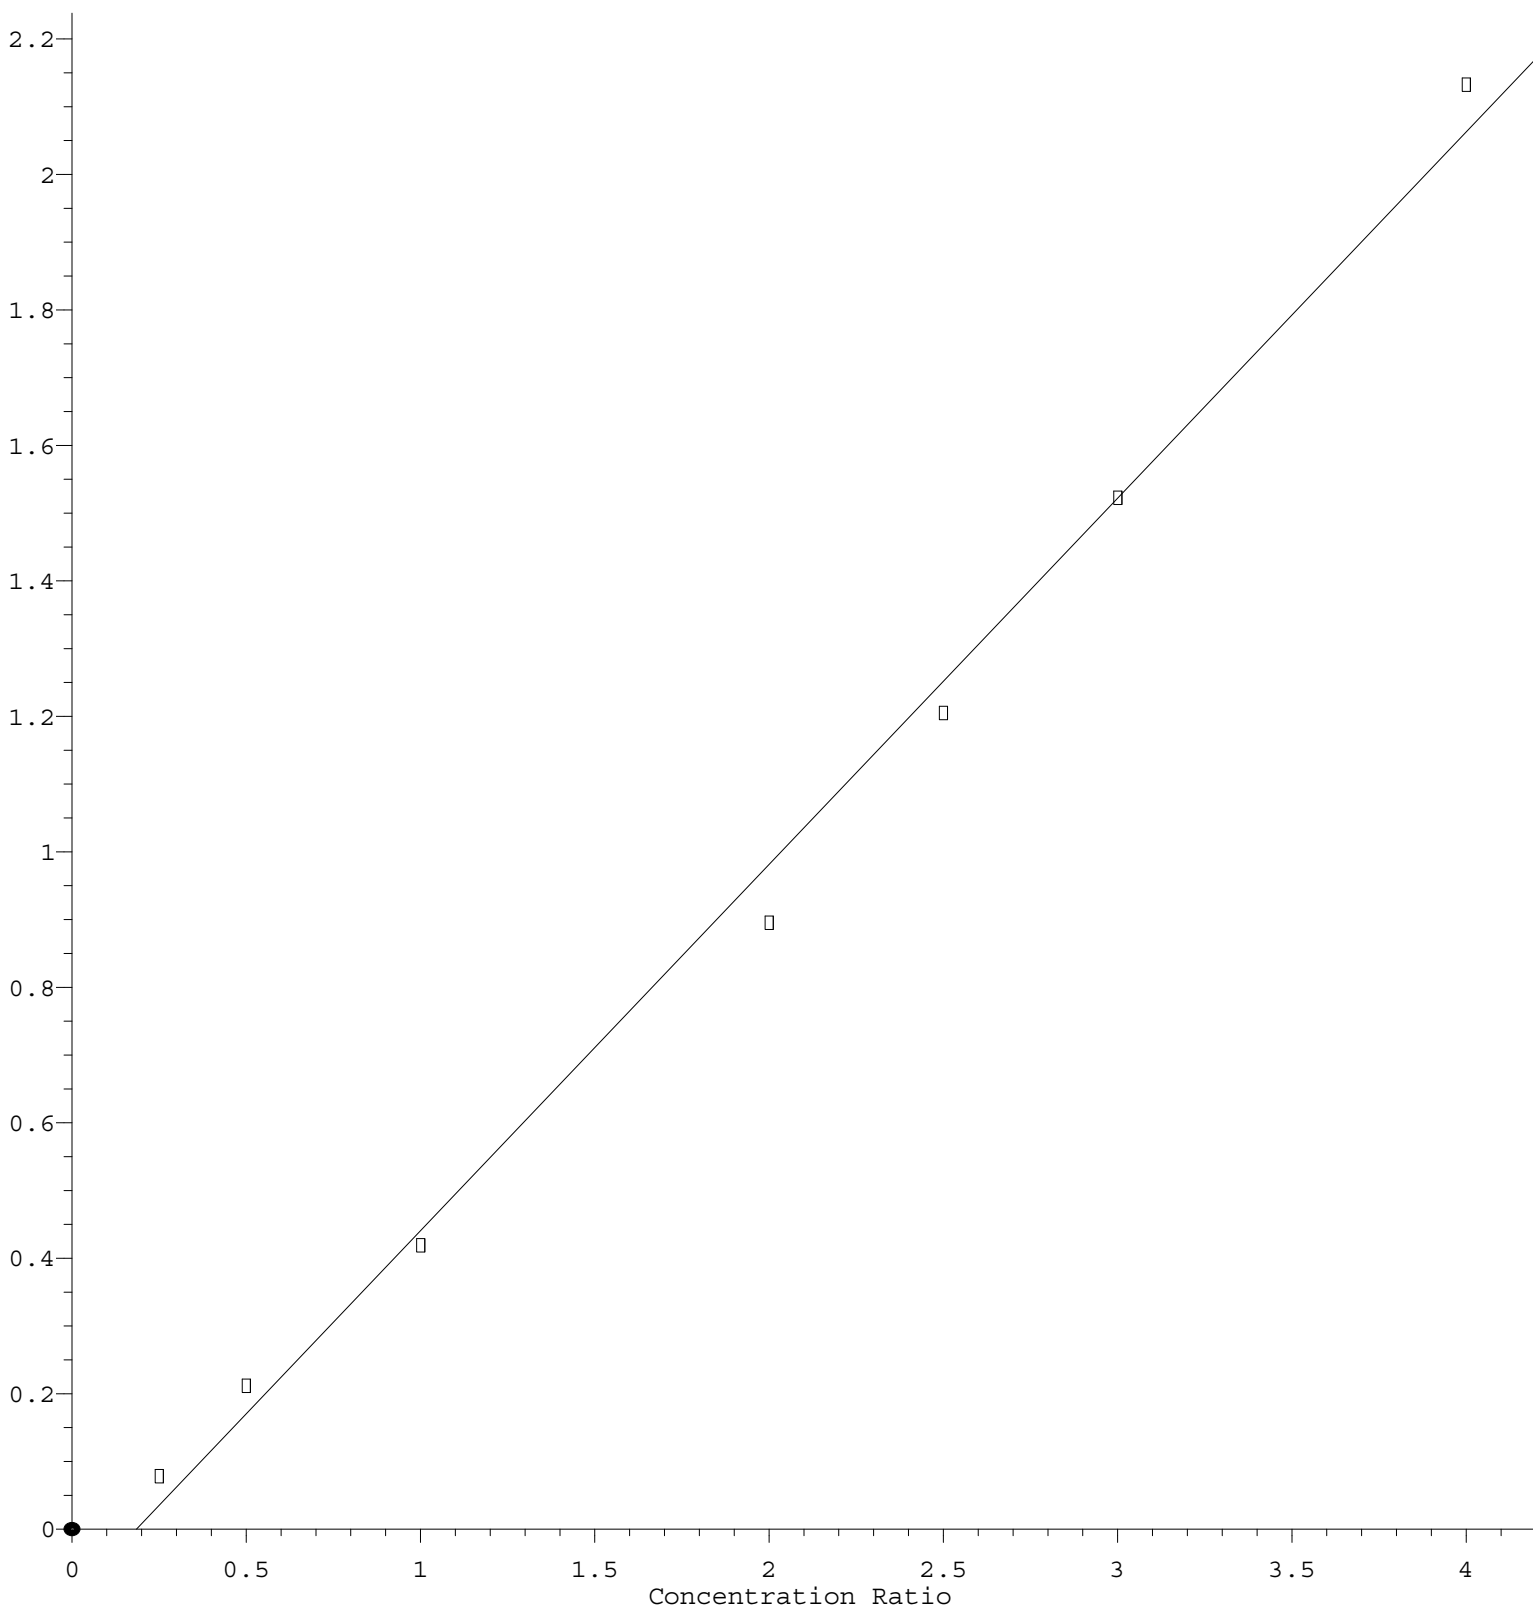

$$\text{Response} = 5.407\text{e-}001 * \text{Amt} - 1.001\text{e-}001$$


Coef of Det (r^2) = 0.994527 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021

Bis(2-ethylhexyl)phthalate

Response Ratio

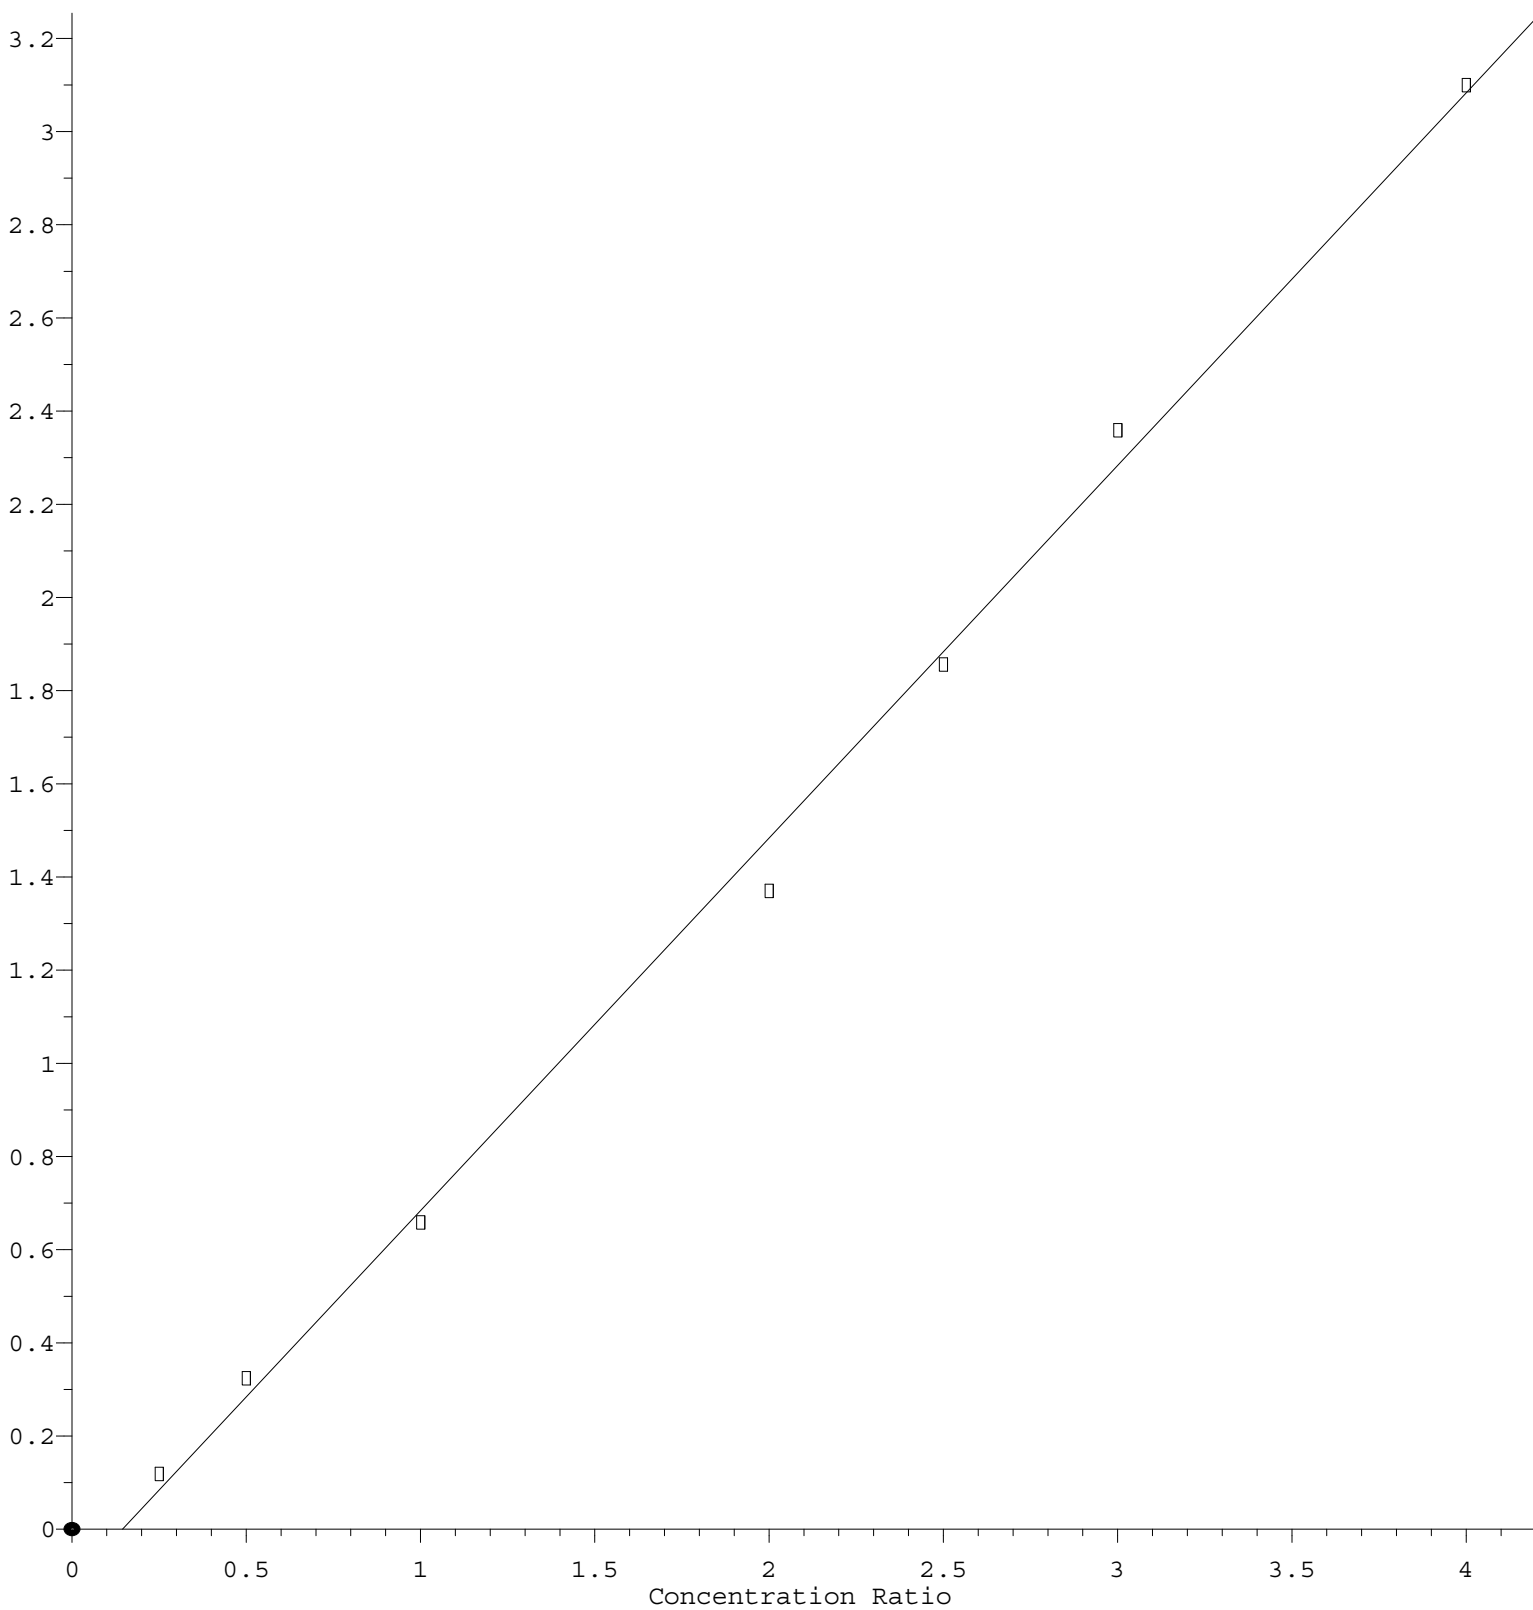

$$\text{Response} = 7.996\text{e-}001 * \text{Amt} - 1.158\text{e-}001$$

Coef of Det (r^2) = 0.996874 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM090821.M

Calibration Table Last Updated: Wed Sep 08 19:23:17 2021