

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
 Data File : BM032103.D
 Acq On : 08 Sep 2021 20:05
 Operator : CG/JU
 Sample : PB138943BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB138943BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM032103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.663	8	13	20	rVB2	53995	99154	2.44%	0.495%
2	2.746	24	27	36	rVB	57177	63562	1.56%	0.317%
3	5.004	405	411	427	rBV	1667408	2448249	60.21%	12.220%
4	6.569	670	677	699	rBV	1664190	2639626	64.92%	13.175%
5	7.363	805	812	821	rBV	287926	452767	11.14%	2.260%
6	8.516	1001	1008	1026	rBV	987132	1629630	40.08%	8.134%
7	10.116	1271	1280	1293	rBV	337148	592958	14.58%	2.960%
8	12.627	1699	1707	1724	rBV	2429600	3596298	88.45%	17.950%
9	14.021	1937	1944	1956	rBV	493190	756292	18.60%	3.775%
10	15.533	2194	2201	2224	rBV	952134	1627054	40.01%	8.121%
11	16.786	2408	2414	2429	rBV	516979	806909	19.84%	4.027%
12	19.445	2860	2866	2888	rBV	3264048	4066135	100.00%	20.295%
13	21.003	3126	3131	3143	rBV	447380	655619	16.12%	3.272%
14	23.097	3482	3487	3499	rBV2	292163	601131	14.78%	3.000%




Sum of corrected areas: 20035384

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
Data File : BM032103.D
Acq On : 08 Sep 2021 20:05
Operator : CG/JU
Sample : PB138943BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138943BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

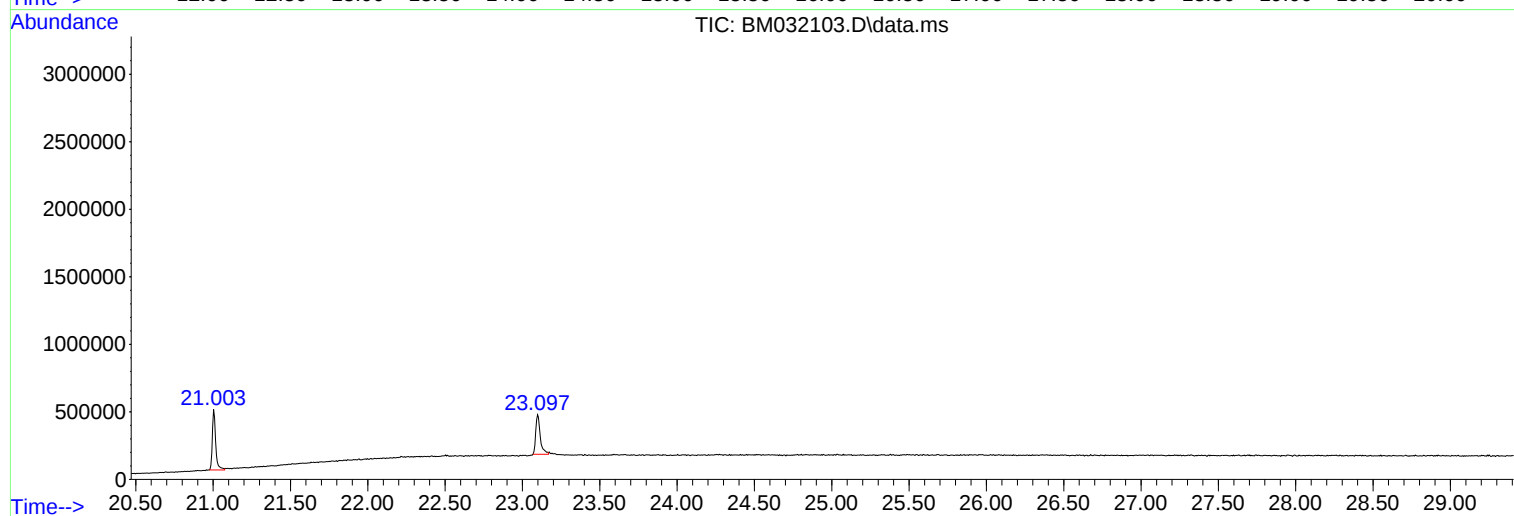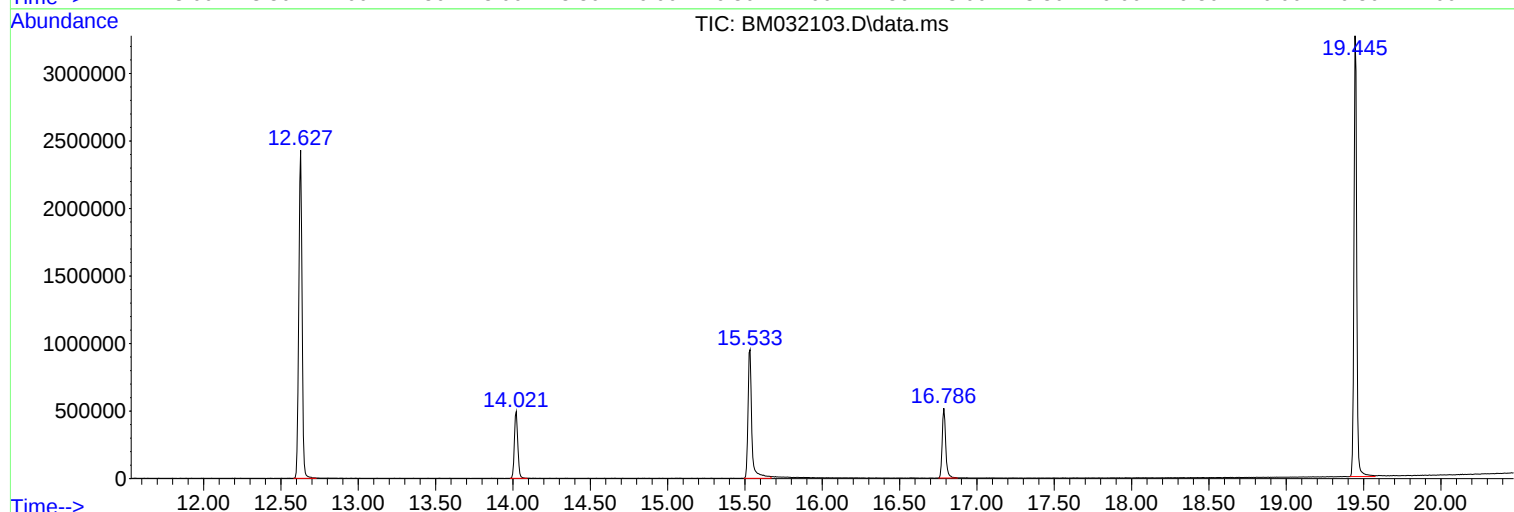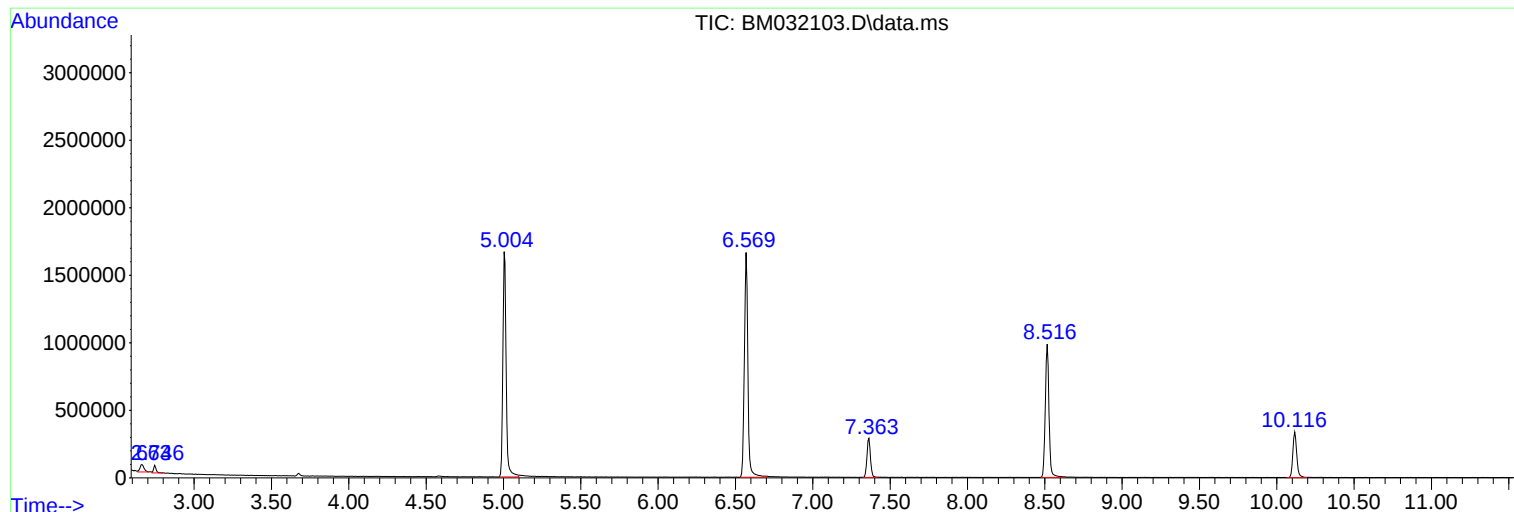

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
Data File : BM032103.D
Acq On : 08 Sep 2021 20:05
Operator : CG/JU
Sample : PB138943BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138943BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.746	2.81 ng	63562	1,4-Dichlorobenzene-d4	7.363

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
4			2,5-Dimethyl-4-hydroxy-3-hexanone	144	C8H16O2	000815-77-0	28
5			Butanoic acid, 2-hydroxy-2-methyl-	132	C6H12O3	032793-34-3	23

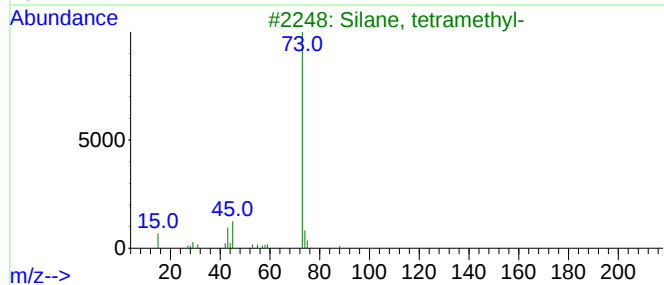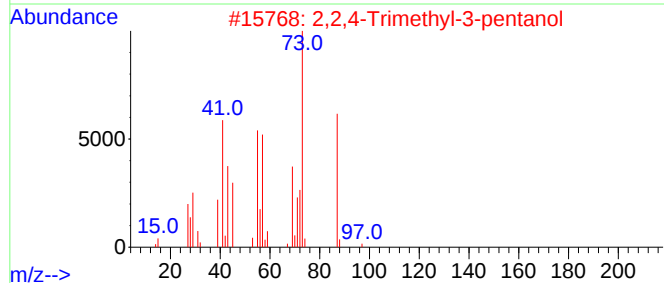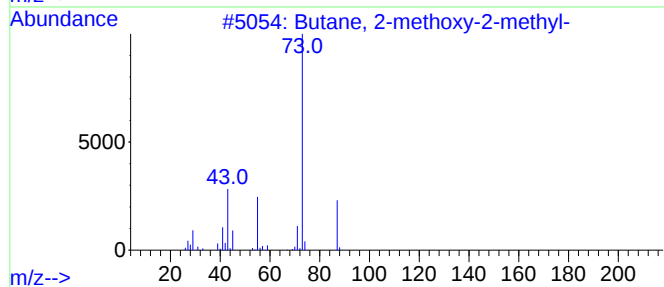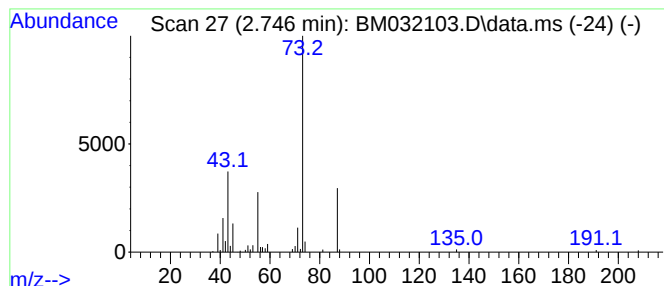

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
Data File : BM032103.D
Acq On : 08 Sep 2021 20:05
Operator : CG/JU
Sample : PB138943BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB138943BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.746	2.8	ng	63562	1	7.363	452767	20.0