
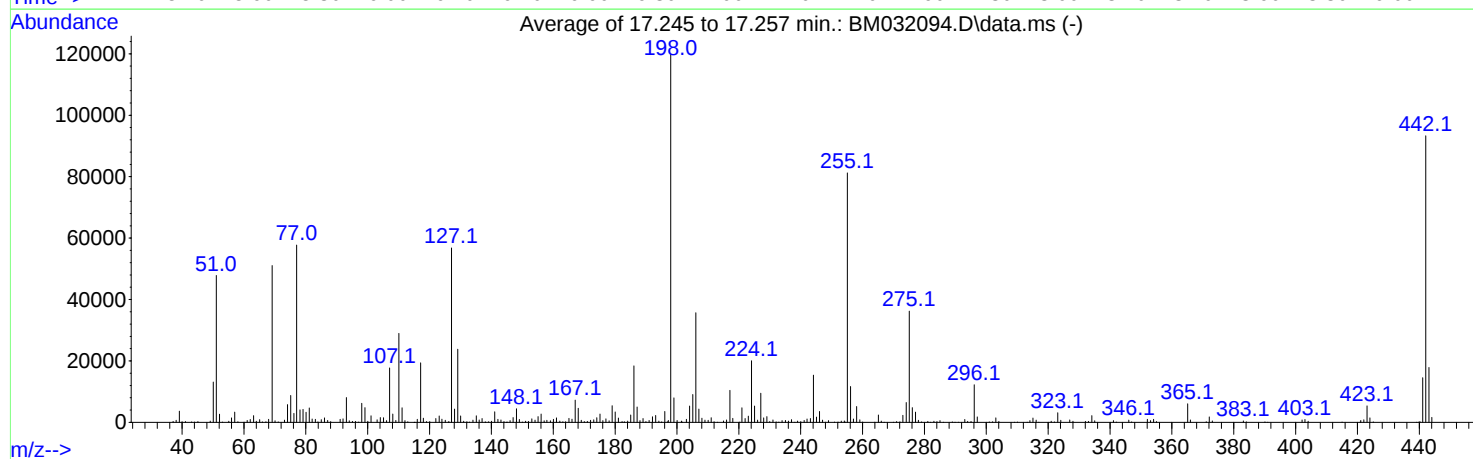


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
 Data File : BM032094.D
 Acq On : 08 Sep 2021 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 08 19:23:17 2021

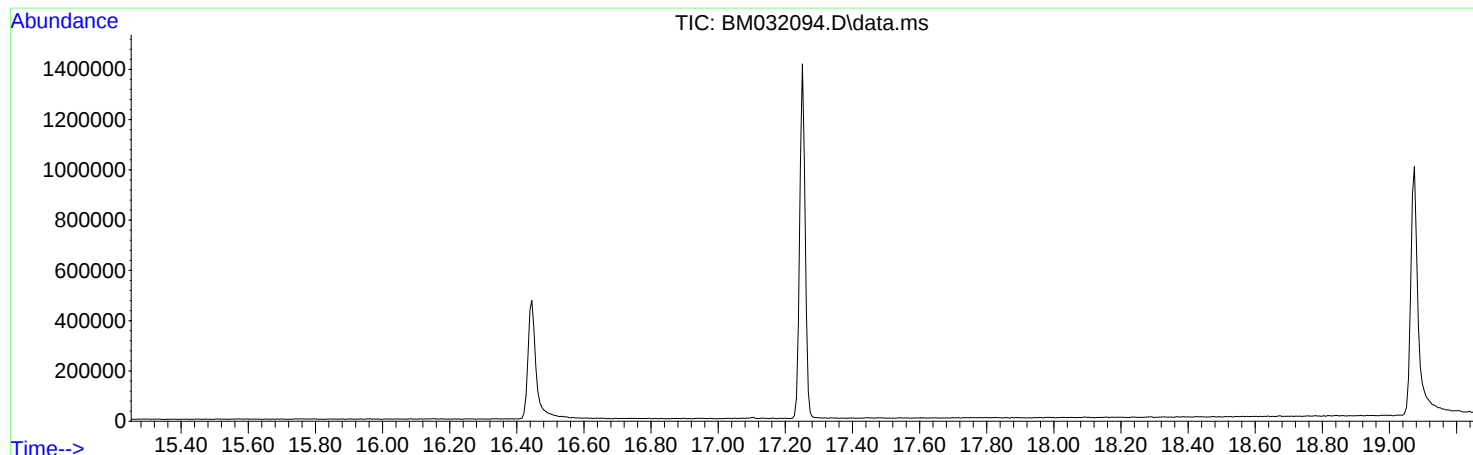




AutoFind: Scans 2407, 2408, 2409; Background Corrected with Scan 2401

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	47846	PASS
68	69	0.00	2	2.0	1019	PASS
69	198	0.00	100	42.6	51054	PASS
70	69	0.00	2	1.0	511	PASS
127	198	10	80	47.4	56779	PASS
197	198	0.00	2	0.5	624	PASS
198	198	100	100	100.0	119773	PASS
199	198	5	9	6.7	7986	PASS
275	198	10	60	30.2	36221	PASS
365	198	1	100	5.1	6052	PASS
441	198	0.01	100	12.1	14529	PASS
442	442	50	100	100.0	93280	PASS
443	442	15	24	19.2	17882	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
 Data File : BM032094.D
 Acq On : 08 Sep 2021 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 08 20:04:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 19:23:17 2021
 Response via : Initial Calibration

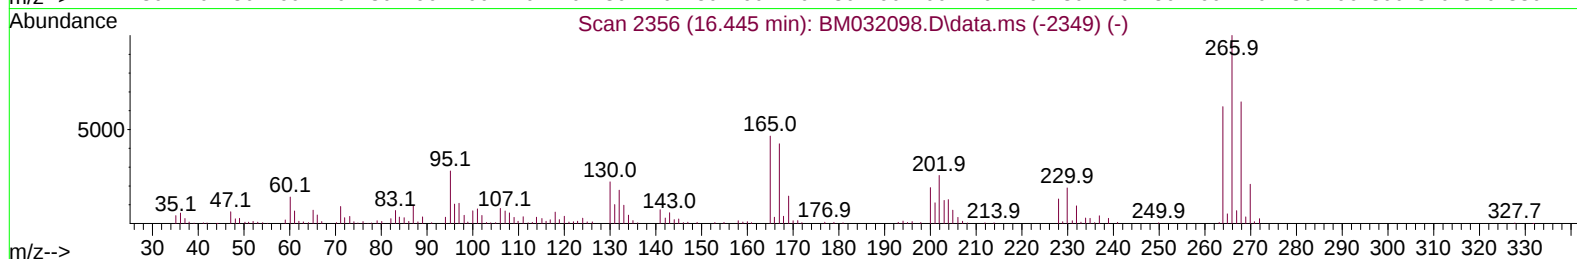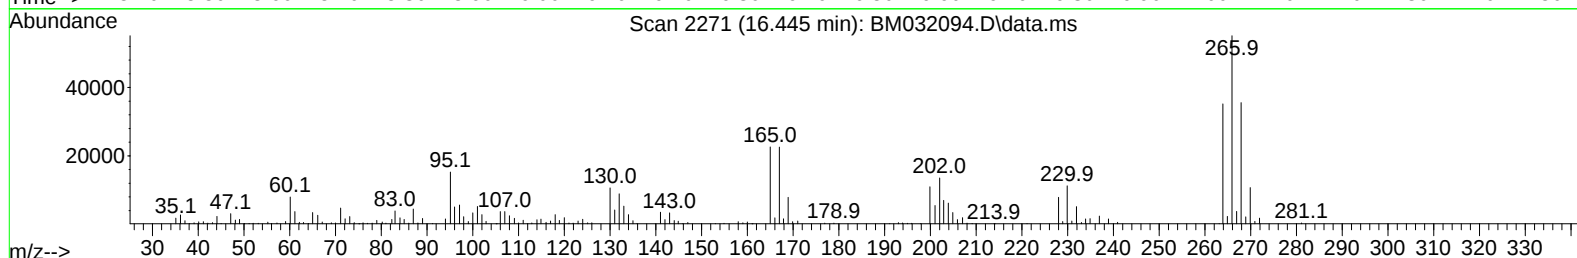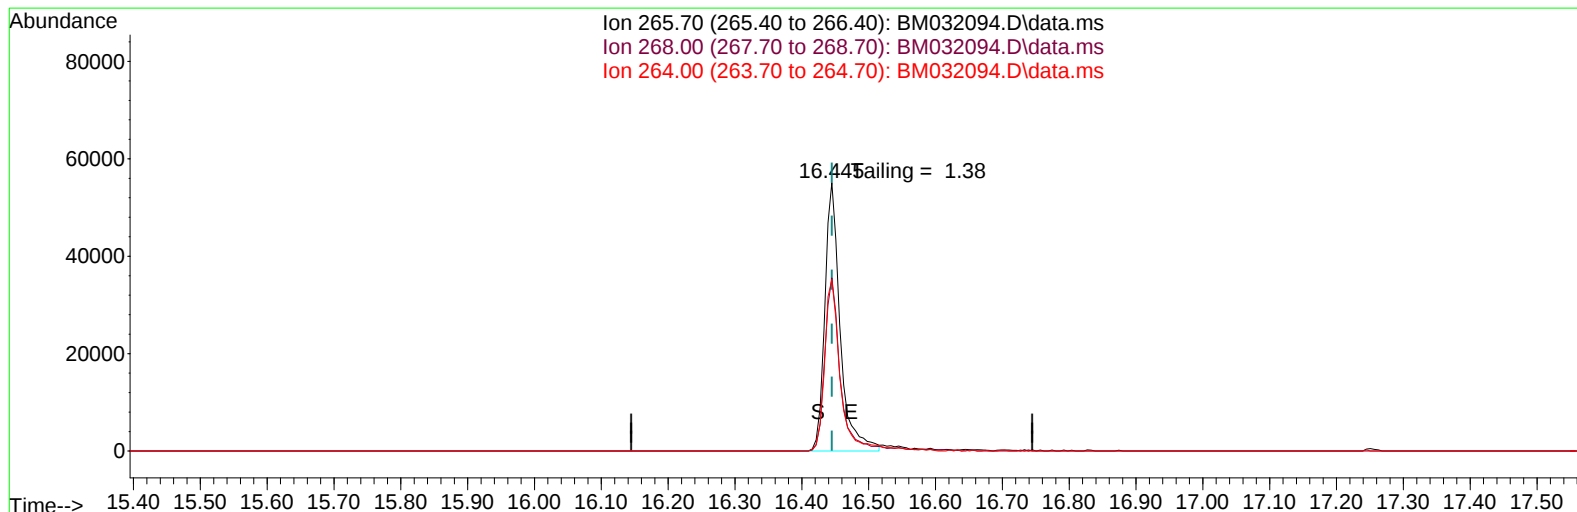

TIC: BM032094.D\data.ms

(70) Pentachlorophenol (C)

16.445min (+ 0.000) 0.00 ng




response 90770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.49
264.00	65.10	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM090821\
 Data File : BM032094.D
 Acq On : 08 Sep 2021 11:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 08 20:04:01 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM090821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 19:23:17 2021
 Response via : Initial Calibration

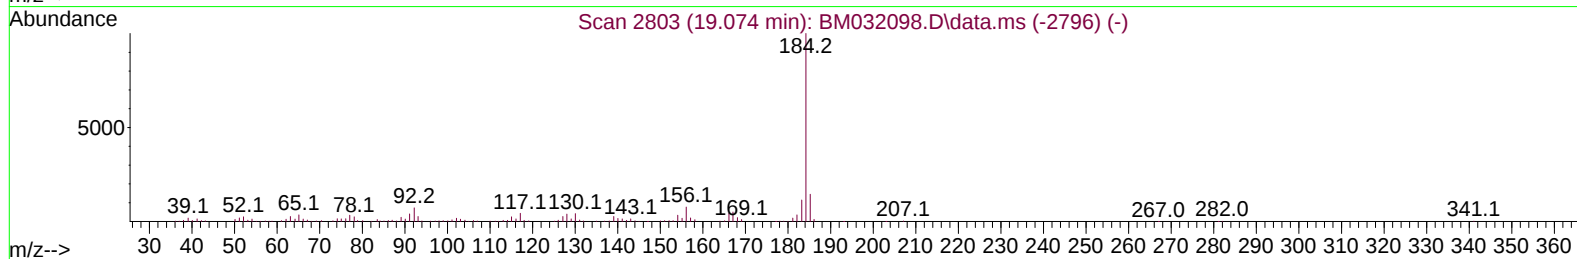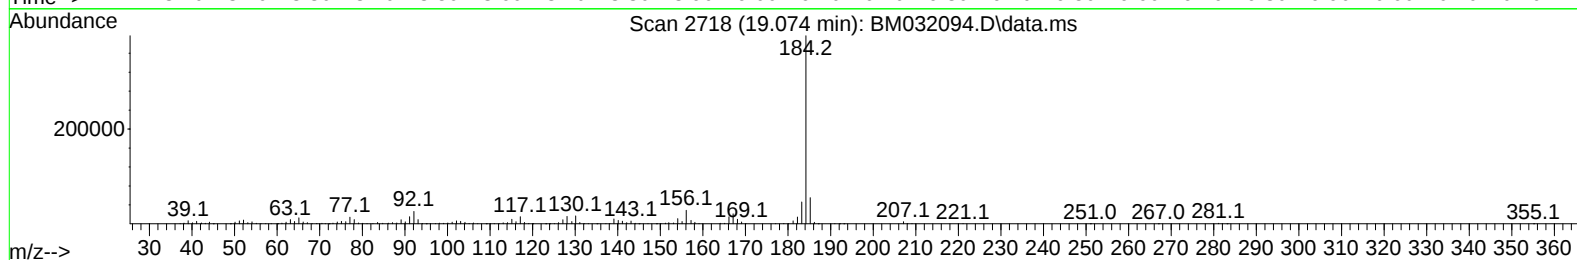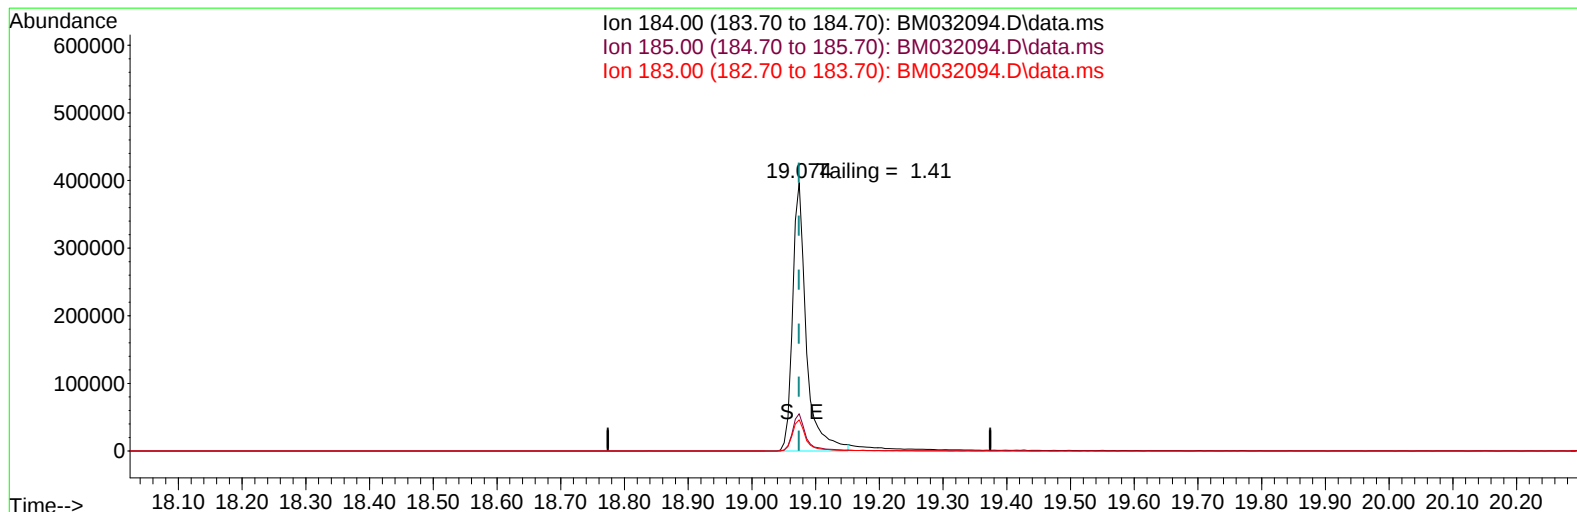

TIC: BM032094.D\data.ms

(77) Benzidine

19.074min (+ 0.000) 0.00 ng

response 626975

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.92
183.00	11.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/8/2021	BNA_M	<u>BM032094.D</u>
Compound Name	Response	Retention Time
DDT	249326	20.3
DDD	597	19.86
DDE	441	19.35
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1038	250364	0.41

Instrument :
BNA_M
ClientSampleId :
DFTPP