

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090916\
 Data File : BM007469.D
 Acq On : 09 Sep 2016 16:08
 Operator : UM/SJ
 Sample : PB93305BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	736	744	756	rBV	788320	1327478	13.95%	1.876%
2	7.122	765	771	783	rVB	635612	1025391	10.77%	1.449%
3	7.322	798	805	815	rBV	850596	1390414	14.61%	1.965%
4	7.786	876	884	897	rBV	565989	942001	9.90%	1.331%
5	8.492	997	1004	1014	rBV	1095907	1807477	18.99%	2.554%
6	8.945	1072	1081	1092	rBV	872893	1460037	15.34%	2.063%
7	9.663	1194	1203	1216	rBV	763105	1313122	13.80%	1.856%
8	10.198	1285	1294	1308	rBV	1055672	1890374	19.86%	2.671%
9	10.575	1350	1358	1368	rBV	878786	1473591	15.48%	2.082%
10	10.710	1374	1381	1405	rBV	825825	1523301	16.00%	2.153%
11	13.827	1905	1911	1922	rBV	2504607	3703011	38.91%	5.233%
12	14.115	1952	1960	1974	rBV	2569652	3992856	41.95%	5.642%
13	14.421	2005	2012	2025	rVB2	1554581	2334062	24.52%	3.298%
14	14.633	2041	2048	2077	rBV	986467	1899604	19.96%	2.684%
15	15.415	2174	2181	2193	rBV	3622853	5267215	55.34%	7.443%
16	15.539	2196	2202	2215	rVV	1218222	1828856	19.21%	2.584%
17	17.162	2472	2478	2488	rBV2	2224444	3197725	33.60%	4.519%
18	17.262	2488	2495	2520	rVV2	4306779	6365427	66.88%	8.995%
19	19.556	2879	2885	2899	rBV2	5646976	8120711	85.32%	11.475%
20	21.344	3184	3189	3200	rBV	3789740	4935794	51.86%	6.975%
21	23.474	3543	3551	3565	rVV2	4867778	9518013	100.00%	13.450%
22	23.615	3568	3575	3589	rVB	2547712	5000267	52.53%	7.066%
23	24.127	3657	3662	3671	rVB	115278	217963	2.29%	0.308%
24	24.879	3785	3790	3797	rVB4	106117	232583	2.44%	0.329%


Sum of corrected areas: 70767273

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090916\
Data File : BM007469.D
Acq On : 09 Sep 2016 16:08
Operator : UM/SJ
Sample : PB93305BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

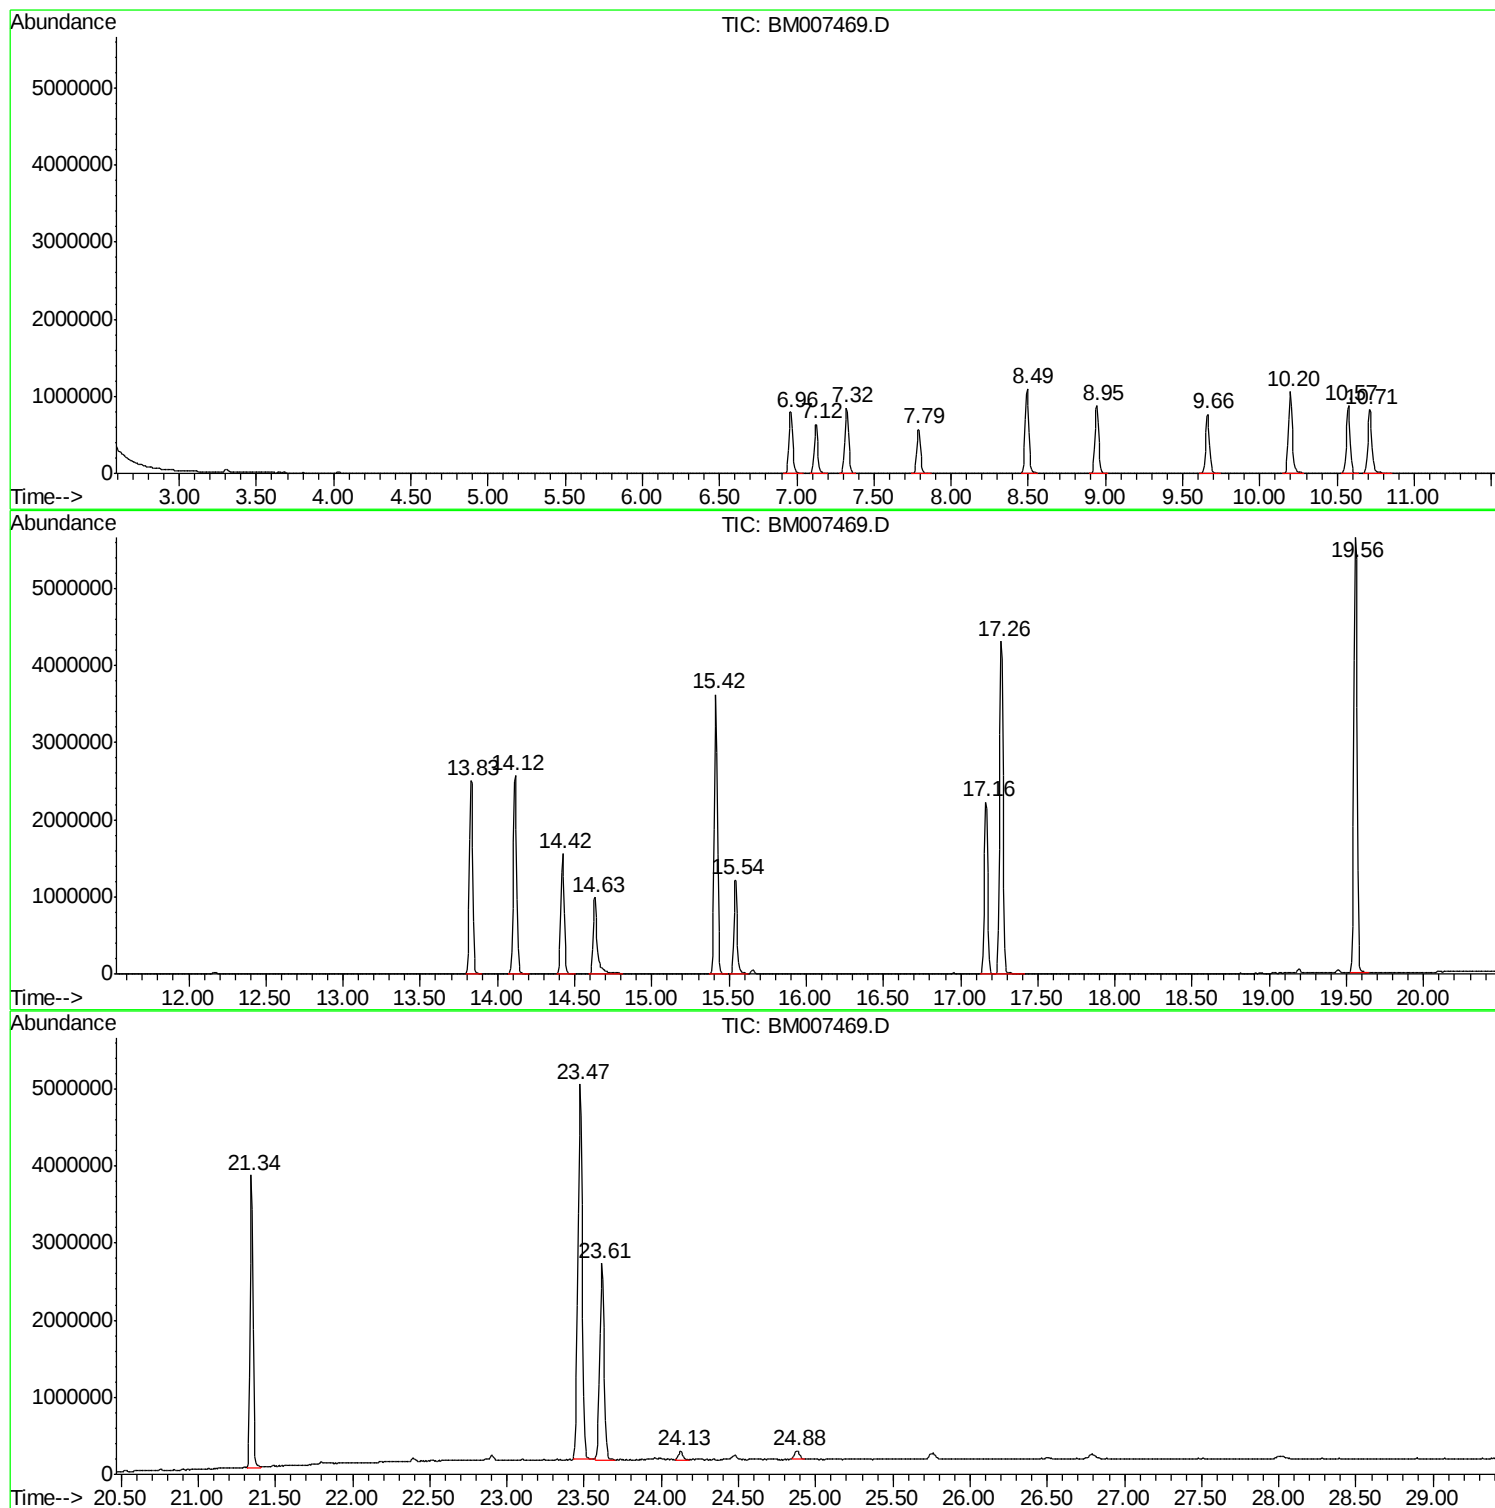

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090916\
Data File : BM007469.D
Acq On : 09 Sep 2016 16:08
Operator : UM/SJ
Sample : PB93305BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM090916\
Data File : BM007469.D
Acq On : 09 Sep 2016 16:08
Operator : UM/SJ
Sample : PB93305BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc