

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
 Data File : BM027384.D
 Acq On : 10 Sep 2020 21:27
 Operator : JU/CG
 Sample : L3855-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW283

Quant Time: Sep 11 00:34:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 11 00:29:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	177245	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	707757	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	509455	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	1182916	20.00	ng/ul	0.00
78) Chrysene-d12	21.15	240	1257989	20.00	ng/ul	0.00
86) Perylene-d12	23.32	264	1103236	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	17270	4.34	ng/uL	0.00
5) Phenol-d5	6.75	99	300857	20.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	211081	21.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	239164	22.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	245992	20.65	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	120777	22.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	134717	23.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	264433	21.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	328424	22.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	930890	22.96	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1110275	24.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	110852	15.53	ng/ul	0.00
58) Fluorene-d10	15.20	176	802375	22.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	118387	15.64	ng/ul	0.00
71) Anthracene-d10	17.05	188	1289624	23.05	ng/ul	0.00
79) Pyrene-d10	19.35	212	1556405	27.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.18	264	1361931	23.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	183795	4.302	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027384.D
Acq On : 10 Sep 2020 21:27
Operator : JU/CG
Sample : L3855-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
EW283

Quant Time: Sep 11 00:34:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 11 00:29:15 2020
Response via : Initial Calibration

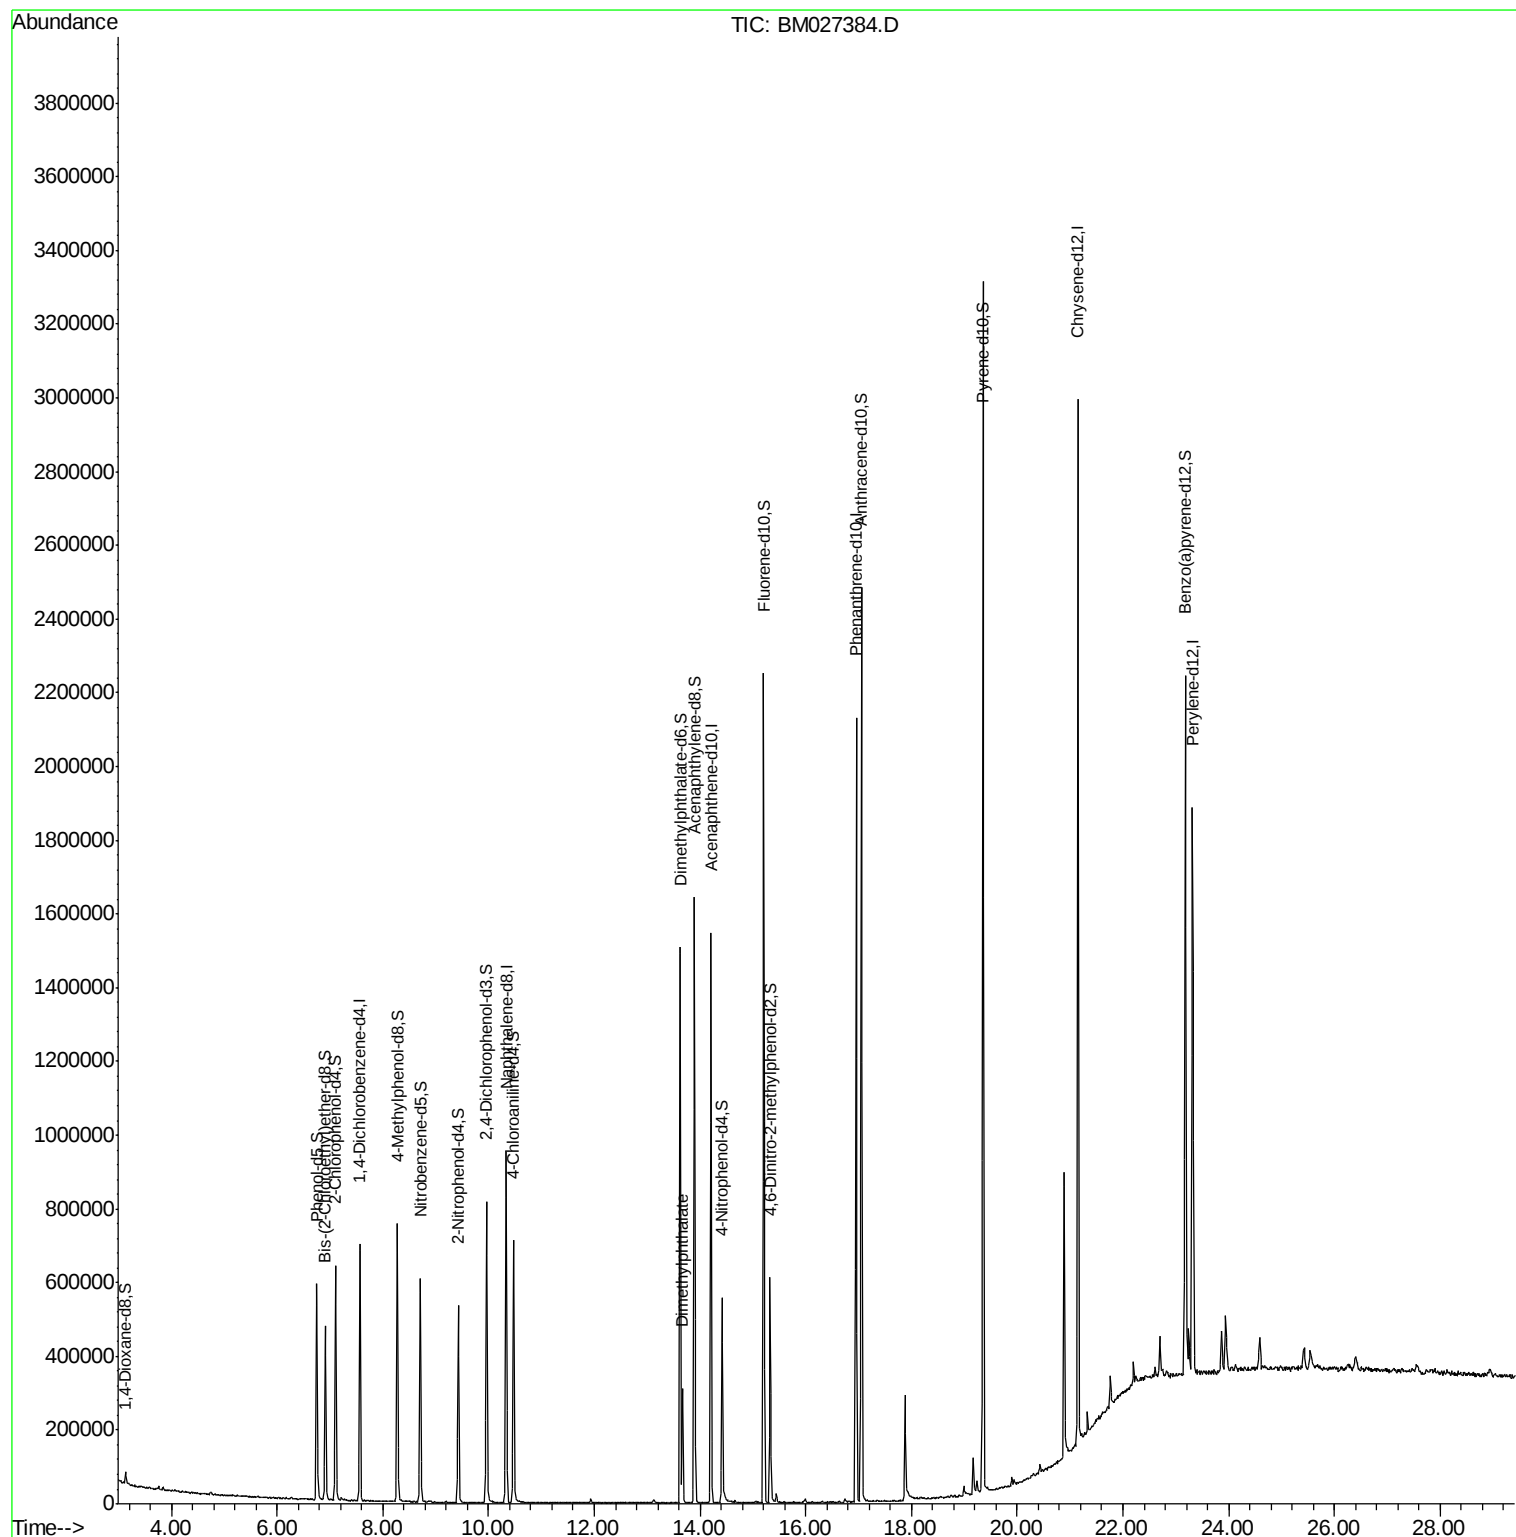

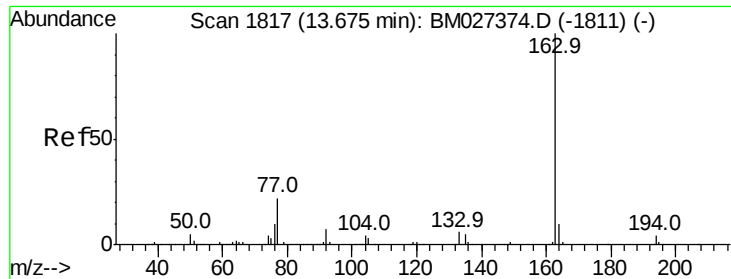

#45

Dimethylphthalate

Concen: 4.302 ng/ul

RT: 13.67 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM027384.D

Acq: 10 Sep 2020 21:27

Instrument :

BNA_M

ClientSampleId :

EW283


Tot Ion:163 Resp: 183795

Ion Ratio Lower Upper

163 100

194 3.8 3.3 4.9

164 9.8 8.1 12.1

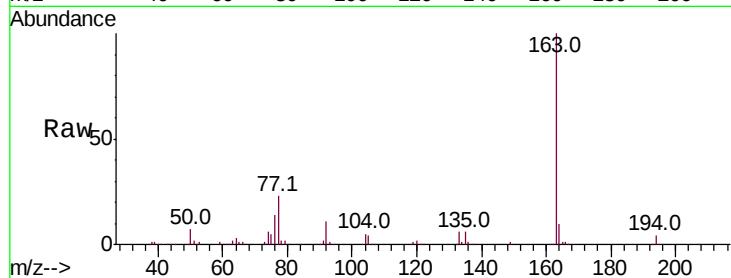

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

