

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
 Data File : BM027373.D
 Acq On : 10 Sep 2020 14:46
 Operator : JU/CG
 Sample : L3855-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW280

Quant Time: Sep 10 15:17:37 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 10 09:59:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	200782	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	829410	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	589178	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1345629	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1323032	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1094556	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	11880	2.63	ng/uL	0.00
5) Phenol-d5	6.75	99	233614	14.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	163348	14.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	185854	15.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	195515	14.49	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	96310	15.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	108640	15.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	207873	14.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	265966	15.27	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	745314	15.90	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	896341	16.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	69747	8.45	ng/ul	0.00
58) Fluorene-d10	15.20	176	640543	15.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	80530	9.35	ng/ul	0.00
71) Anthracene-d10	17.05	188	1037542	16.30	ng/ul	0.00
79) Pyrene-d10	19.36	212	1181532	20.05	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	934439	15.92	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.67	163	160078	3.240	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027373.D
Acq On : 10 Sep 2020 14:46
Operator : JU/CG
Sample : L3855-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW280

Quant Time: Sep 10 15:17:37 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 10 09:59:57 2020
Response via : Initial Calibration

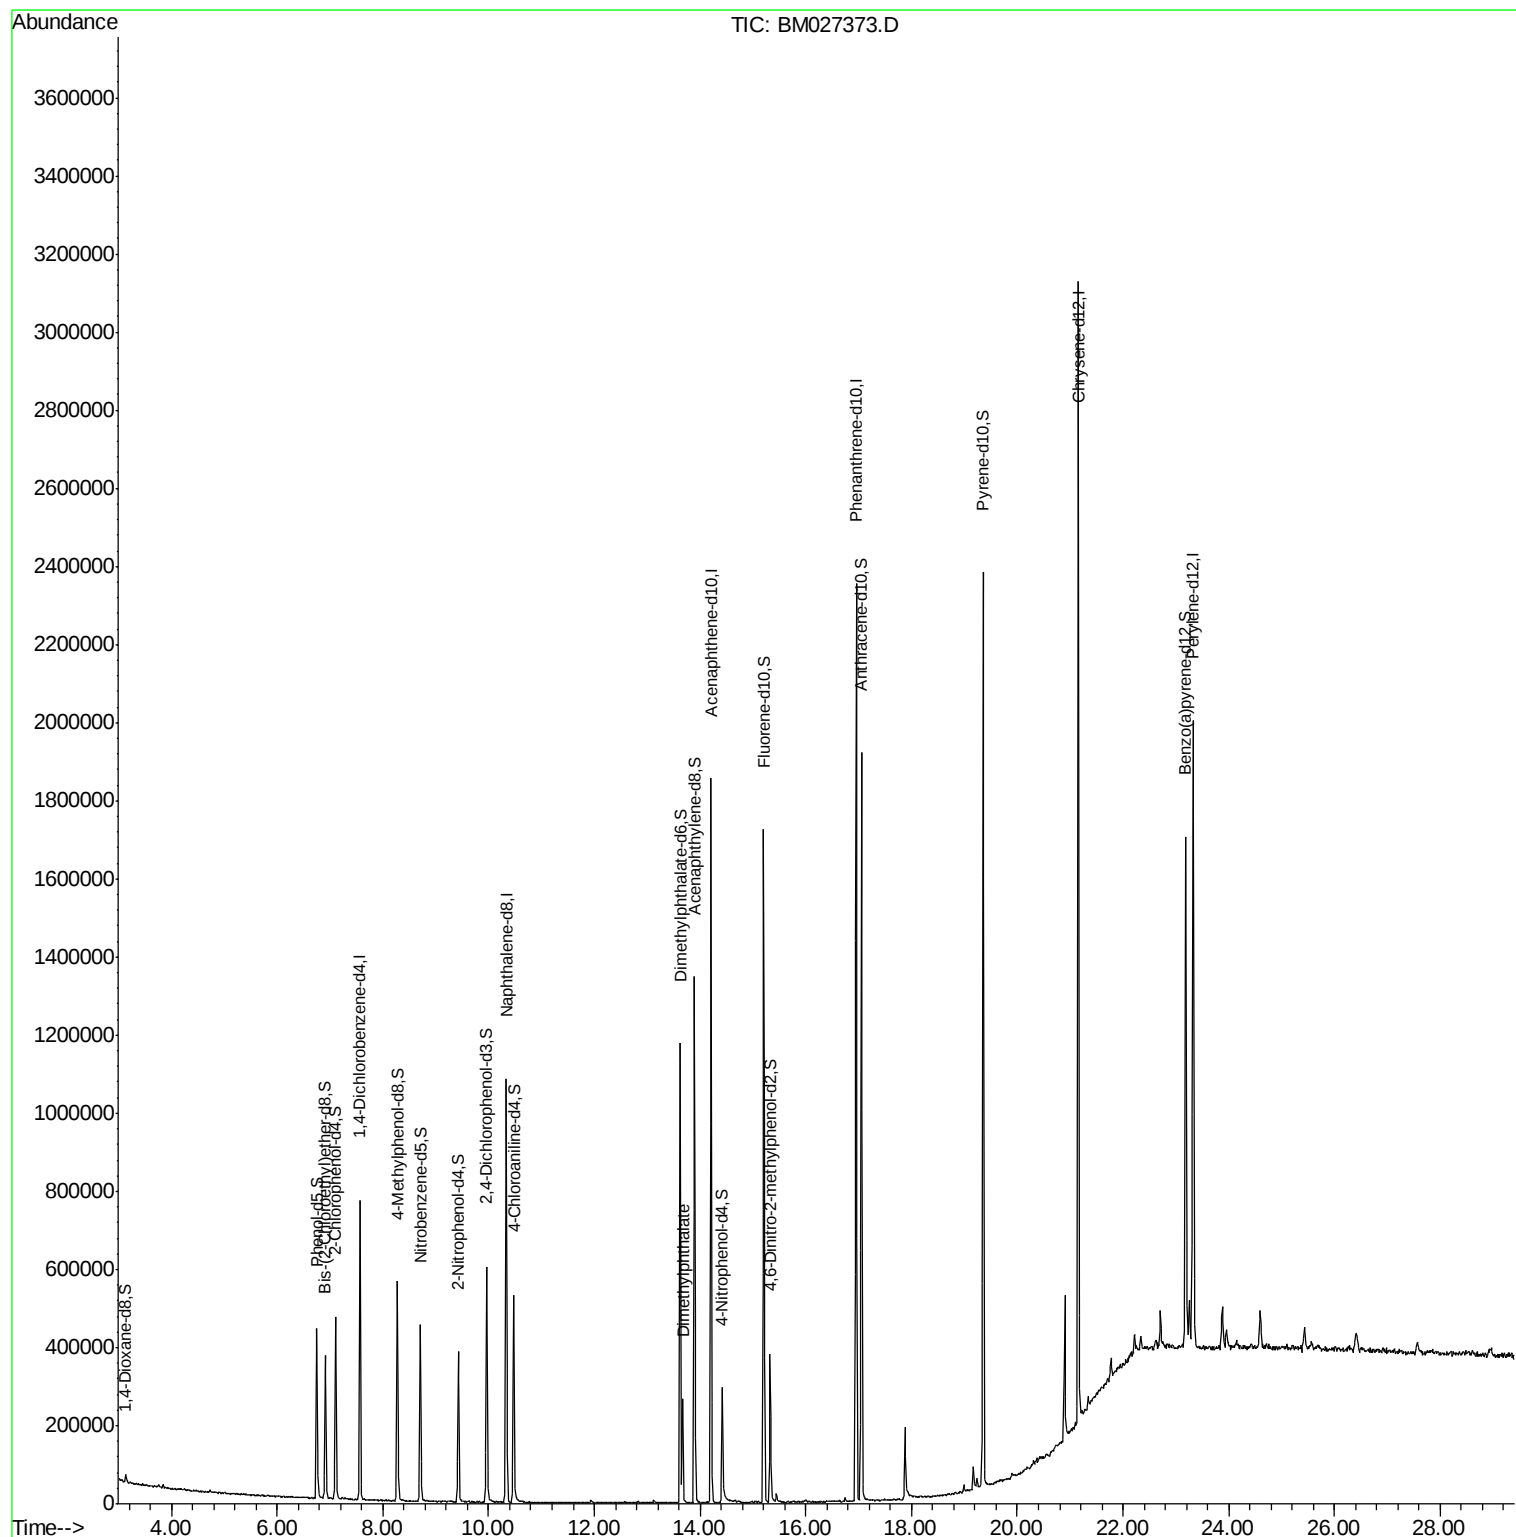

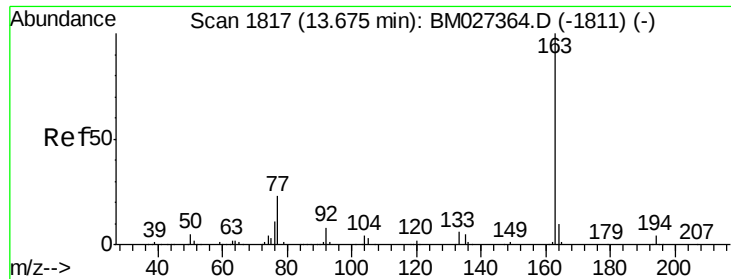

#45

Dimethylphthalate

Concen: 3.240 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM027373.D

Acq: 10 Sep 2020 14:46

Instrument :

BNA_M

ClientSampleId :

EW280

Tot Ion:163 Resp: 160078

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 10.6 8.1 12.1

