

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
 Data File : BM027375.D
 Acq On : 10 Sep 2020 15:59
 Operator : JU/CG
 Sample : L3855-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW275

Quant Time: Sep 10 16:30:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 10 09:59:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	142684	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	587776	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	426641	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	985959	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1157348	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1120042	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	10074	3.14	ng/uL	0.00
5) Phenol-d5	6.75	99	166352	14.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	128047	16.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	130258	15.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	118239	12.33	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	70509	15.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	79767	16.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	145009	13.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	151278	12.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	584470	17.22	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	607662	15.85	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	60477	10.12	ng/ul	0.00
58) Fluorene-d10	15.20	176	469551	15.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	77870	12.34	ng/ul	0.00
71) Anthracene-d10	17.05	188	716459	15.37	ng/ul	0.00
79) Pyrene-d10	19.36	212	916300	17.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	922830	15.36	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.67	163	126179	3.527	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027375.D
Acq On : 10 Sep 2020 15:59
Operator : JU/CG
Sample : L3855-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW275

Quant Time: Sep 10 16:30:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 10 09:59:57 2020
Response via : Initial Calibration

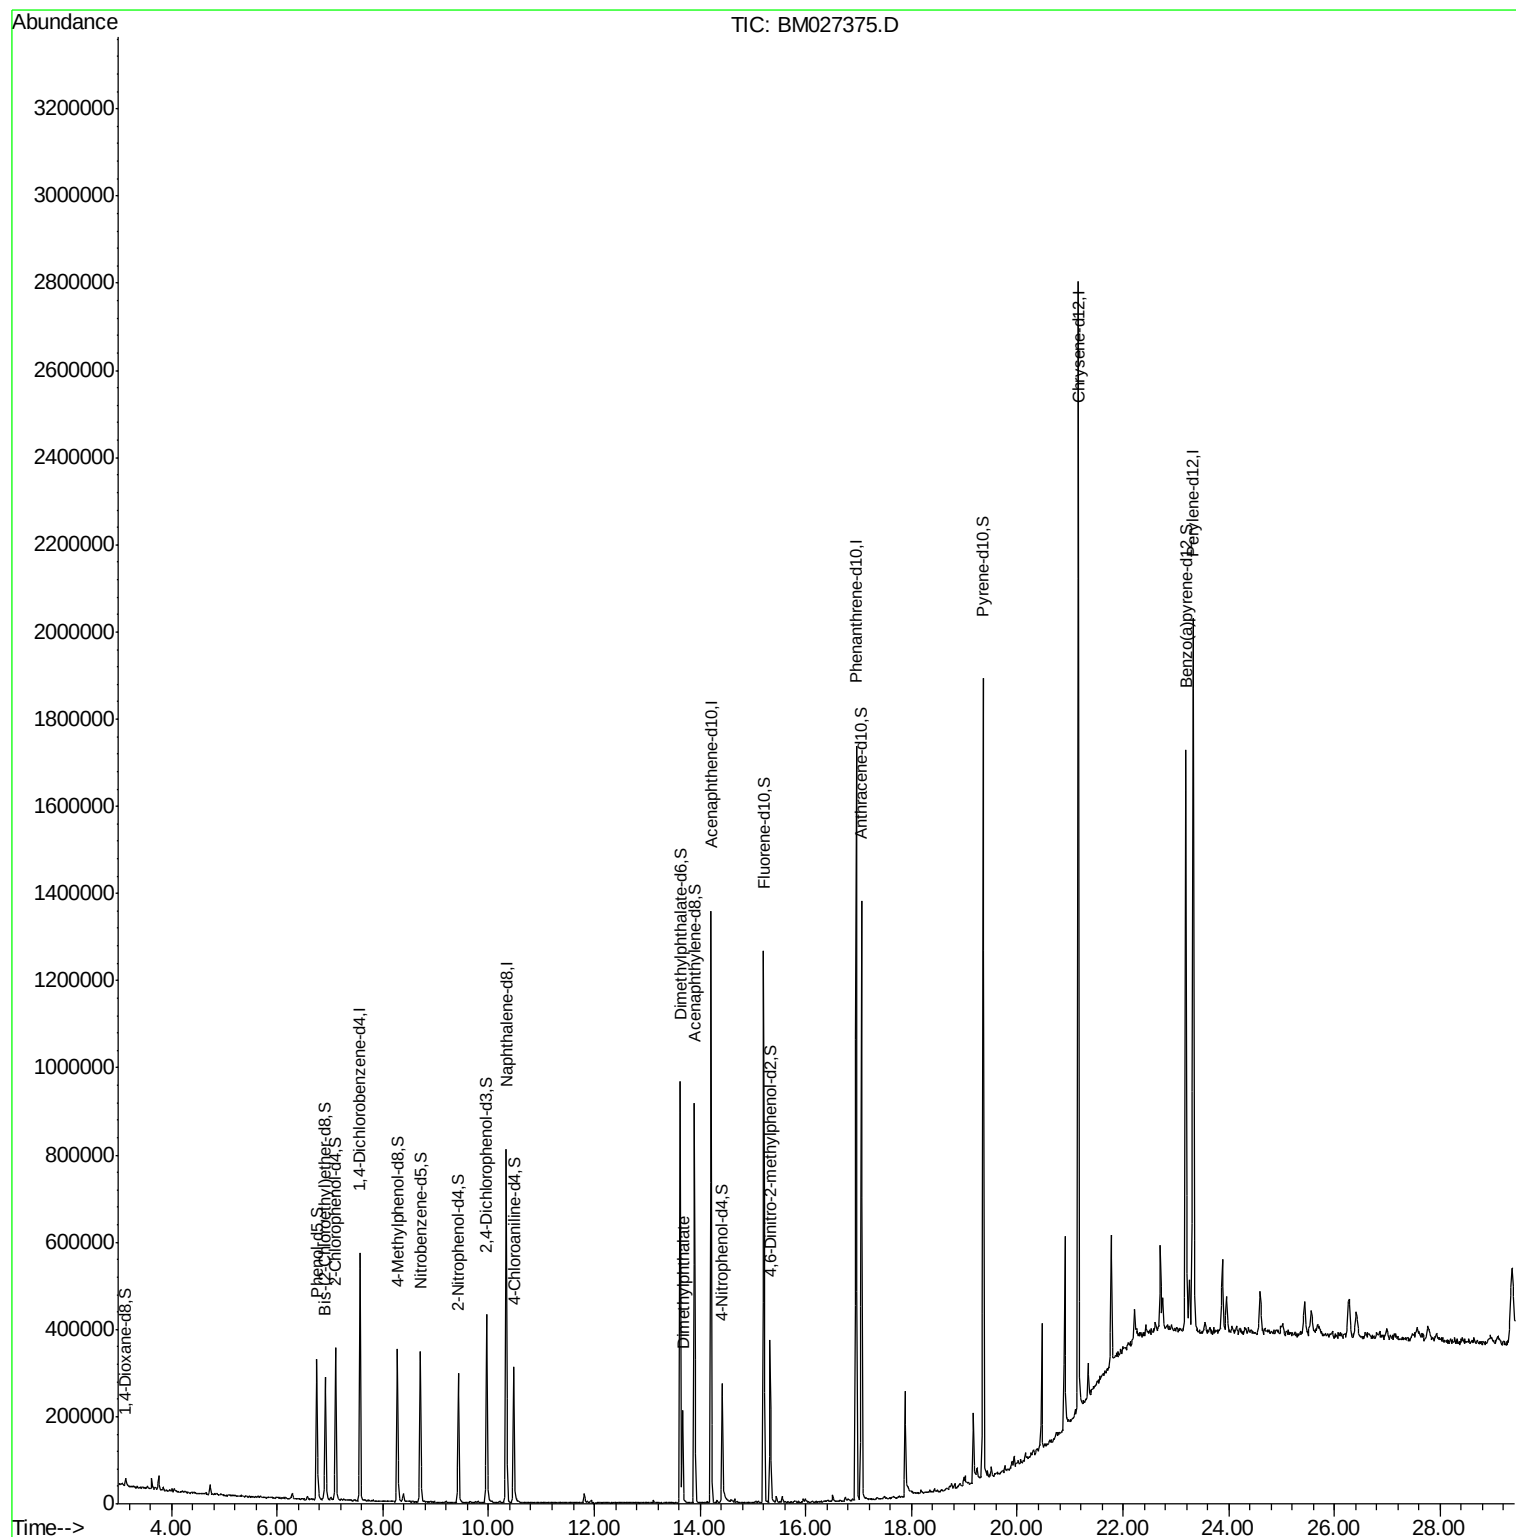

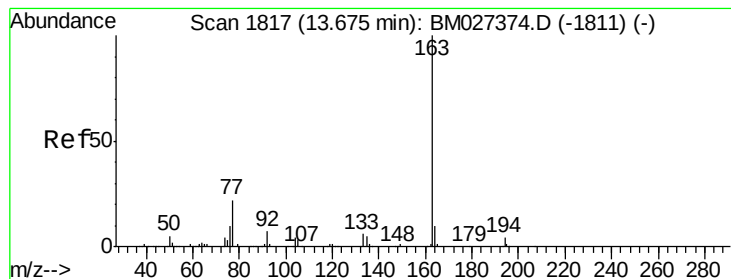

#45

Dimethylphthalate

Concen: 3.527 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM027375.D

Acq: 10 Sep 2020 15:59

Instrument :

BNA_M

ClientSampleId :

EW275

Tot Ion:163 Resp: 126179

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9

164 10.5 8.1 12.1

