

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
 Data File : BM027377.D
 Acq On : 10 Sep 2020 17:12
 Operator : JU/CG
 Sample : L3855-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW270

Quant Time: Sep 10 18:26:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 10 09:59:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	167108	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	682278	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.21	164	492939	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.96	188	1139217	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	1234623	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1088045	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	19261	5.13	ng/uL	0.00
5) Phenol-d5	6.75	99	360682	26.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	246891	26.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	282399	28.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	292885	26.07	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	143276	27.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	163536	29.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	315870	26.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	362118	25.27	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	1056701	26.94	ng/ul	0.00
47) Acenaphthylene-d8	13.90	160	1288172	29.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	121813	17.64	ng/ul	0.00
58) Fluorene-d10	15.20	176	918482	26.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	135249	18.55	ng/ul	0.00
71) Anthracene-d10	17.05	188	1422544	26.41	ng/ul	0.00
79) Pyrene-d10	19.36	212	1737573	31.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1586888	27.19	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.67	163	277864	6.722	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027377.D
Acq On : 10 Sep 2020 17:12
Operator : JU/CG
Sample : L3855-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW270

Quant Time: Sep 10 18:26:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 10 09:59:57 2020
Response via : Initial Calibration

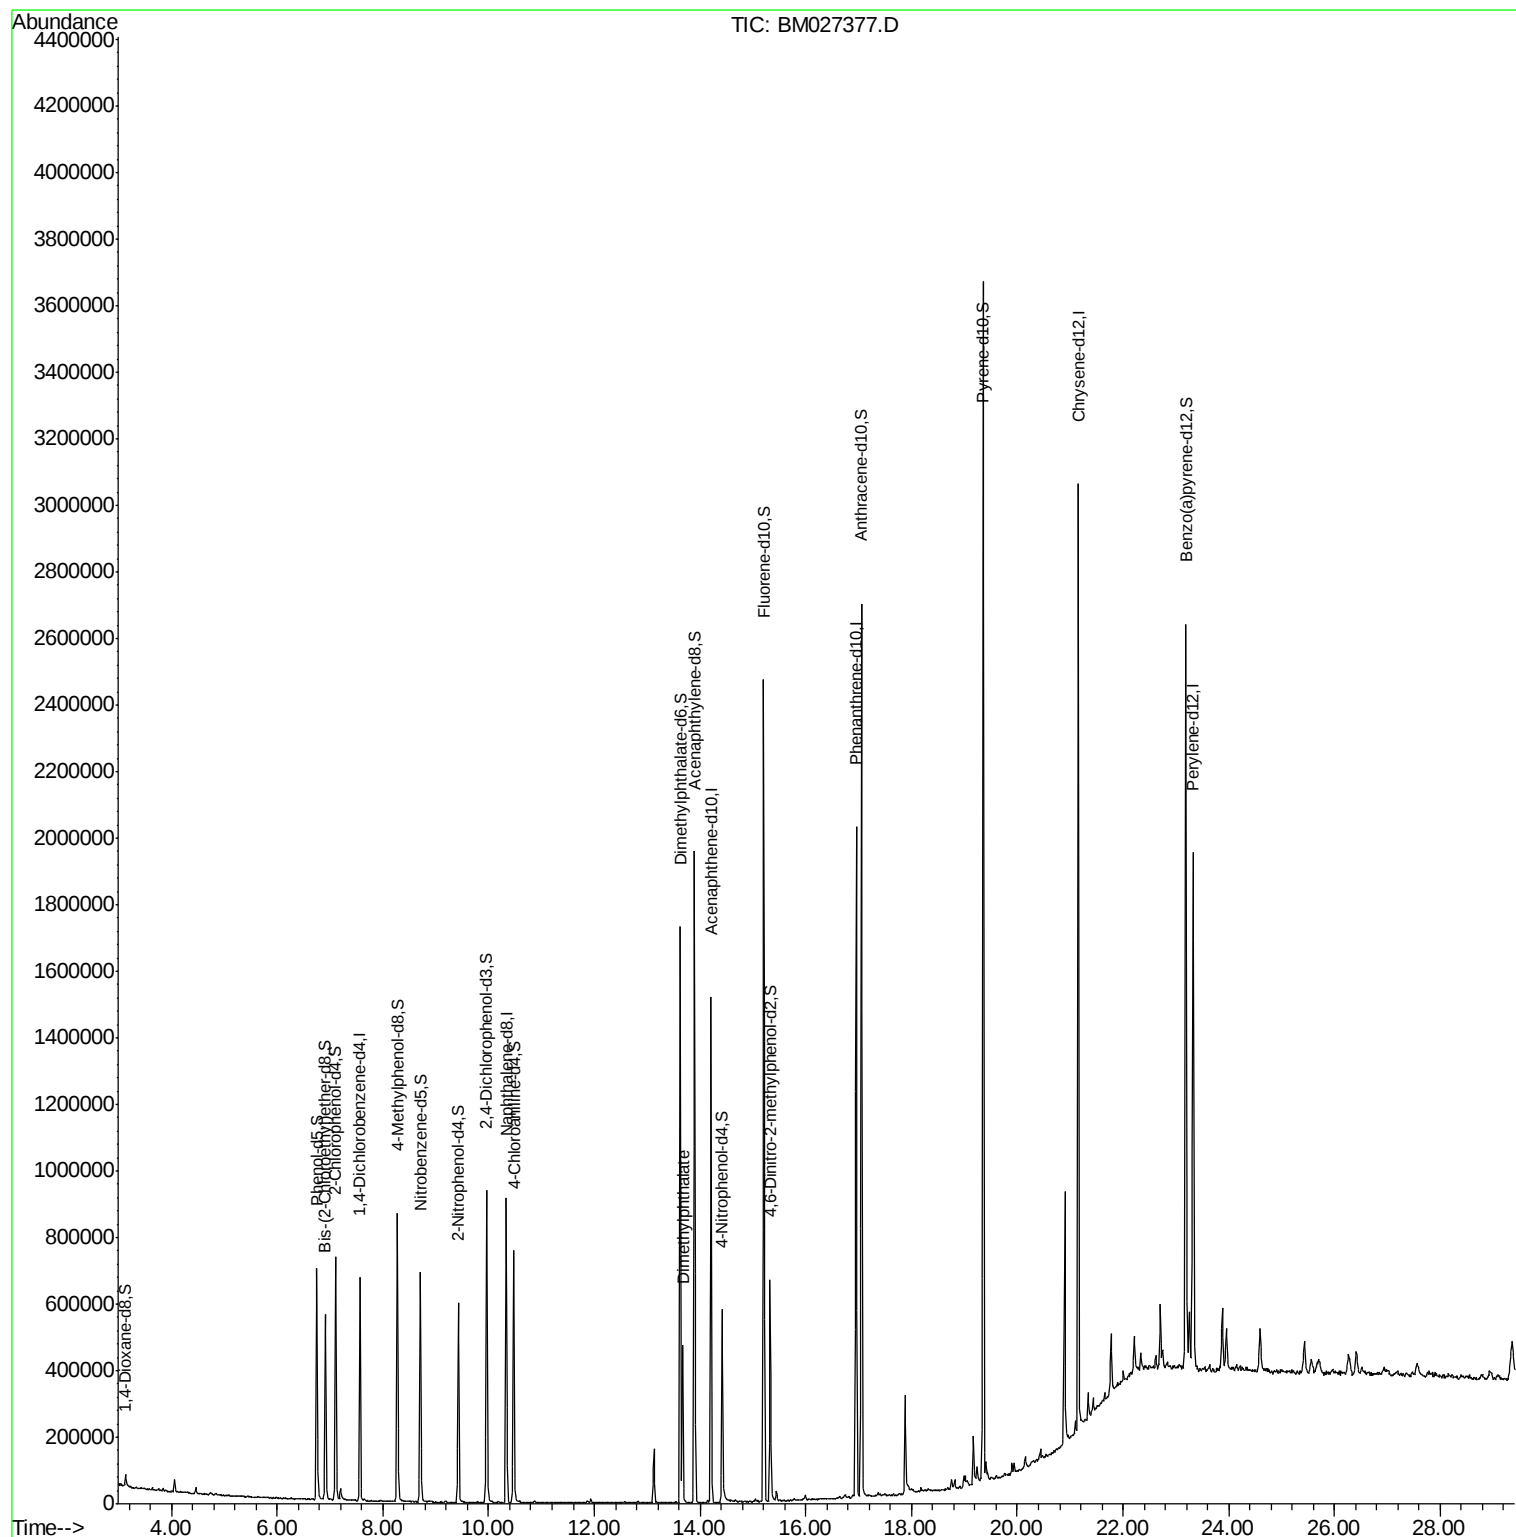

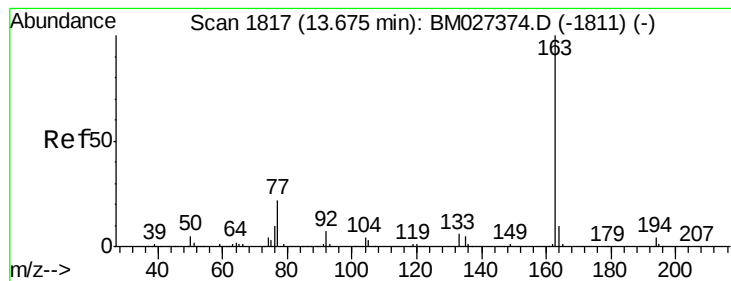

#45

Dimethylphthalate

Concen: 6.722 ng/ul

RT: 13.67 min Scan# 1817

Delta R.T. -0.00 min

Lab File: BM027377.D

Acq: 10 Sep 2020 17:12

Instrument :

BNA_M

ClientSampleId :

EW270


Tot Ion:163 Resp: 277864

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.1 8.1 12.1

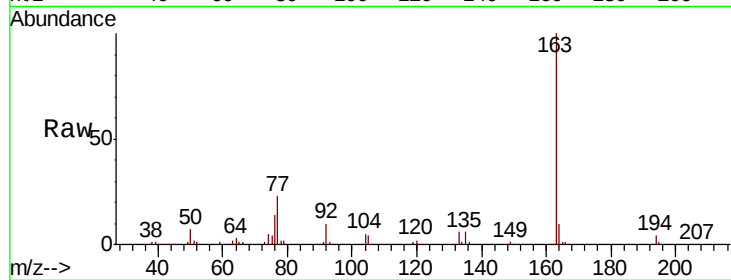

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

