

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
 Data File : BM027394.D
 Acq On : 11 Sep 2020 04:05
 Operator : JU/CG
 Sample : L3907-19
 Misc : GCMS CONFIRMATION
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET1A6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.063	9	13	18	rVB	163008	158723	9.41%	1.795%
2	3.387	65	68	72	rVB2	18264	21518	1.28%	0.243%
3	3.746	128	129	133	rBV3	5636	7996	0.47%	0.090%
4	3.840	142	145	152	rVB4	9040	15395	0.91%	0.174%
5	4.010	172	174	175	rBV2	3432	2597	0.15%	0.029%
6	4.946	331	333	336	rBV	2858	2319	0.14%	0.026%
7	6.045	518	520	525	rVB2	1792	2692	0.16%	0.030%
8	6.116	531	532	535	rBV	2016	2001	0.12%	0.023%
9	6.345	567	571	575	rBV6	2518	4308	0.26%	0.049%
10	7.204	715	717	723	rBV2	1911	2866	0.17%	0.032%
11	7.563	772	778	787	rBV	484060	745325	44.19%	8.427%
12	7.839	821	825	830	rBV5	1297	2048	0.12%	0.023%
13	8.181	877	883	888	rVB3	1155	2634	0.16%	0.030%
14	8.804	982	989	995	rBV2	10217	16024	0.95%	0.181%
15	10.333	1240	1249	1261	rBV	535504	902350	53.50%	10.203%
16	10.492	1271	1276	1280	rVB5	2126	2781	0.16%	0.031%
17	10.969	1355	1357	1360	rBV3	1326	1698	0.10%	0.019%
18	11.798	1493	1498	1501	rBV3	2112	3372	0.20%	0.038%
19	13.057	1708	1712	1717	rBV3	2972	4785	0.28%	0.054%
20	13.716	1823	1824	1829	rBV2	1786	1823	0.11%	0.021%
21	14.139	1891	1896	1901	rBV4	5210	6586	0.39%	0.074%
22	14.204	1901	1907	1917	rBV2	889384	1313810	77.90%	14.855%
23	15.092	2053	2058	2062	rBV4	4200	6670	0.40%	0.075%
24	15.486	2121	2125	2126	rBV	1893	2018	0.12%	0.023%
25	15.498	2126	2127	2131	rVB2	2112	2221	0.13%	0.025%
26	15.962	2201	2206	2207	rBV3	3959	4840	0.29%	0.055%
27	15.980	2207	2209	2214	rVB3	4536	5382	0.32%	0.061%
28	16.509	2296	2299	2301	rBV4	1314	1828	0.11%	0.021%
29	16.745	2335	2339	2344	rBV4	5517	8951	0.53%	0.101%
30	16.798	2344	2348	2353	rBV6	2555	4181	0.25%	0.047%
31	16.845	2353	2356	2358	rVB2	2099	1833	0.11%	0.021%
32	16.951	2366	2374	2388	rBV	1242224	1686490	100.00%	19.069%
33	17.045	2388	2390	2395	rVV2	3436	4720	0.28%	0.053%
34	17.139	2403	2406	2411	rVB5	3808	5498	0.33%	0.062%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
 Data File : BM027394.D
 Acq On : 11 Sep 2020 04:05
 Operator : JU/CG
 Sample : L3907-19
 Misc : GCMS CONFIRMATION
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET1A6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Title : SVOA CALIBRATION

35	17.415	2449	2453	2457	rVB8	2458	3323	0.20%	0.038%
36	17.492	2462	2466	2470	rVB6	3823	5752	0.34%	0.065%
37	17.562	2472	2478	2485	rBV3	32100	60006	3.56%	0.678%
38	17.680	2494	2498	2502	rVB5	2112	3179	0.19%	0.036%
39	17.809	2516	2520	2524	rBV2	11970	14911	0.88%	0.169%
40	17.868	2526	2530	2537	rVV4	17286	24871	1.47%	0.281%
41	18.033	2553	2558	2563	rVV2	49435	65279	3.87%	0.738%
42	18.092	2563	2568	2572	rVV	37629	45943	2.72%	0.519%
43	18.133	2572	2575	2579	rVV2	16327	19244	1.14%	0.218%
44	18.174	2579	2582	2586	rVB5	3164	3935	0.23%	0.044%
45	18.209	2586	2588	2590	rVB2	2261	1992	0.12%	0.023%
46	18.256	2594	2596	2598	rBV2	1695	1694	0.10%	0.019%
47	18.315	2602	2606	2611	rBV3	33425	42891	2.54%	0.485%
48	18.368	2611	2615	2619	rVB4	9701	12617	0.75%	0.143%
49	18.421	2621	2624	2628	rBV4	3564	5711	0.34%	0.065%
50	18.456	2628	2630	2633	rBV4	6158	7401	0.44%	0.084%
51	18.492	2633	2636	2642	rVB	24968	30485	1.81%	0.345%
52	18.598	2651	2654	2657	rBV4	3598	4591	0.27%	0.052%
53	18.751	2677	2680	2684	rBV4	2579	4109	0.24%	0.046%
54	18.809	2686	2690	2694	rVV3	28512	39027	2.31%	0.441%
55	18.856	2694	2698	2701	rVV2	29495	42075	2.49%	0.476%
56	18.898	2701	2705	2711	rVB2	69013	104942	6.22%	1.187%
57	18.974	2716	2718	2720	rVB2	4149	3367	0.20%	0.038%
58	19.109	2736	2741	2748	rBV7	23245	57953	3.44%	0.655%
59	19.174	2748	2752	2756	rVB2	51544	67988	4.03%	0.769%
60	19.239	2759	2763	2767	rVV3	19812	21747	1.29%	0.246%
61	19.433	2793	2796	2802	rVB7	11447	13743	0.81%	0.155%
62	19.509	2806	2809	2815	rVB5	18466	21760	1.29%	0.246%
63	19.562	2815	2818	2822	rBV6	7616	10143	0.60%	0.115%
64	19.621	2824	2828	2833	rVV2	42366	52557	3.12%	0.594%
65	19.745	2847	2849	2850	rBV2	4730	3998	0.24%	0.045%
66	19.762	2850	2852	2855	rVB4	6045	7014	0.42%	0.079%
67	19.886	2869	2873	2878	rBV8	18479	22700	1.35%	0.257%
68	19.933	2878	2881	2886	rBV3	43344	56444	3.35%	0.638%
69	20.168	2918	2921	2925	rBV5	17606	16437	0.97%	0.186%
70	20.215	2927	2929	2930	rBV2	9699	6416	0.38%	0.073%
71	20.245	2931	2934	2937	rVB5	16370	17801	1.06%	0.201%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027394.D
Acq On : 11 Sep 2020 04:05
Operator : JU/CG
Sample : L3907-19
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET1A6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Title : SVOA CALIBRATION

72	20.480	2972	2974	2980	rVB7	16558	21409	1.27%	0.242%
73	21.150	3083	3088	3098	rBV	1273773	1576454	93.48%	17.825%
74	22.697	3349	3351	3358	rVB3	77149	106786	6.33%	1.207%
75	23.315	3450	3456	3467	rBV	688094	1257017	74.53%	14.213%


Sum of corrected areas: 8843995

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027394.D
Acq On : 11 Sep 2020 04:05
Operator : JU/CG
Sample : L3907-19
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET1A6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

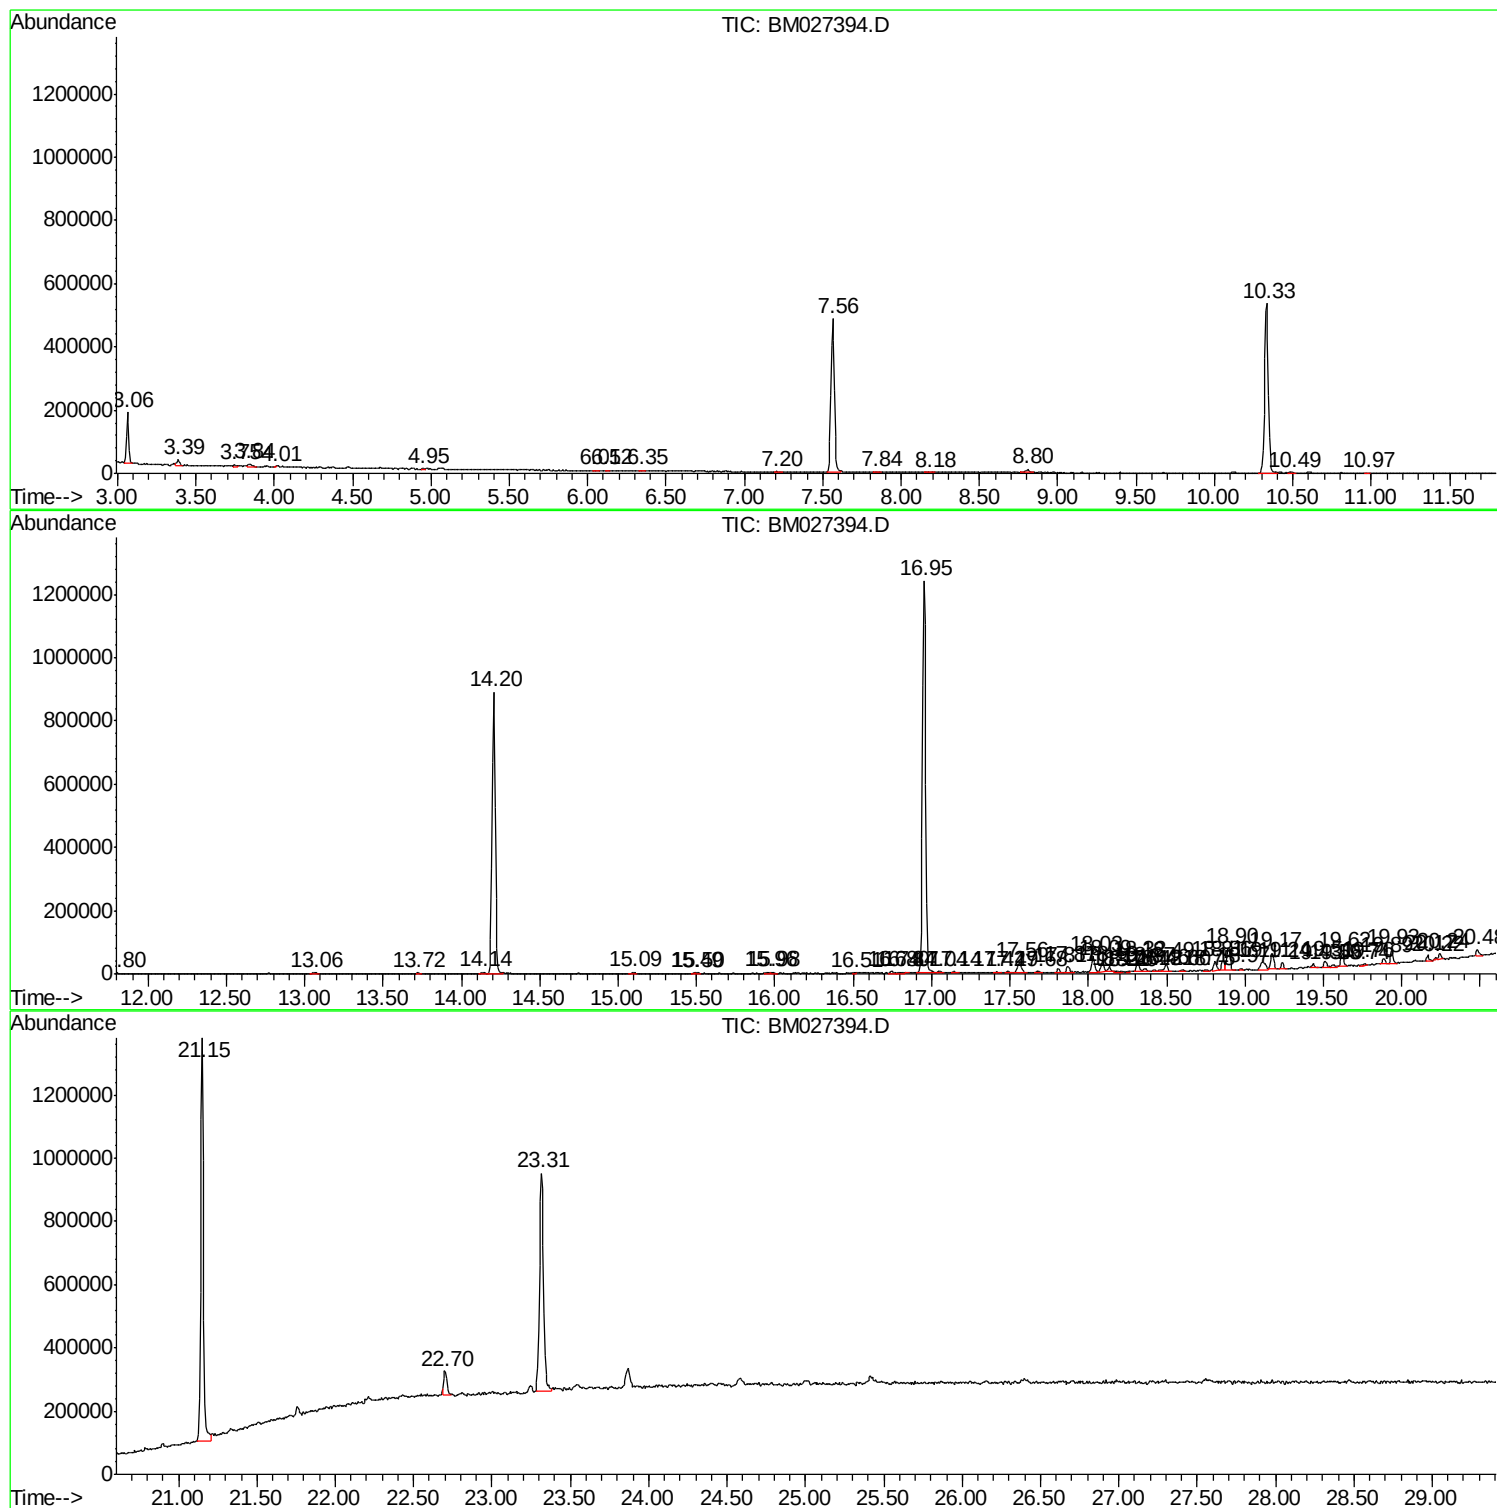

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091020\
Data File : BM027394.D
Acq On : 11 Sep 2020 04:05
Operator : JU/CG
Sample : L3907-19
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET1A6










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.06	4.26 ng/ul	158723	1,4-Dichlorobenzene-d4	7.56

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	72
2		n-Butyric acid 2-ethylhexyl ester	200	C12H24O2	025415-84-3	64
3		Hexane, 3-methyl-	100	C7H16	000589-34-4	53
4		Heptane	100	C7H16	000142-82-5	52
5		Butane, 2,2-dimethyl-	86	C6H14	000075-83-2	50

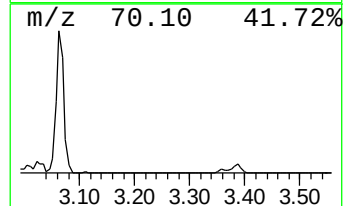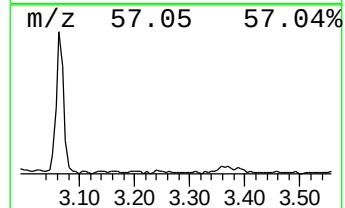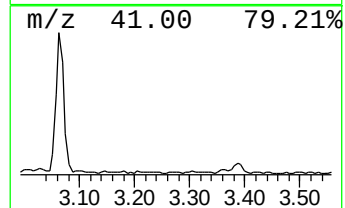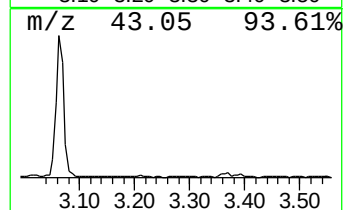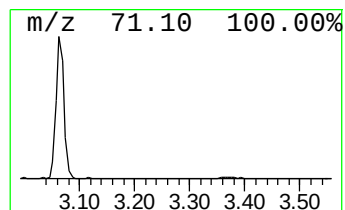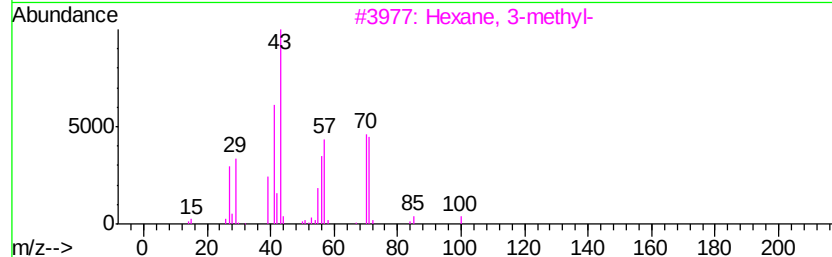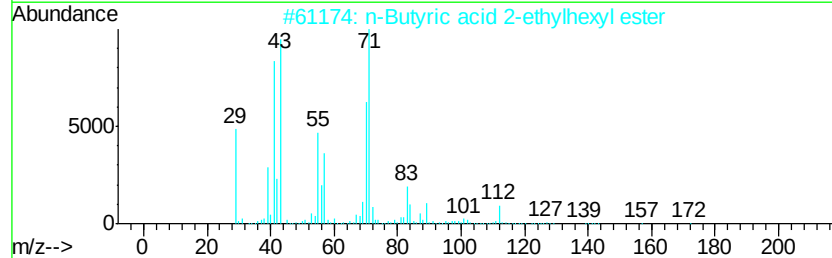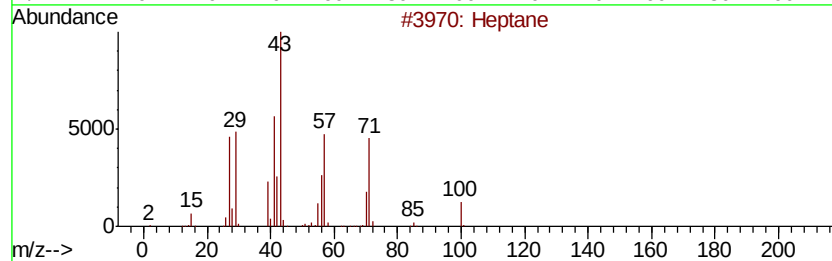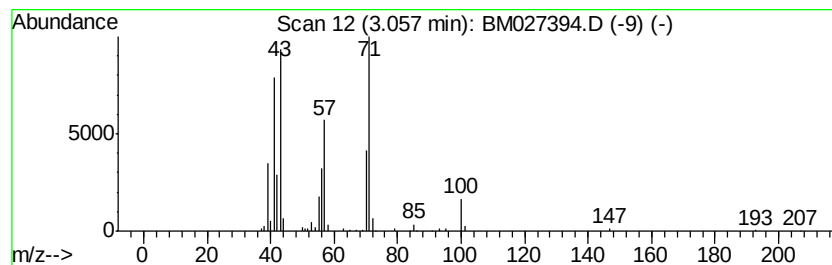

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091020\
Data File : BM027394.D
Acq On : 11 Sep 2020 04:05
Operator : JU/CG
Sample : L3907-19
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET1A6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.06	4.3	ng/ul	158723	1	7.56	745325	20.0