

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091115\
 Data File : BM002688.D
 Acq On : 11 Sep 2015 19:13
 Operator : UM/IZ
 Sample : MDL-07-W
 Misc :
 ALS Vial : 10 Sample Multiplier: 1


Quant Time: Sep 12 01:54:27 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 12 01:33:03 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	8113	0.40	ng/ul	0.00
4) Naphthalene-d8	11.64	136	30624	0.40	ng/ul	0.00
8) Acenaphthene-d10	15.36	164	13134	0.40	ng/ul	0.00
12) Phenanthrene-d10	18.08	188	24619	0.40	ng/ul	0.01
18) Chrysene-d12	22.16	240	22105	0.40	ng/ul	0.00
22) Perylene-d12	24.78	264	21469	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
6) 2-Methylnaphthalene-d10	13.17	152	14047	0.34	ng/ul	0.00
16) Fluoranthene-d10	20.04	212	19728	0.35	ng/ul	0.00
Target Compounds						
13) Pentachlorophenol	17.74	266	201	0.08	ng/ul	Qvalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091115\
Data File : BM002688.D
Acq On : 11 Sep 2015 19:13
Operator : UM/IZ
Sample : MDL-07-W
Misc :
ALS Vial : 10 Sample Multiplier: 1


Quant Time: Sep 12 01:54:27 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 12 01:33:03 2015
Response via : Initial Calibration

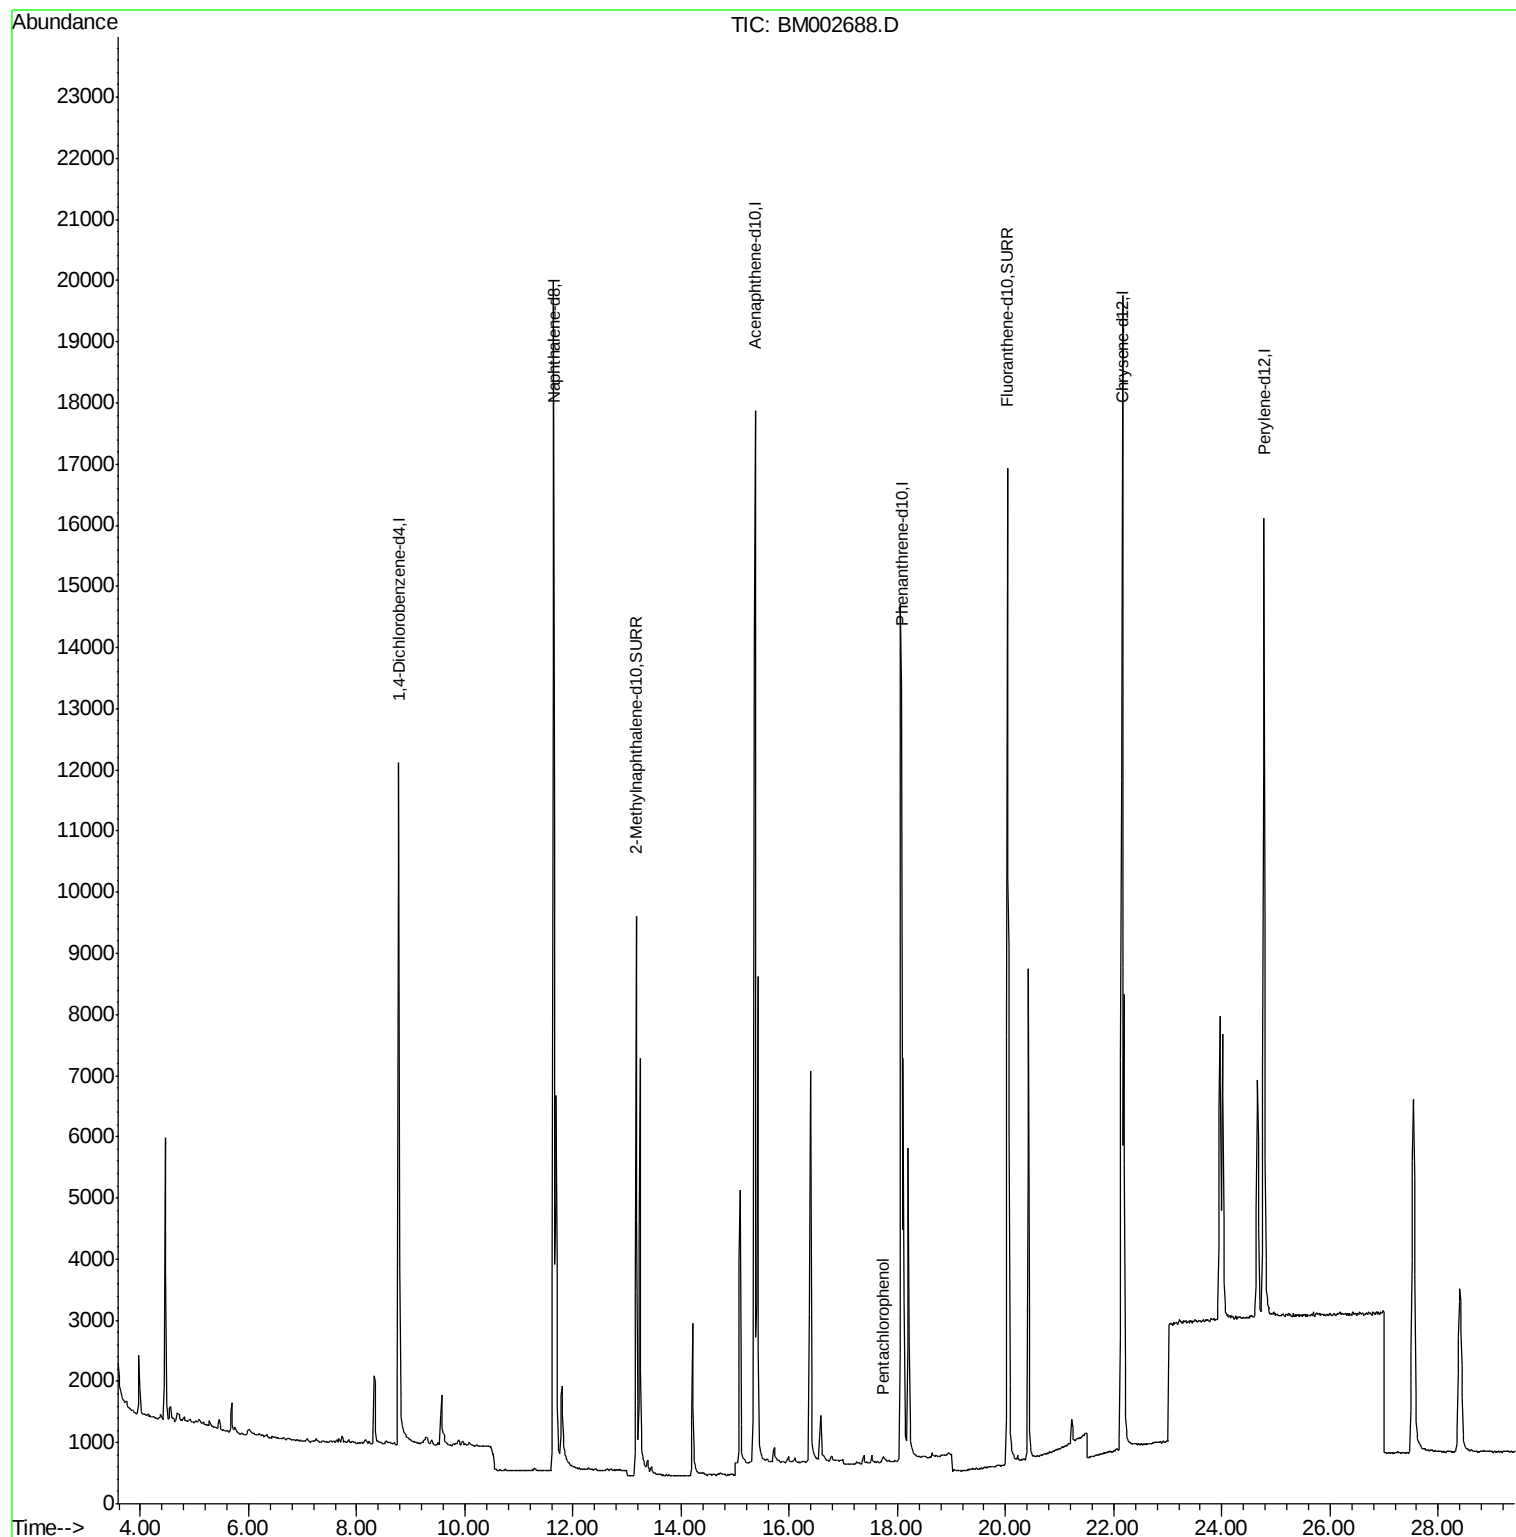

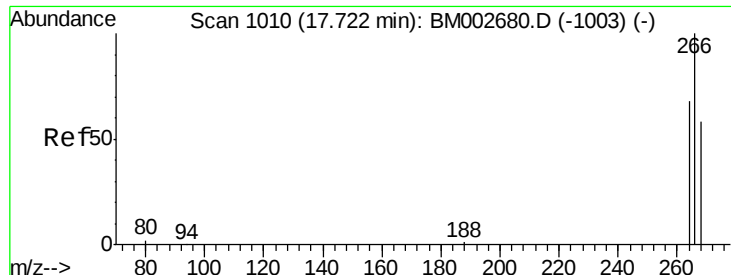

#13
 Pentachlorophenol
 Concen: 0.08 ng/ul
 RT: 17.74 min Scan# 1011
 Delta R.T. 0.01 min
 Lab File: BM002688.D
 Acq: 11 Sep 2015 19:13

Tgt Ion:	266	Resp:	201
Ion	Ratio	Lower	Upper
266	100		
264	74.1	53.5	80.3
268	59.2	54.2	81.2

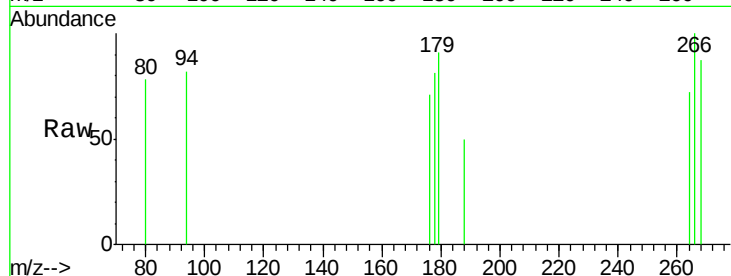

Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

