

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
 Data File : BM047492.D
 Acq On : 11 Sep 2024 21:56
 Operator : RC/JU
 Sample : P3878-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DDC49

Quant Time: Sep 12 02:39:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 11 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.869	152	589394	20.000	ng/u1	0.00
20) Naphthalene-d8	10.663	136	2653515	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.498	164	1708700	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.233	188	3469785	20.000	ng/u1	0.00
79) Chrysene-d12	21.456	240	2847140	20.000	ng/u1	-0.01
88) Perylene-d12	24.503	264	2567835	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	38571	2.639	ng/uL	0.00
4) Pyridine-d5	3.710	84	649530	13.911	ng/u1	0.00
7) Phenol-d5	7.022	99	773080	13.993	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.192	67	485722	14.124	ng/u1	0.00
11) 2-Chlorophenol-d4	7.398	132	636221	15.120	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	652509	15.026	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	315478	15.395	ng/u1	0.00
24) 2-Nitrophenol-d4	9.739	143	314643	16.253	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.280	165	613897	15.596	ng/u1	0.00
31) 4-Chloroaniline-d4	10.792	131	985757	15.301	ng/u1	0.00
46) Dimethylphthalate-d6	13.904	166	2110281	16.803	ng/u1	0.00
49) Acenaphthylene-d8	14.186	160	2415817	15.941	ng/u1	0.00
54) 4-Nitrophenol-d4	14.668	143	277859	11.166	ng/u1	0.00
60) Fluorene-d10	15.486	176	1823158	16.799	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.586	200	88505	4.825	ng/u1	-0.01
73) Anthracene-d10	17.327	188	2902996	17.374	ng/u1	0.00
81) Pyrene-d10	19.609	212	3175302	19.136	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.291	264	2404766	17.623	ng/u1	-0.02
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.880	266	42288	1.638	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
Data File : BM047492.D
Acq On : 11 Sep 2024 21:56
Operator : RC/JU
Sample : P3878-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DDC49

Quant Time: Sep 12 02:39:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 11 00:35:12 2024
Response via : Initial Calibration

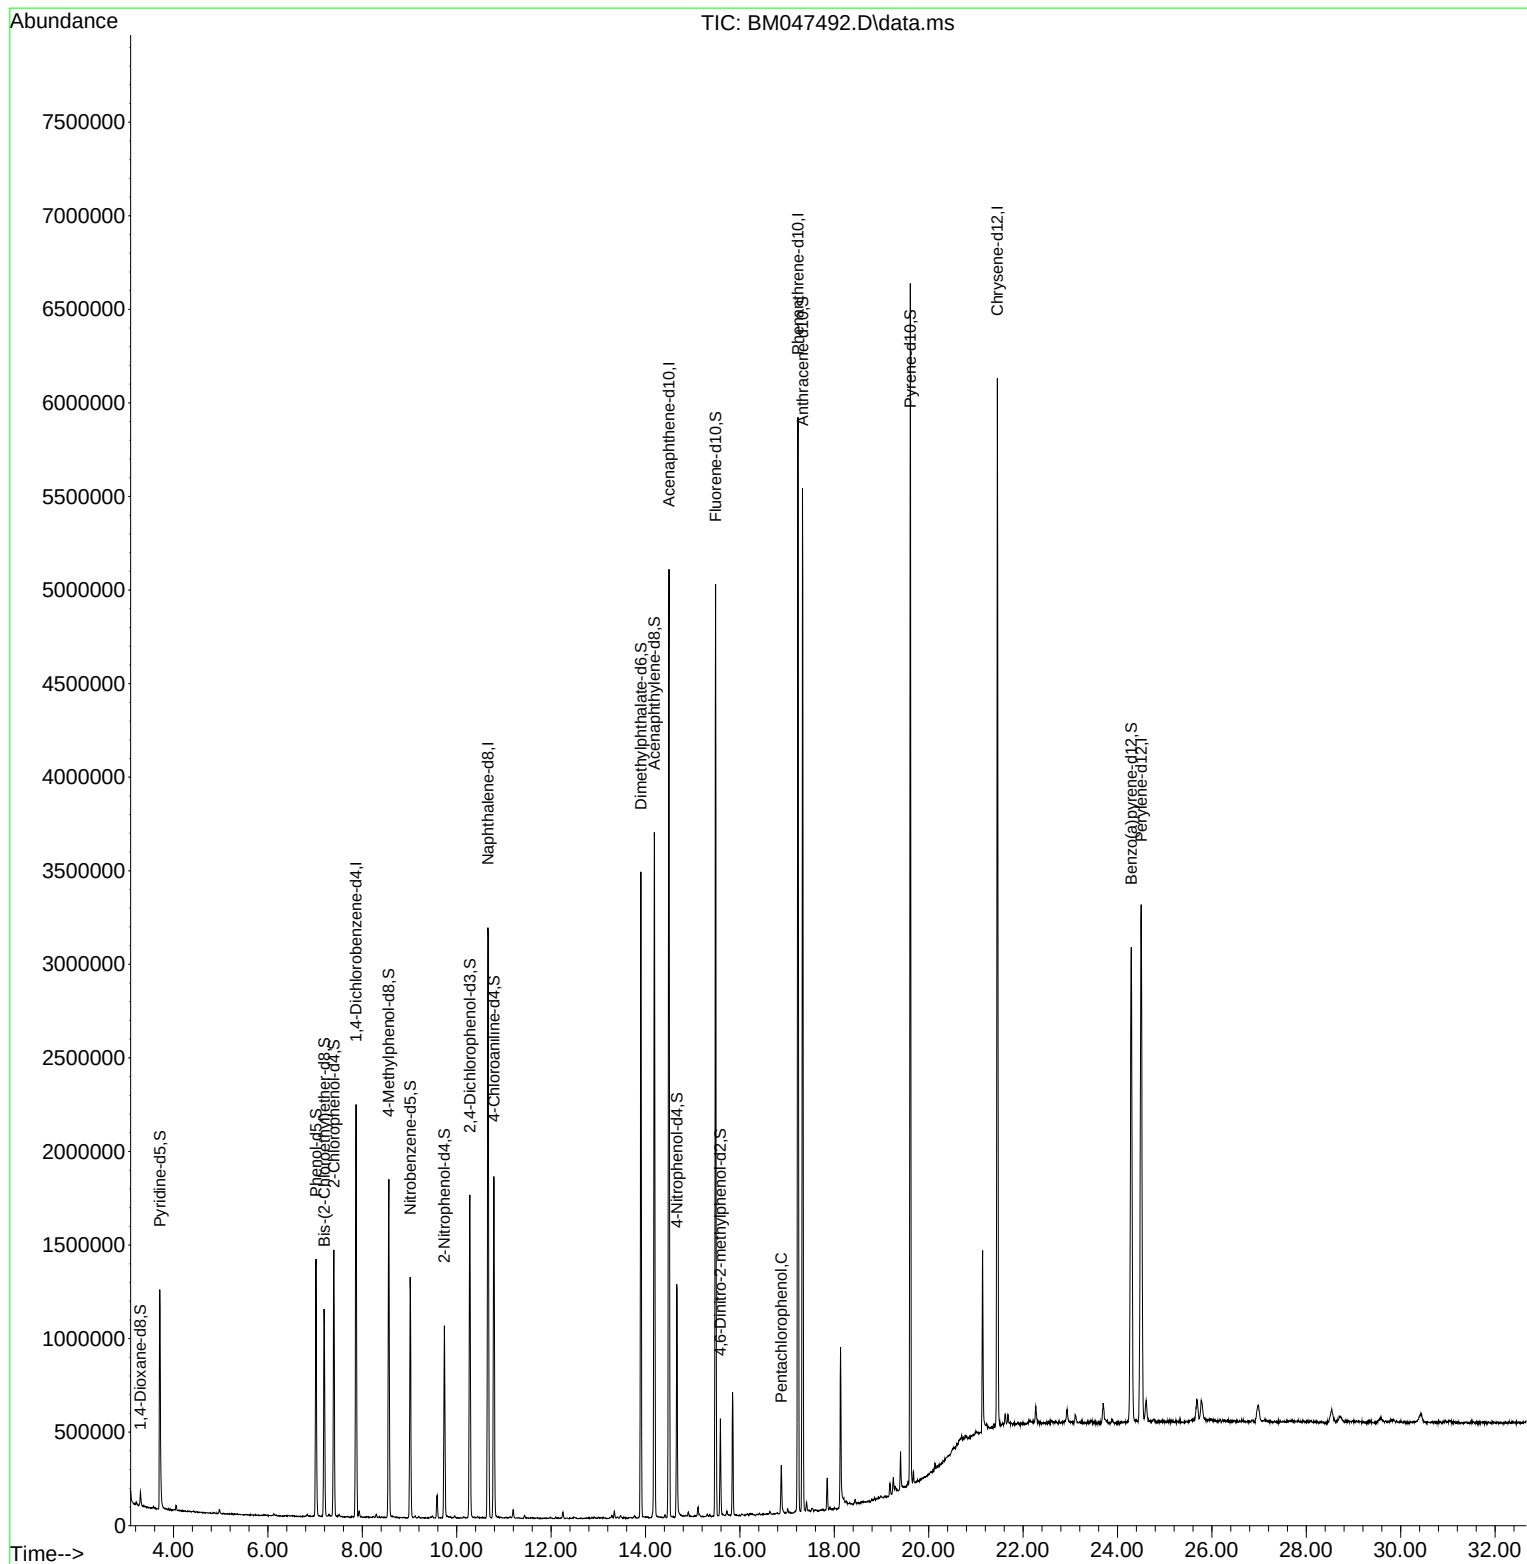

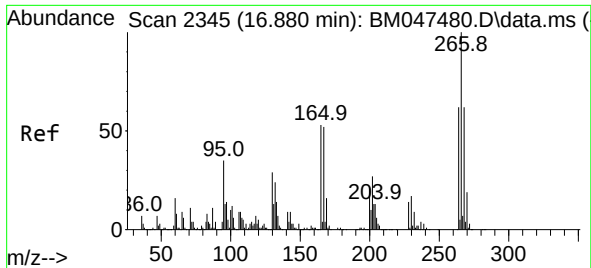

#71
 Pentachlorophenol
 Concen: 1.638 ng/ul
 RT: 16.880 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM047492.D
 Acq: 11 Sep 2024 21:56

Instrument :
 BNA_M
 ClientSampleId :
 DDC49

Tgt Ion:266 Resp: 42288
 Ion Ratio Lower Upper
 266 100
 264 64.3 49.5 74.3
 268 63.8 51.0 76.4

