

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
 Data File : BM047479.D
 Acq On : 11 Sep 2024 13:10
 Operator : RC/JU
 Sample : PB163275BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK275

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	16	rVB2	24265	37584	0.41%	0.037%
2	3.305	33	37	42	rVB	113888	149140	1.63%	0.148%
3	3.710	102	106	120	rBV	1562648	2236671	24.47%	2.222%
4	4.057	161	165	170	rBV	30707	41154	0.45%	0.041%
5	7.022	661	669	679	rBV	1688267	2641672	28.90%	2.624%
6	7.198	690	699	709	rBV	1405141	2211466	24.19%	2.197%
7	7.398	726	733	744	rBV	1693543	2635511	28.83%	2.618%
8	7.869	805	813	821	rVB	1520234	2401470	26.27%	2.386%
9	8.563	923	931	940	rBV	2082150	3250472	35.56%	3.229%
10	9.022	1000	1009	1019	rBV	1596010	2671041	29.22%	2.654%
11	9.745	1125	1132	1143	rBV	1203728	1980032	21.66%	1.967%
12	10.281	1214	1223	1234	rBV	1930690	3164409	34.62%	3.144%
13	10.669	1280	1289	1299	rBV	2199678	3638810	39.80%	3.615%
14	10.792	1302	1310	1319	rBV	1988420	3326212	36.39%	3.304%
15	11.439	1415	1420	1425	rVB8	10174	18512	0.20%	0.018%
16	12.251	1552	1558	1564	rVB	34305	61926	0.68%	0.062%
17	13.904	1833	1839	1848	rBV	3693834	5101362	55.80%	5.068%
18	14.192	1880	1888	1897	rBV	4424295	6197874	67.80%	6.157%
19	14.498	1933	1940	1948	rBV	3438530	4900420	53.61%	4.868%
20	14.563	1948	1951	1956	rVB6	8244	11510	0.13%	0.011%
21	14.669	1961	1969	1979	rBV	1866376	2693292	29.46%	2.676%
22	14.910	2004	2010	2013	rVB6	8859	17059	0.19%	0.017%
23	15.486	2101	2108	2116	rBV	5297481	7521912	82.28%	7.473%
24	15.592	2119	2126	2142	rVV	1454389	2046327	22.38%	2.033%
25	15.727	2144	2149	2158	rVB5	23125	47187	0.52%	0.047%
26	15.851	2165	2170	2174	rBV8	5485	10497	0.11%	0.010%
27	15.998	2192	2195	2199	rVB6	7723	9906	0.11%	0.010%
28	16.268	2238	2241	2247	rVB5	17923	23690	0.26%	0.024%
29	16.915	2348	2351	2354	rVB4	6966	9200	0.10%	0.009%
30	17.233	2398	2405	2413	rBV	4120327	5590886	61.16%	5.554%
31	17.333	2415	2422	2433	rBV	6037922	8258551	90.34%	8.205%
32	19.180	2733	2736	2741	rVB5	61612	79638	0.87%	0.079%
33	19.251	2745	2748	2752	rVB	51429	71287	0.78%	0.071%
34	19.615	2804	2810	2819	rBV	7247730	9141597	100.00%	9.082%
35	21.462	3118	3124	3135	rVB	3885229	5497661	60.14%	5.462%
36	24.303	3598	3607	3622	rVB2	3321808	7870736	86.10%	7.819%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
Data File : BM047479.D
Acq On : 11 Sep 2024 13:10
Operator : RC/JU
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK275

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Title : SVOA CALIBRATION

37	24.509	3634	3642	3655	rVB	2080855	5091040	55.69%	5.058%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 100657714

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
Data File : BM047479.D
Acq On : 11 Sep 2024 13:10
Operator : RC/JU
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

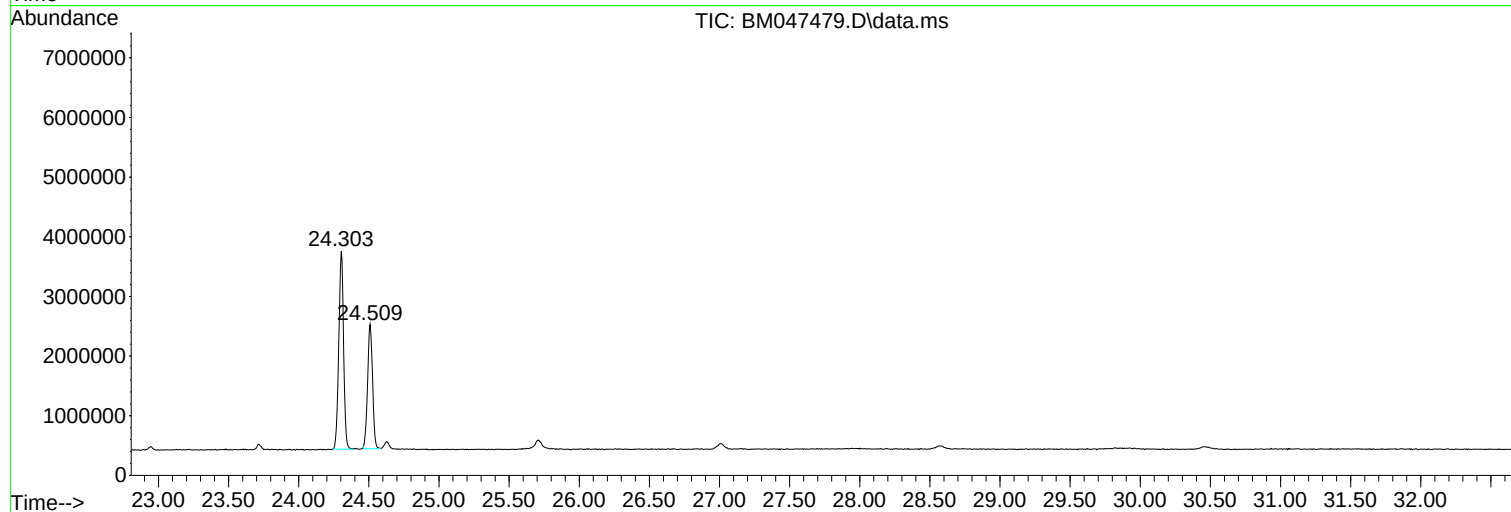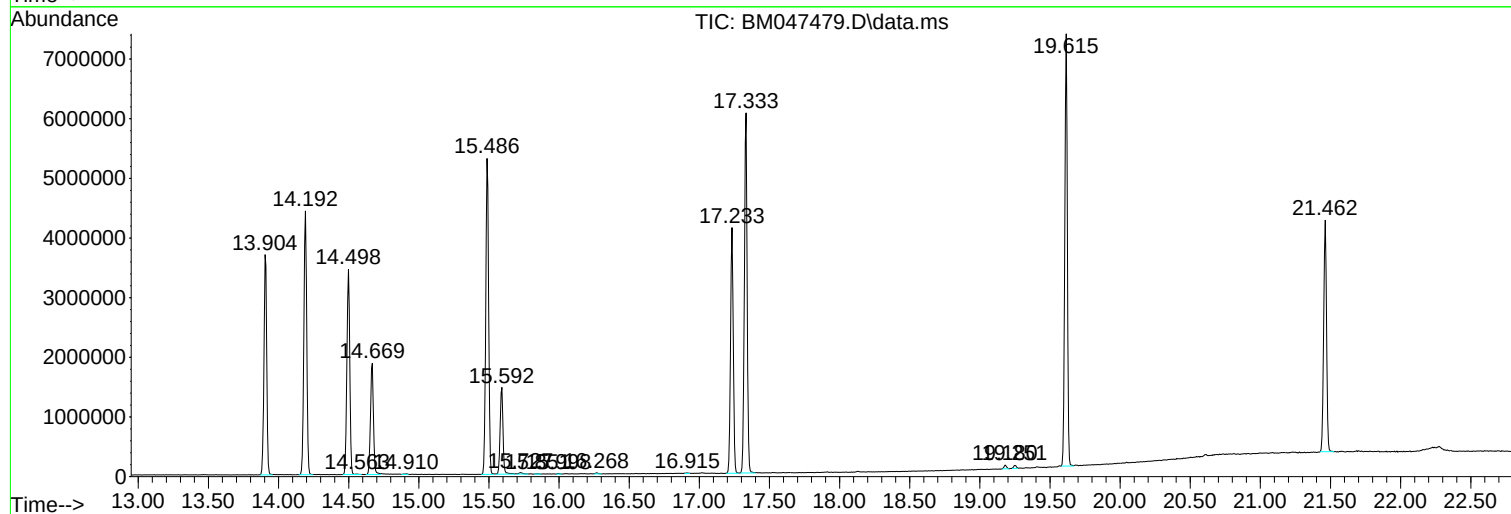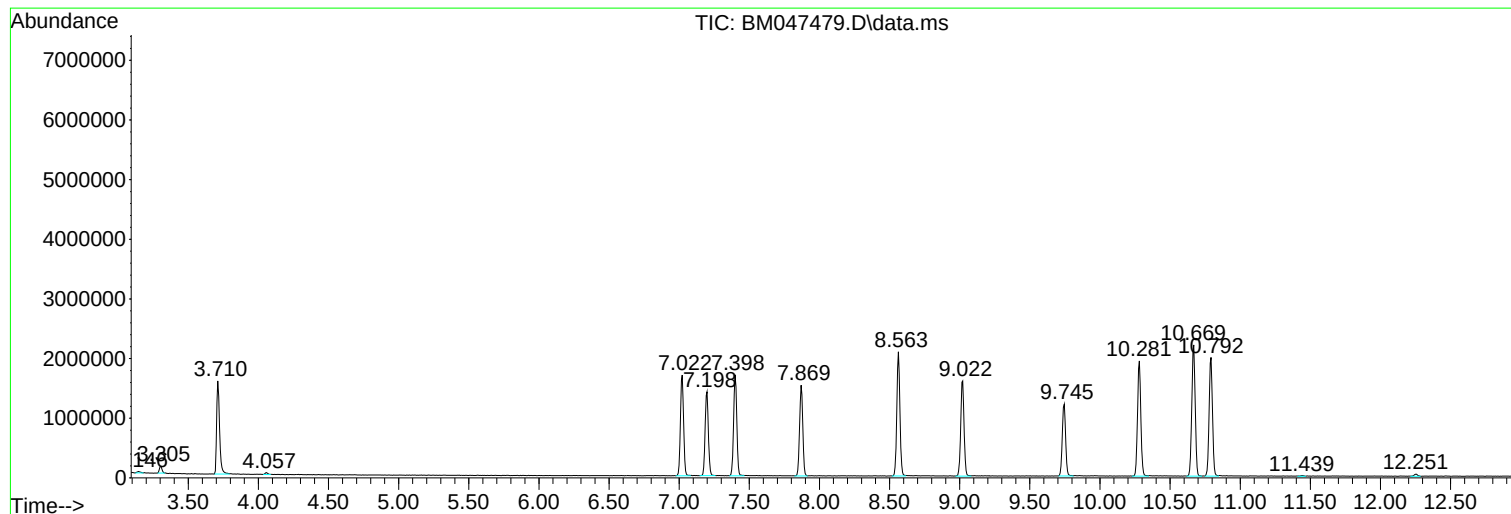

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
Data File : BM047479.D
Acq On : 11 Sep 2024 13:10
Operator : RC/JU
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091124\
Data File : BM047479.D
Acq On : 11 Sep 2024 13:10
Operator : RC/JU
Sample : PB163275BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK275

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc