

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM091217\
 Data File : BM011524.D
 Acq On : 12 Sep 2017 18:59
 Operator : SJ/JU
 Sample : I5145-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG0

Quant Time: Sep 13 08:07:35 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 13 07:51:23 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	566709	20.00	ng/ul	0.00
18) Naphthalene-d8	10.78	136	2619272	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	1515666	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.34	188	3360782	20.00	ng/ul	0.00
78) Chrysene-d12	21.51	240	3433379	20.00	ng/ul	0.00
86) Perylene-d12	23.88	264	2843335	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.39	96	44678	3.55	ng/uL	0.00
5) Phenol-d5	7.12	99	326876	6.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.30	67	914582	24.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.50	132	869995	21.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.67	113	615520	14.49	ng/ul	0.00
19) Nitrobenzene-d5	9.14	128	517510	26.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.86	143	549625	26.59	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.40	165	1082849	26.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	1255	0.03	ng/ul	0.01
44) Dimethylphthalate-d6	14.01	166	3774322	29.46	ng/ul	0.00
47) Acenaphthylene-d8	14.30	160	4353859	28.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.79	143	113194	4.70	ng/ul	0.00
58) Fluorene-d10	15.59	176	3250662	29.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.70	200	488767	24.99	ng/ul	0.00
71) Anthracene-d10	17.44	188	5025670	30.37	ng/ul	0.00
79) Pyrene-d10	19.73	212	5623404	34.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.73	264	4208266	31.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
57) Diethylphthalate	15.41	149	181453	1.421	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM091217\
Data File : BM011524.D
Acq On : 12 Sep 2017 18:59
Operator : SJ/JU
Sample : I5145-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG0

Quant Time: Sep 13 08:07:35 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 13 07:51:23 2017
Response via : Initial Calibration

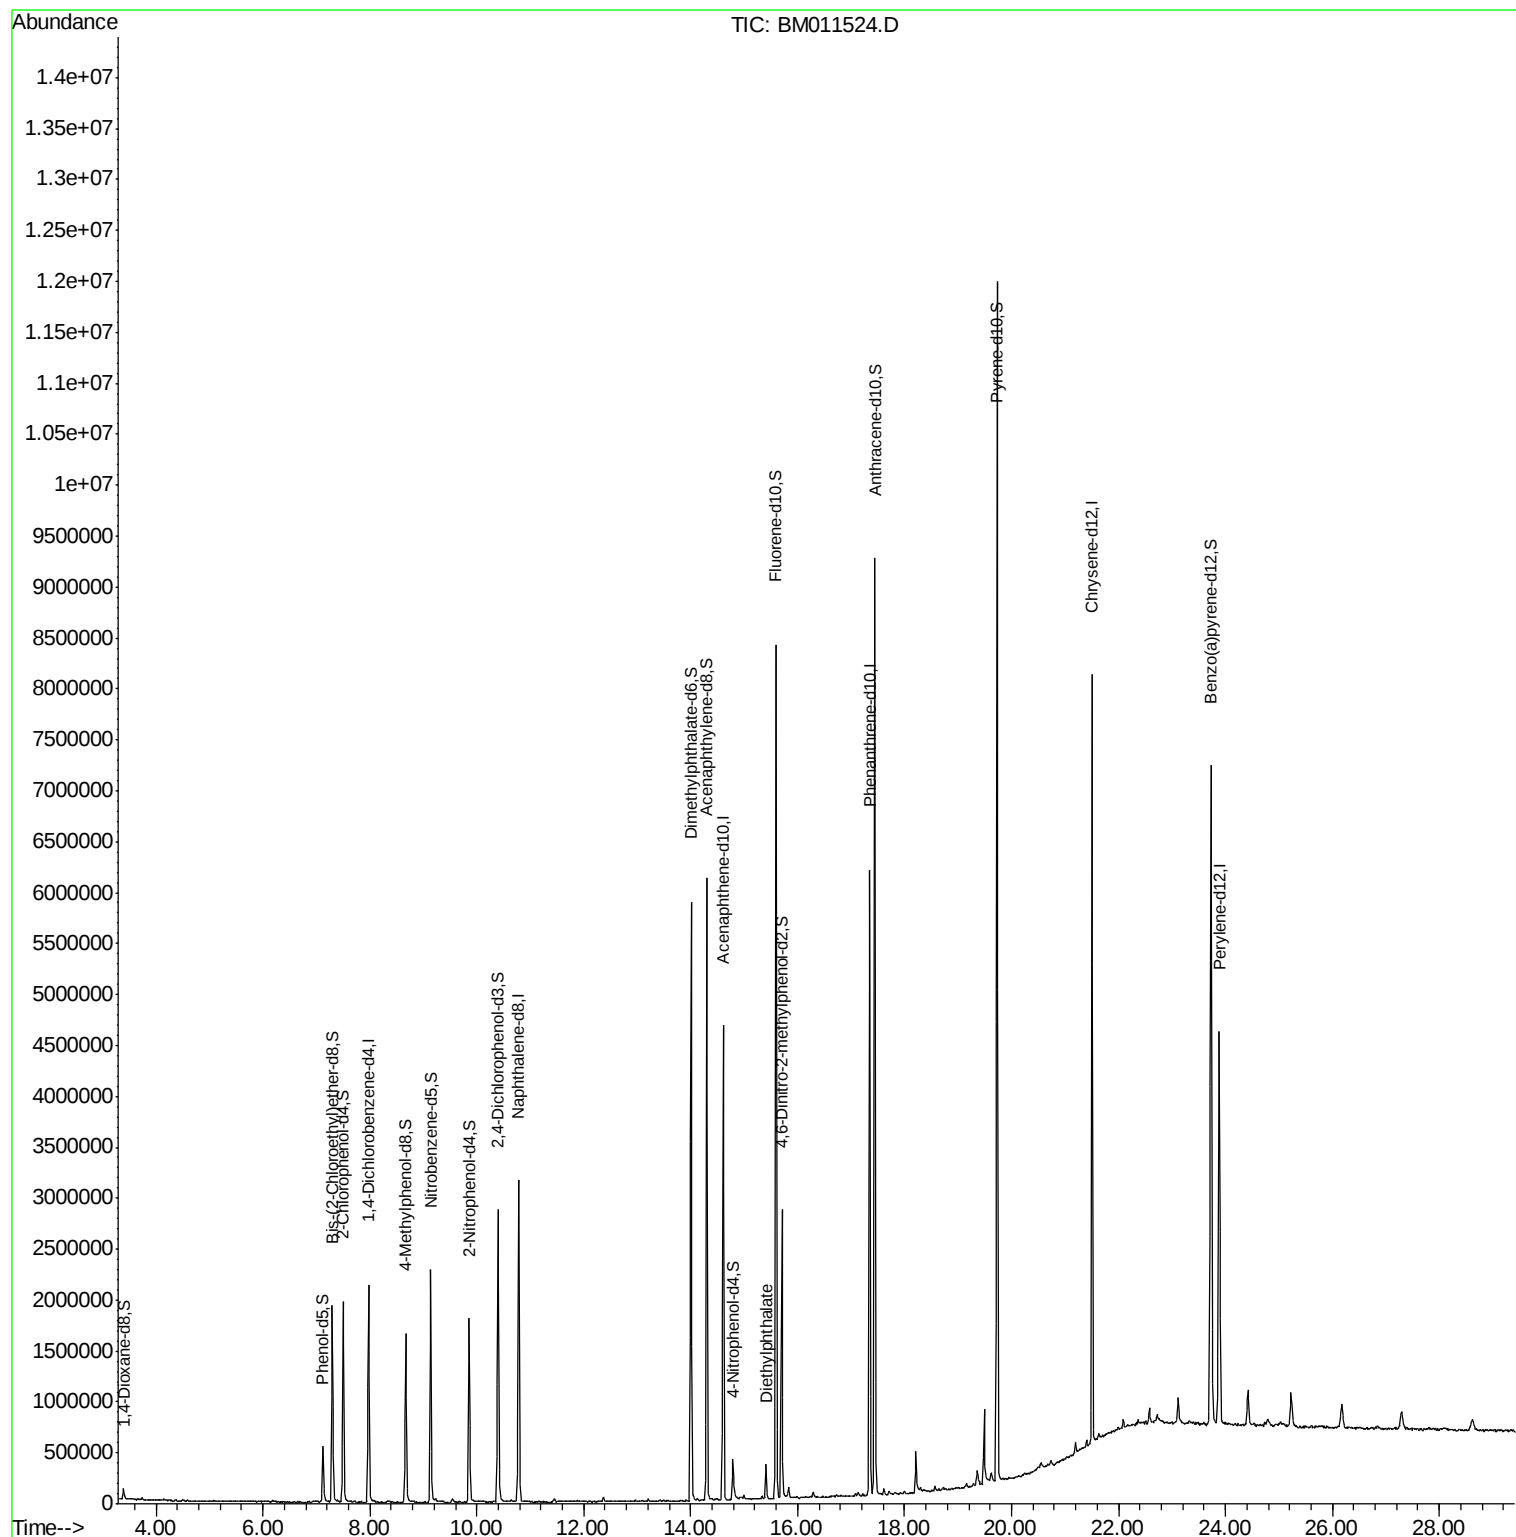


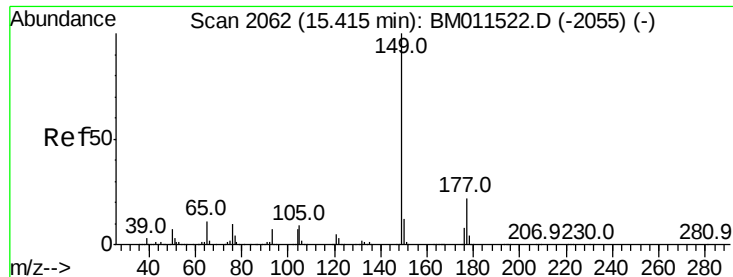

#57
 Diethylphthalate
 Concen: 1.421 ng/ul
 RT: 15.41 min Scan# 2061
 Delta R.T. -0.01 min
 Lab File: BM011524.D
 Acq: 12 Sep 2017 18:59

Instrument :
 BNA_M
 ClientSampleId :
 C0AG0

Tot Ion	Ratio	Lower	Upper
149	100		
177	20.4	19.3	28.9
150	10.8	10.6	15.8

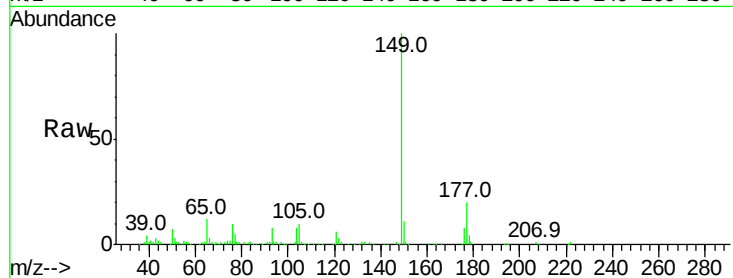

Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E

