

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
 Data File : BM047511.D
 Acq On : 13 Sep 2024 09:29
 Operator : RC/JU
 Sample : PB163349BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	45	rVB	114671	158084	1.92%	0.170%
2	3.710	101	106	118	rBV	1462071	2190622	26.62%	2.360%
3	4.052	161	164	171	rVB	26496	40405	0.49%	0.044%
4	7.016	661	668	679	rBV	1689439	2598794	31.58%	2.800%
5	7.193	691	698	708	rVB	1386635	2158613	26.23%	2.326%
6	7.393	725	732	741	rBV	1640454	2583119	31.39%	2.783%
7	7.863	805	812	820	rBV	1538053	2412840	29.32%	2.600%
8	8.557	922	930	942	rBV	2006108	3262563	39.64%	3.516%
9	9.016	1000	1008	1019	rBV	1579357	2616374	31.79%	2.819%
10	9.739	1123	1131	1140	rBV	1162987	1904622	23.14%	2.052%
11	10.275	1214	1222	1232	rBV	2030804	3258189	39.59%	3.511%
12	10.657	1280	1287	1299	rVB	2185918	3695396	44.90%	3.982%
13	10.787	1299	1309	1321	rBV	1983882	3355275	40.77%	3.615%
14	11.439	1415	1420	1423	rBV7	5895	10442	0.13%	0.011%
15	12.245	1550	1557	1564	rBV2	35505	57788	0.70%	0.062%
16	13.469	1759	1765	1769	rBV3	6644	10162	0.12%	0.011%
17	13.898	1831	1838	1853	rBV	3660029	4821480	58.59%	5.195%
18	14.186	1879	1887	1897	rBV	4127273	6081567	73.90%	6.553%
19	14.492	1932	1939	1947	rBV	3524818	4964324	60.32%	5.349%
20	14.663	1961	1968	1980	rBV	1563417	2192355	26.64%	2.362%
21	14.904	2004	2009	2012	rVB6	8030	10412	0.13%	0.011%
22	15.480	2100	2107	2115	rBV	5305944	7271921	88.36%	7.836%
23	15.586	2118	2125	2139	rVV	1058082	1507650	18.32%	1.625%
24	15.716	2143	2147	2153	rVB6	24402	43676	0.53%	0.047%
25	15.986	2189	2193	2197	rVB7	6681	11209	0.14%	0.012%
26	16.045	2197	2203	2205	rBV6	7331	10286	0.12%	0.011%
27	16.263	2235	2240	2243	rBV6	16276	24127	0.29%	0.026%
28	16.904	2347	2349	2354	rVB6	8363	11115	0.14%	0.012%
29	17.010	2362	2367	2370	rBV2	9183	12951	0.16%	0.014%
30	17.227	2396	2404	2410	rBV	3971769	5477301	66.56%	5.902%
31	17.321	2414	2420	2432	rVB	5475912	7678566	93.31%	8.274%
32	17.904	2516	2519	2522	rVB5	8199	10459	0.13%	0.011%
33	19.174	2731	2735	2739	rBV2	58743	74046	0.90%	0.080%
34	19.245	2743	2747	2751	rVB	46482	63717	0.77%	0.069%
35	19.609	2802	2809	2818	rBV	6289689	8229523	100.00%	8.868%
36	21.451	3116	3122	3132	rBV	3125959	4452989	54.11%	4.798%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047511.D
Acq On : 13 Sep 2024 09:29
Operator : RC/JU
Sample : PB163349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK349

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Title : SVOA CALIBRATION

37	24.280	3594	3603	3615	rBV2	2346928	5683133	69.06%	6.124%
38	24.486	3630	3638	3649	rVB2	1559365	3857893	46.88%	4.157%


Sum of corrected areas: 92803988

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047511.D
Acq On : 13 Sep 2024 09:29
Operator : RC/JU
Sample : PB163349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

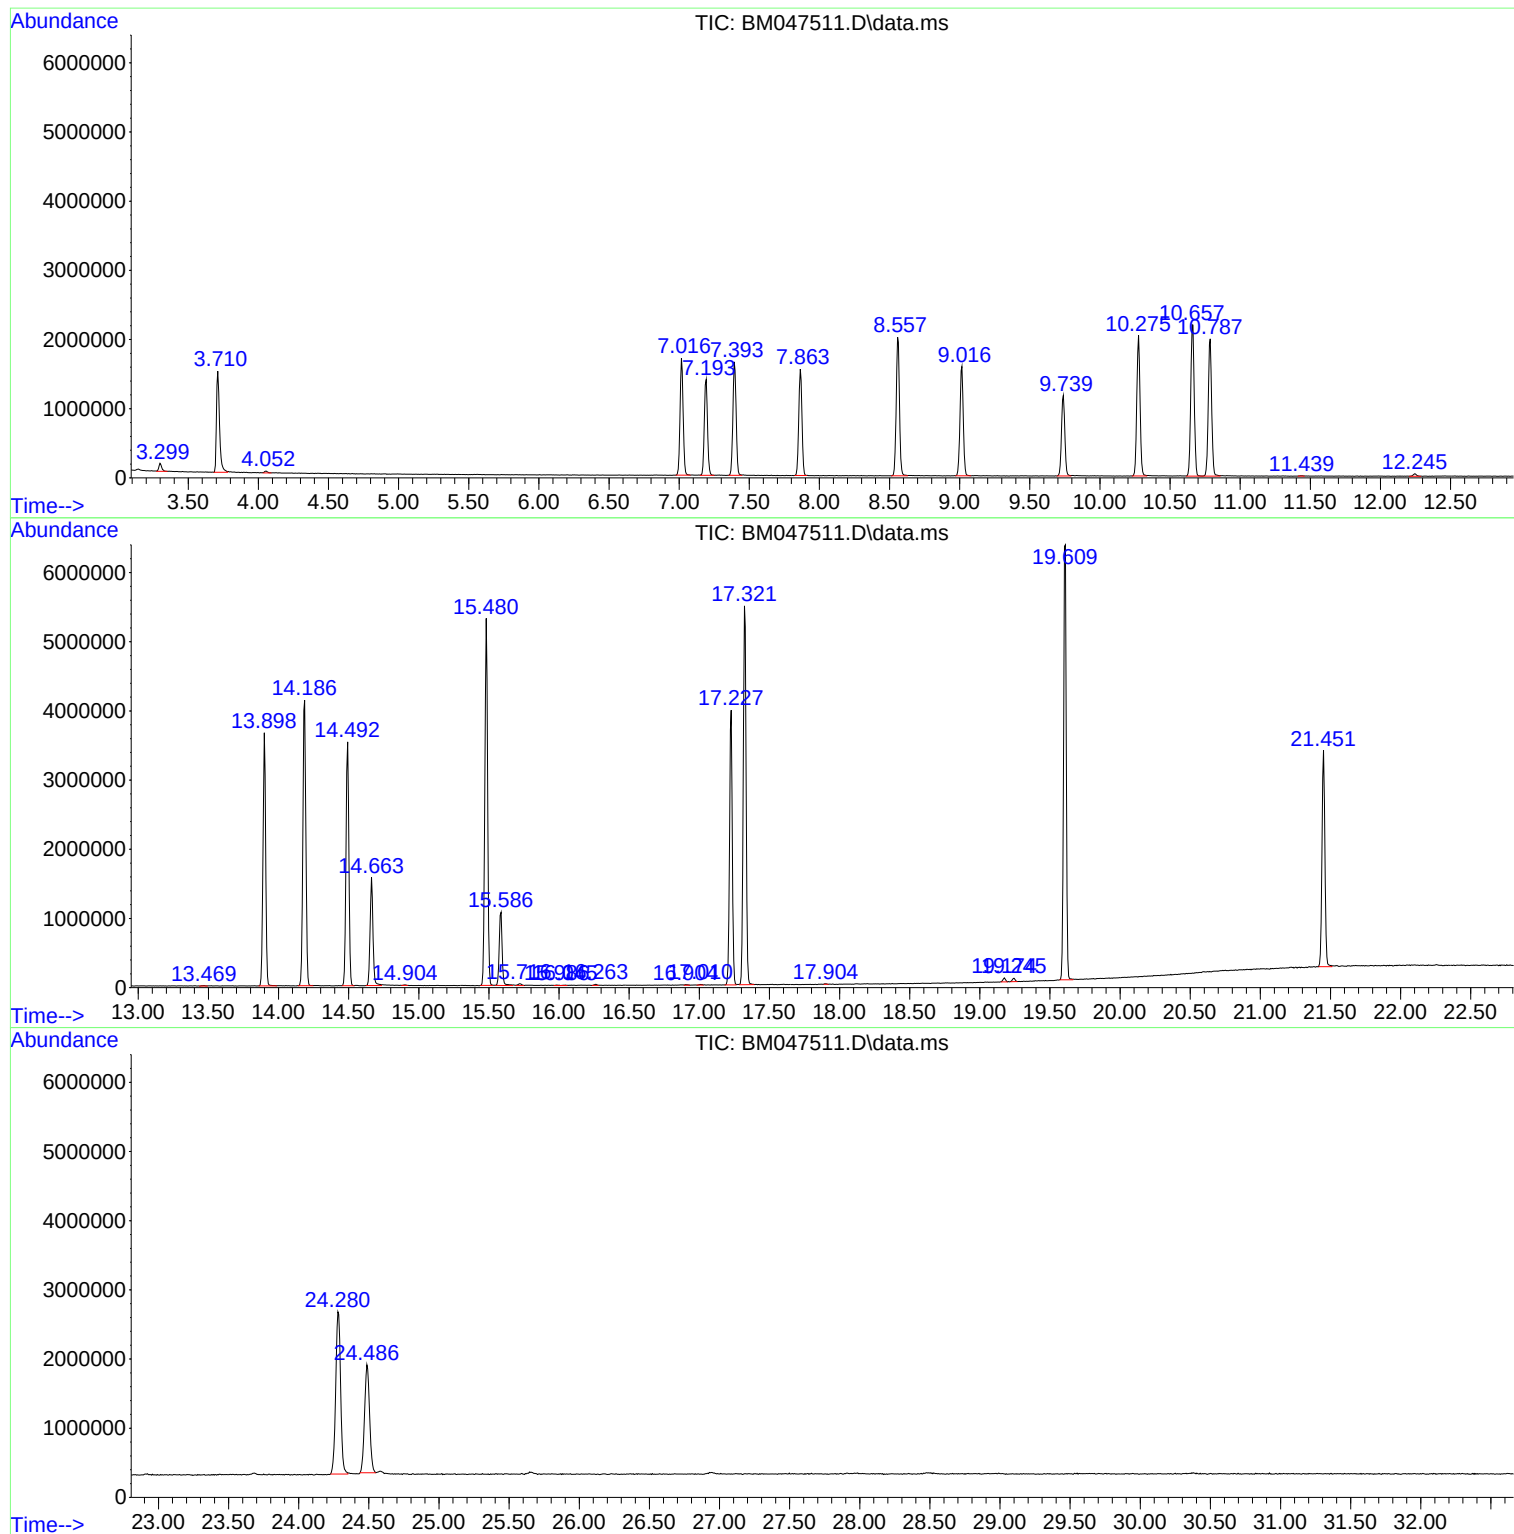

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047511.D
Acq On : 13 Sep 2024 09:29
Operator : RC/JU
Sample : PB163349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047511.D
Acq On : 13 Sep 2024 09:29
Operator : RC/JU
Sample : PB163349BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------