

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
 Data File : BM047515.D
 Acq On : 13 Sep 2024 12:12
 Operator : RC/JU
 Sample : P3952-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	34	rBV2	75128	108360	1.13%	0.129%
2	3.299	34	36	40	rVB	86931	101040	1.06%	0.121%
3	3.716	103	107	115	rBV	282134	452578	4.73%	0.540%
4	4.057	161	165	170	rVB3	18197	28202	0.29%	0.034%
5	4.269	199	201	205	rVB4	12720	14490	0.15%	0.017%
6	4.587	250	255	266	rVB3	139701	245601	2.57%	0.293%
7	4.857	298	301	306	rVB5	12043	16050	0.17%	0.019%
8	4.975	316	321	327	rVB3	51007	76570	0.80%	0.091%
9	6.122	511	516	521	rVB5	18905	28499	0.30%	0.034%
10	7.016	662	668	676	rBV	402711	636076	6.65%	0.759%
11	7.192	691	698	708	rVB	1299584	2050250	21.44%	2.447%
12	7.392	725	732	743	rBV	1433676	2220076	23.21%	2.649%
13	7.504	746	751	758	rVB5	11676	23617	0.25%	0.028%
14	7.863	805	812	820	rBV	1252001	1963489	20.53%	2.343%
15	7.939	820	825	829	rVB4	8058	14458	0.15%	0.017%
16	8.239	870	876	879	rBV6	5790	10545	0.11%	0.013%
17	8.357	892	896	902	rBV8	6414	11298	0.12%	0.013%
18	8.557	922	930	941	rBV	1154841	1838623	19.22%	2.194%
19	9.016	999	1008	1018	rBV	1514389	2482833	25.96%	2.963%
20	9.739	1120	1131	1139	rBV	1100737	1800175	18.82%	2.148%
21	10.275	1214	1222	1233	rBV	1889327	3045723	31.85%	3.635%
22	10.663	1280	1288	1295	rBV	1757819	3005178	31.42%	3.586%
23	10.786	1299	1309	1321	rBV	1522118	2642982	27.63%	3.154%
24	11.392	1408	1412	1417	rBV2	9587	16947	0.18%	0.020%
25	12.245	1551	1557	1562	rVB4	29328	50754	0.53%	0.061%
26	13.898	1831	1838	1851	rBV	3511054	4765366	49.83%	5.687%
27	14.186	1875	1887	1894	rBV	3792695	5732402	59.94%	6.841%
28	14.492	1931	1939	1946	rBV	2782861	3986218	41.68%	4.757%
29	14.557	1946	1950	1955	rVB6	11021	18911	0.20%	0.023%
30	14.663	1962	1968	1974	rBV	335465	492358	5.15%	0.588%
31	14.898	2003	2008	2013	rBV7	21321	31730	0.33%	0.038%
32	15.304	2070	2077	2082	rBV6	12829	23787	0.25%	0.028%
33	15.480	2100	2107	2114	rBV	5408930	7281486	76.13%	8.689%
34	15.586	2119	2125	2140	rVV	1272638	1767295	18.48%	2.109%
35	15.721	2143	2148	2153	rVB3	22505	36906	0.39%	0.044%
36	16.045	2199	2203	2206	rVB5	8132	12171	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
 Data File : BM047515.D
 Acq On : 13 Sep 2024 12:12
 Operator : RC/JU
 Sample : P3952-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
 Title : SVOA CALIBRATION

37	16.874	2340	2344	2347	rBV4	9580	16585	0.17%	0.020%
38	16.904	2347	2349	2353	rVV4	8417	10241	0.11%	0.012%
39	17.015	2361	2368	2371	rBV6	9856	20410	0.21%	0.024%
40	17.227	2393	2404	2409	rBV	3096661	4389335	45.89%	5.238%
41	17.268	2409	2411	2414	rVV	73914	79064	0.83%	0.094%
42	17.321	2414	2420	2431	rVB	5890518	8284288	86.62%	9.886%
43	17.592	2462	2466	2469	rBV4	10364	13191	0.14%	0.016%
44	18.115	2549	2555	2559	rBV4	50897	87728	0.92%	0.105%
45	18.280	2580	2583	2588	rBV3	21958	31632	0.33%	0.038%
46	18.327	2589	2591	2594	rVB3	11464	12573	0.13%	0.015%
47	18.592	2634	2636	2640	rBV4	18487	23068	0.24%	0.028%
48	18.633	2640	2643	2648	rVB7	15627	21384	0.22%	0.026%
49	19.174	2731	2735	2739	rVB2	65121	85582	0.89%	0.102%
50	19.239	2743	2746	2749	rVV	62904	94053	0.98%	0.112%
51	19.274	2749	2752	2758	rVB	139500	175441	1.83%	0.209%
52	19.392	2770	2772	2779	rVB5	28337	37766	0.39%	0.045%
53	19.550	2797	2799	2802	rBV3	16286	19258	0.20%	0.023%
54	19.609	2803	2809	2818	rVV	7199349	9564000	100.00%	11.413%
55	21.450	3116	3122	3128	rBV2	2541308	3820118	39.94%	4.559%
56	24.285	3595	3604	3622	rVB	2713045	6592616	68.93%	7.867%
57	24.491	3630	3639	3650	rBV	1395169	3388613	35.43%	4.044%




Sum of corrected areas: 83799990

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047515.D
Acq On : 13 Sep 2024 12:12
Operator : RC/JU
Sample : P3952-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

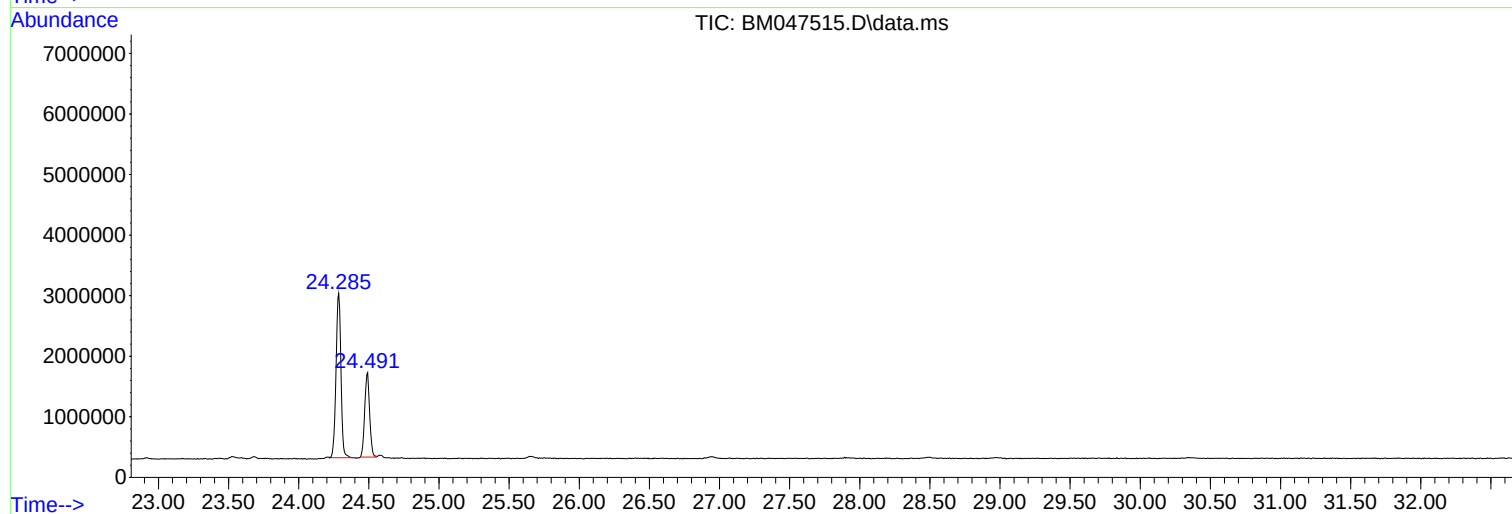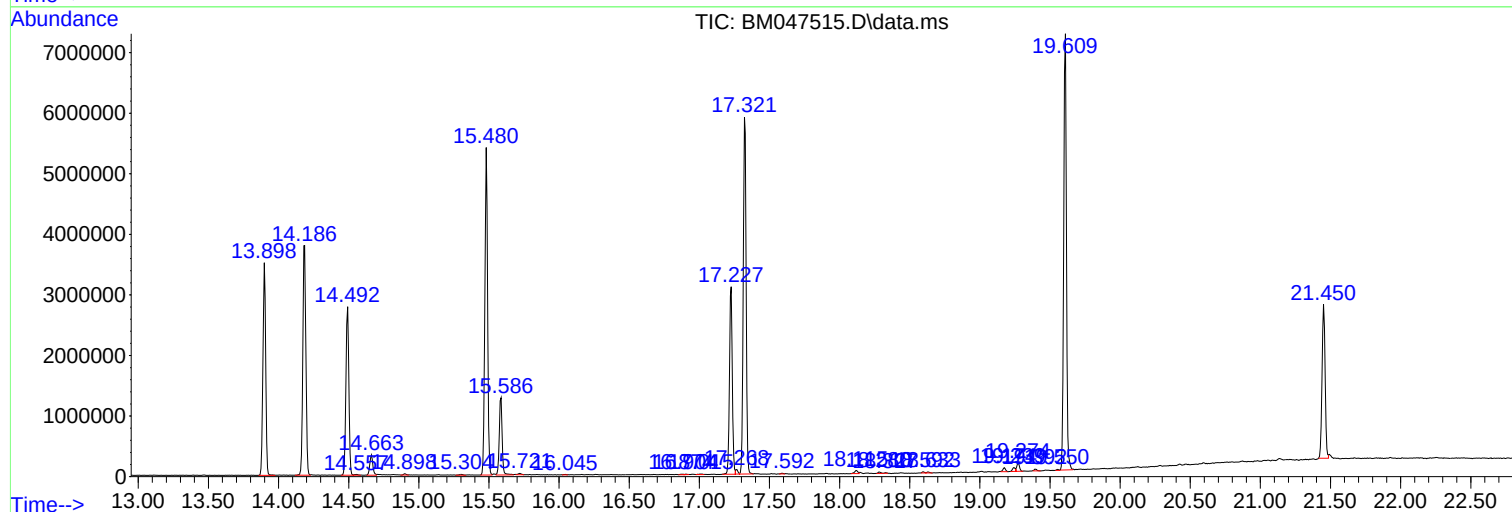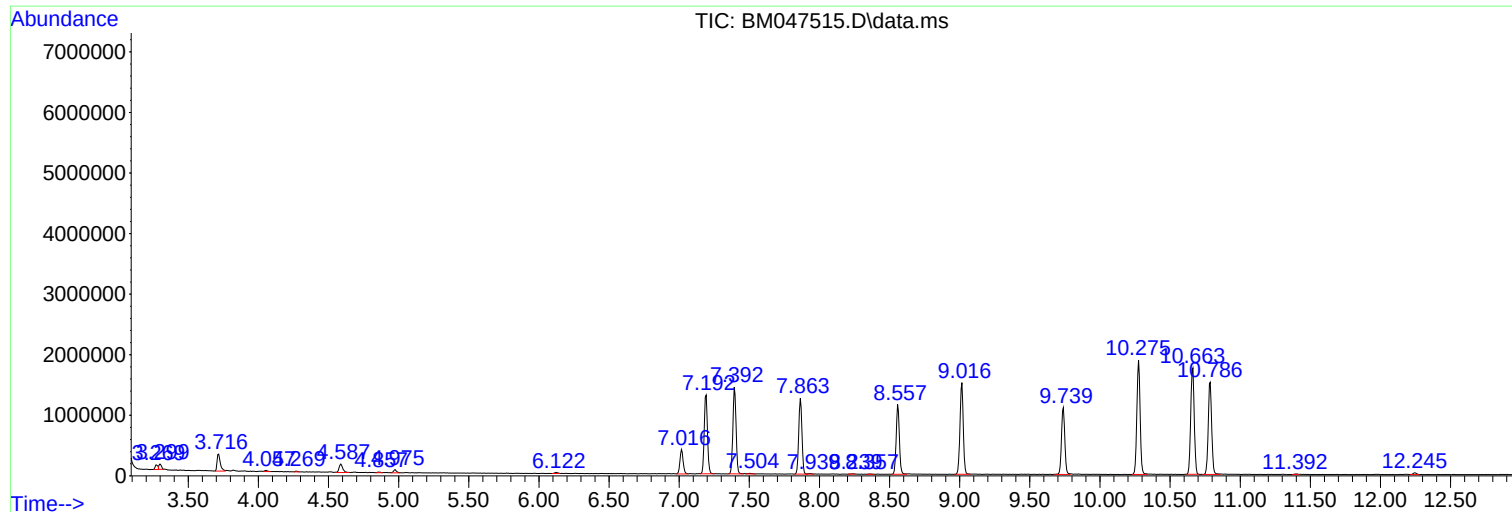

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047515.D
Acq On : 13 Sep 2024 12:12
Operator : RC/JU
Sample : P3952-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091324\
Data File : BM047515.D
Acq On : 13 Sep 2024 12:12
Operator : RC/JU
Sample : P3952-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B35

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc