

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM091417\
 Data File : BM011552.D
 Acq On : 14 Sep 2017 21:50
 Operator : SJ/JU
 Sample : I5191-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC9

Quant Time: Sep 15 02:28:30 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 15 02:27:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	372448	20.00	ng/ul	0.00
18) Naphthalene-d8	10.78	136	1658349	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	951448	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.34	188	2070053	20.00	ng/ul	0.00
78) Chrysene-d12	21.50	240	2077447	20.00	ng/ul	0.00
86) Perylene-d12	23.88	264	1836699	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.39	96	40508	4.89	ng/uL	0.00
5) Phenol-d5	7.12	99	213889	5.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.29	67	748136	31.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.50	132	630249	23.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.67	113	389295	13.94	ng/ul	0.00
19) Nitrobenzene-d5	9.13	128	397695	31.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.86	143	396503	30.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.39	165	693002	26.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	53024	1.82	ng/ul	0.01
44) Dimethylphthalate-d6	14.00	166	2704993	33.63	ng/ul	0.00
47) Acenaphthylene-d8	14.30	160	3131617	32.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.79	143	52623	3.48	ng/ul	0.00
58) Fluorene-d10	15.59	176	2363384	33.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.70	200	333357	27.68	ng/ul	0.00
71) Anthracene-d10	17.44	188	3984670	39.09	ng/ul	0.00
79) Pyrene-d10	19.73	212	4367411	44.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.73	264	3450617	39.42	ng/ul	0.00


Target Compounds				Ovalue	
20) Nitrobenzene	9.18	77	45267	1.529	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM091417\
Data File : BM011552.D
Acq On : 14 Sep 2017 21:50
Operator : SJ/JU
Sample : I5191-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC9

Quant Time: Sep 15 02:28:30 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 15 02:27:08 2017
Response via : Initial Calibration

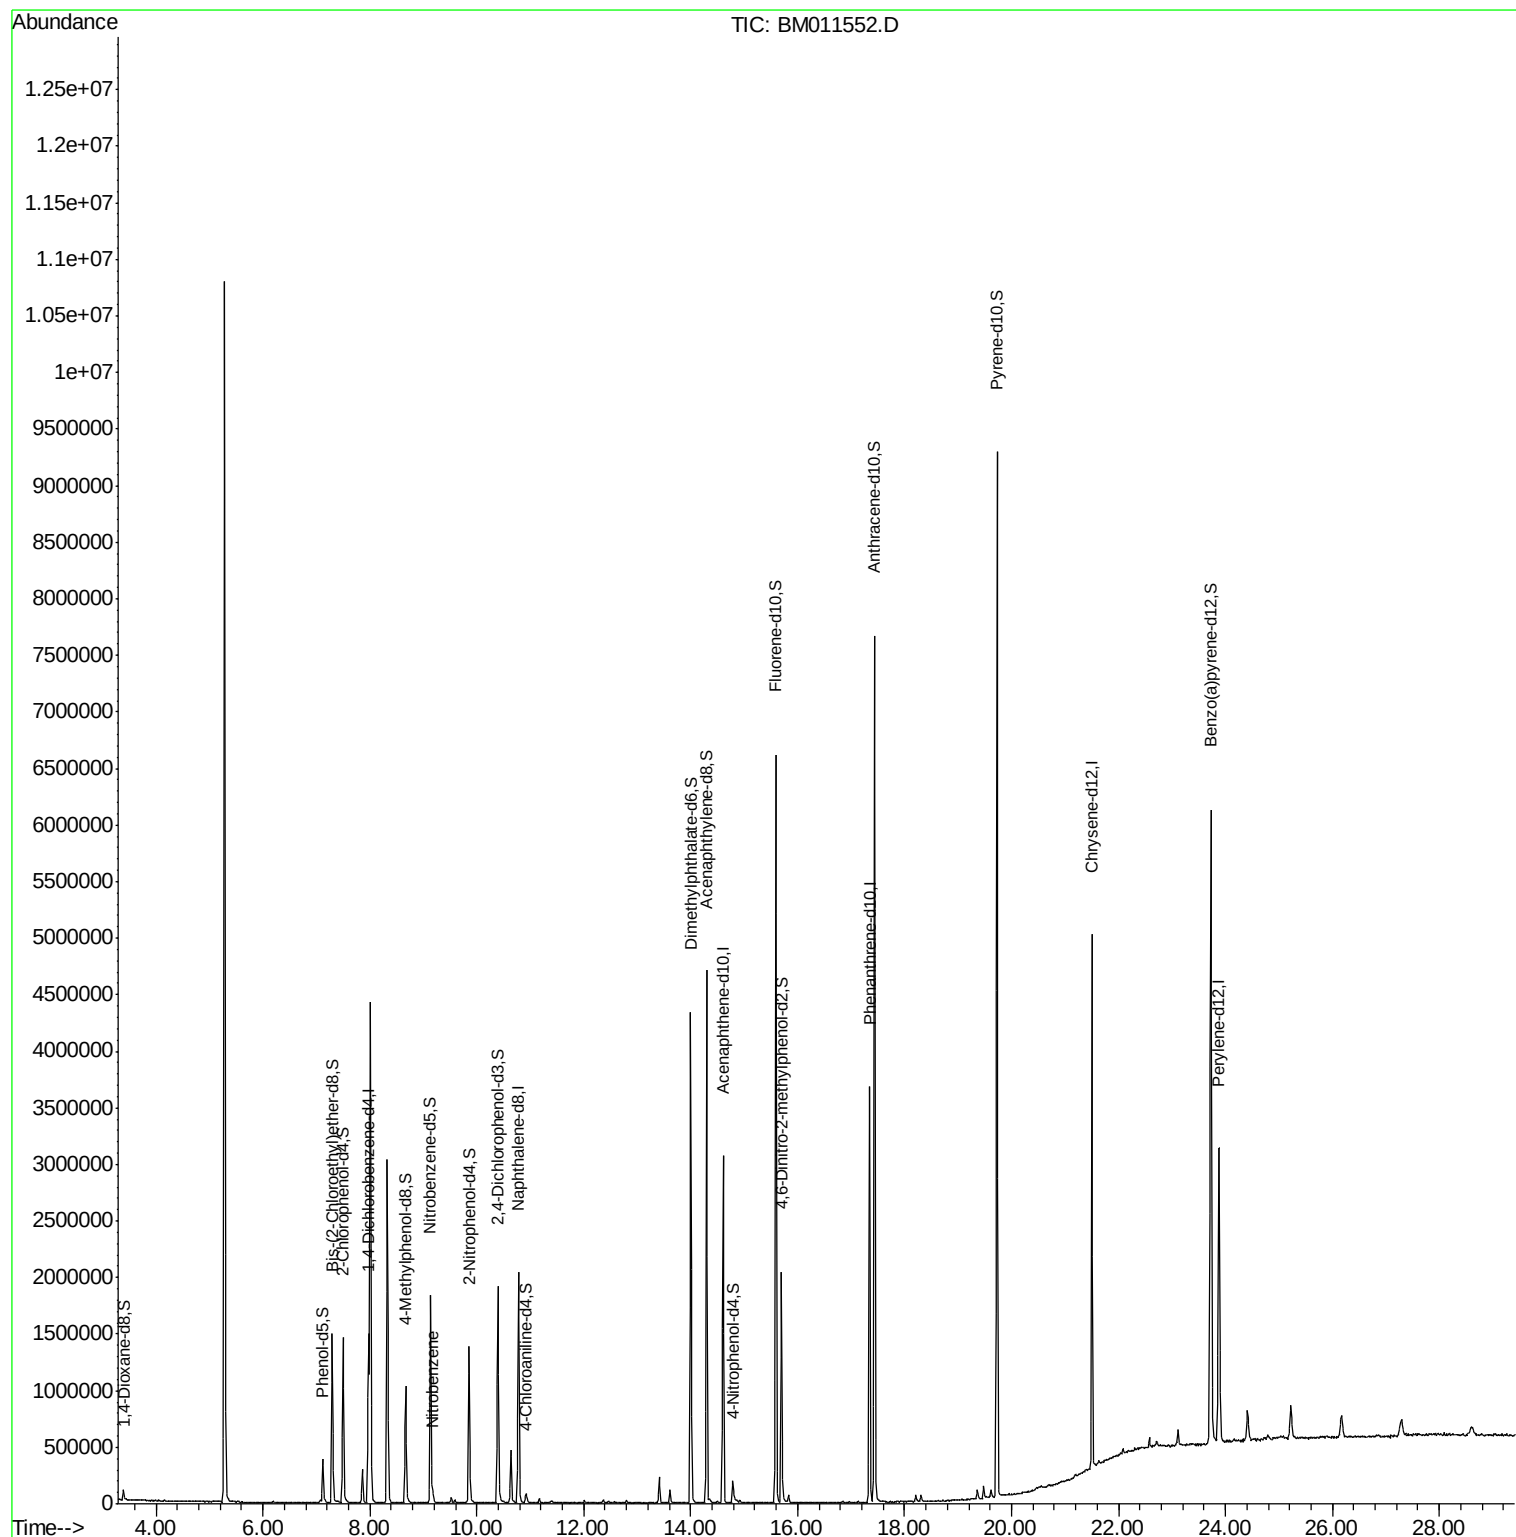

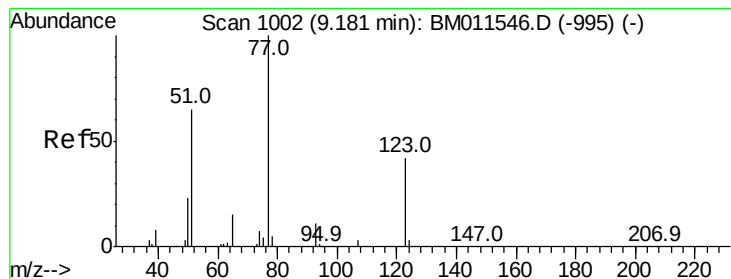

#20

Nitrobenzene

Concen: 1.529 ng/ul

RT: 9.18 min Scan# 1002

Delta R.T. -0.00 min

Lab File: BM011552.D

Acq: 14 Sep 2017 21:50

Instrument :

BNA_M

ClientSampleId :

C0AC9

Tot Ion: 77 Resp: 45267

Ion Ratio Lower Upper

77 100

123 41.4 31.8 47.8

65 17.0 10.6 16.0#

