

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM091417\
 Data File : BM011560.D
 Acq On : 15 Sep 2017 02:42
 Operator : SJ/JU
 Sample : I5191-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF2

Quant Time: Sep 15 03:56:44 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 15 02:27:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	396748	20.00	ng/ul	0.00
18) Naphthalene-d8	10.78	136	1645969	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	945226	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.34	188	2069154	20.00	ng/ul	0.00
78) Chrysene-d12	21.50	240	2153316	20.00	ng/ul	0.00
86) Perylene-d12	23.87	264	2037728	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.40	96	12485	1.42	ng/uL	0.00
5) Phenol-d5	7.12	99	226407	5.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.30	67	831265	32.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.50	132	709808	24.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.67	113	435040	14.63	ng/ul	0.00
19) Nitrobenzene-d5	9.13	128	445961	35.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.86	143	462393	35.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.39	165	790825	30.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	49395	1.71	ng/ul	0.00
44) Dimethylphthalate-d6	14.00	166	2904596	36.35	ng/ul	0.00
47) Acenaphthylene-d8	14.30	160	3434561	35.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.79	143	70503	4.69	ng/ul	0.00
58) Fluorene-d10	15.59	176	2495318	36.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.70	200	356072	29.57	ng/ul	0.00
71) Anthracene-d10	17.44	188	4032698	39.58	ng/ul	0.00
79) Pyrene-d10	19.73	212	4469257	44.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.73	264	3781243	38.94	ng/ul	0.00

Target Compounds


					Ovalue	
11) 2-Methylphenol	8.36	108	371438	12.954	ng/ul	96
20) Nitrobenzene	9.18	77	705855	24.024	ng/ul	96
37) 1,2,4,5-Tetrachlorobenzene	12.80	216	413720	14.755	ng/ul#	96
42) 2-Chloronaphthalene	13.60	162	335936	5.676	ng/ul#	45
46) 2,6-Dinitrotoluene	14.01	165	14436	1.068	ng/ul#	32
73) 1,2,3,4-Tetrachlorobenzene	13.40	216	1834962	66.551	ng/uL	99
74) Pentachlorobenzene	14.92	250	89945	3.216	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM091417\
Data File : BM011560.D
Acq On : 15 Sep 2017 02:42
Operator : SJ/JU
Sample : I5191-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF2

Quant Time: Sep 15 03:56:44 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 15 02:27:08 2017
Response via : Initial Calibration

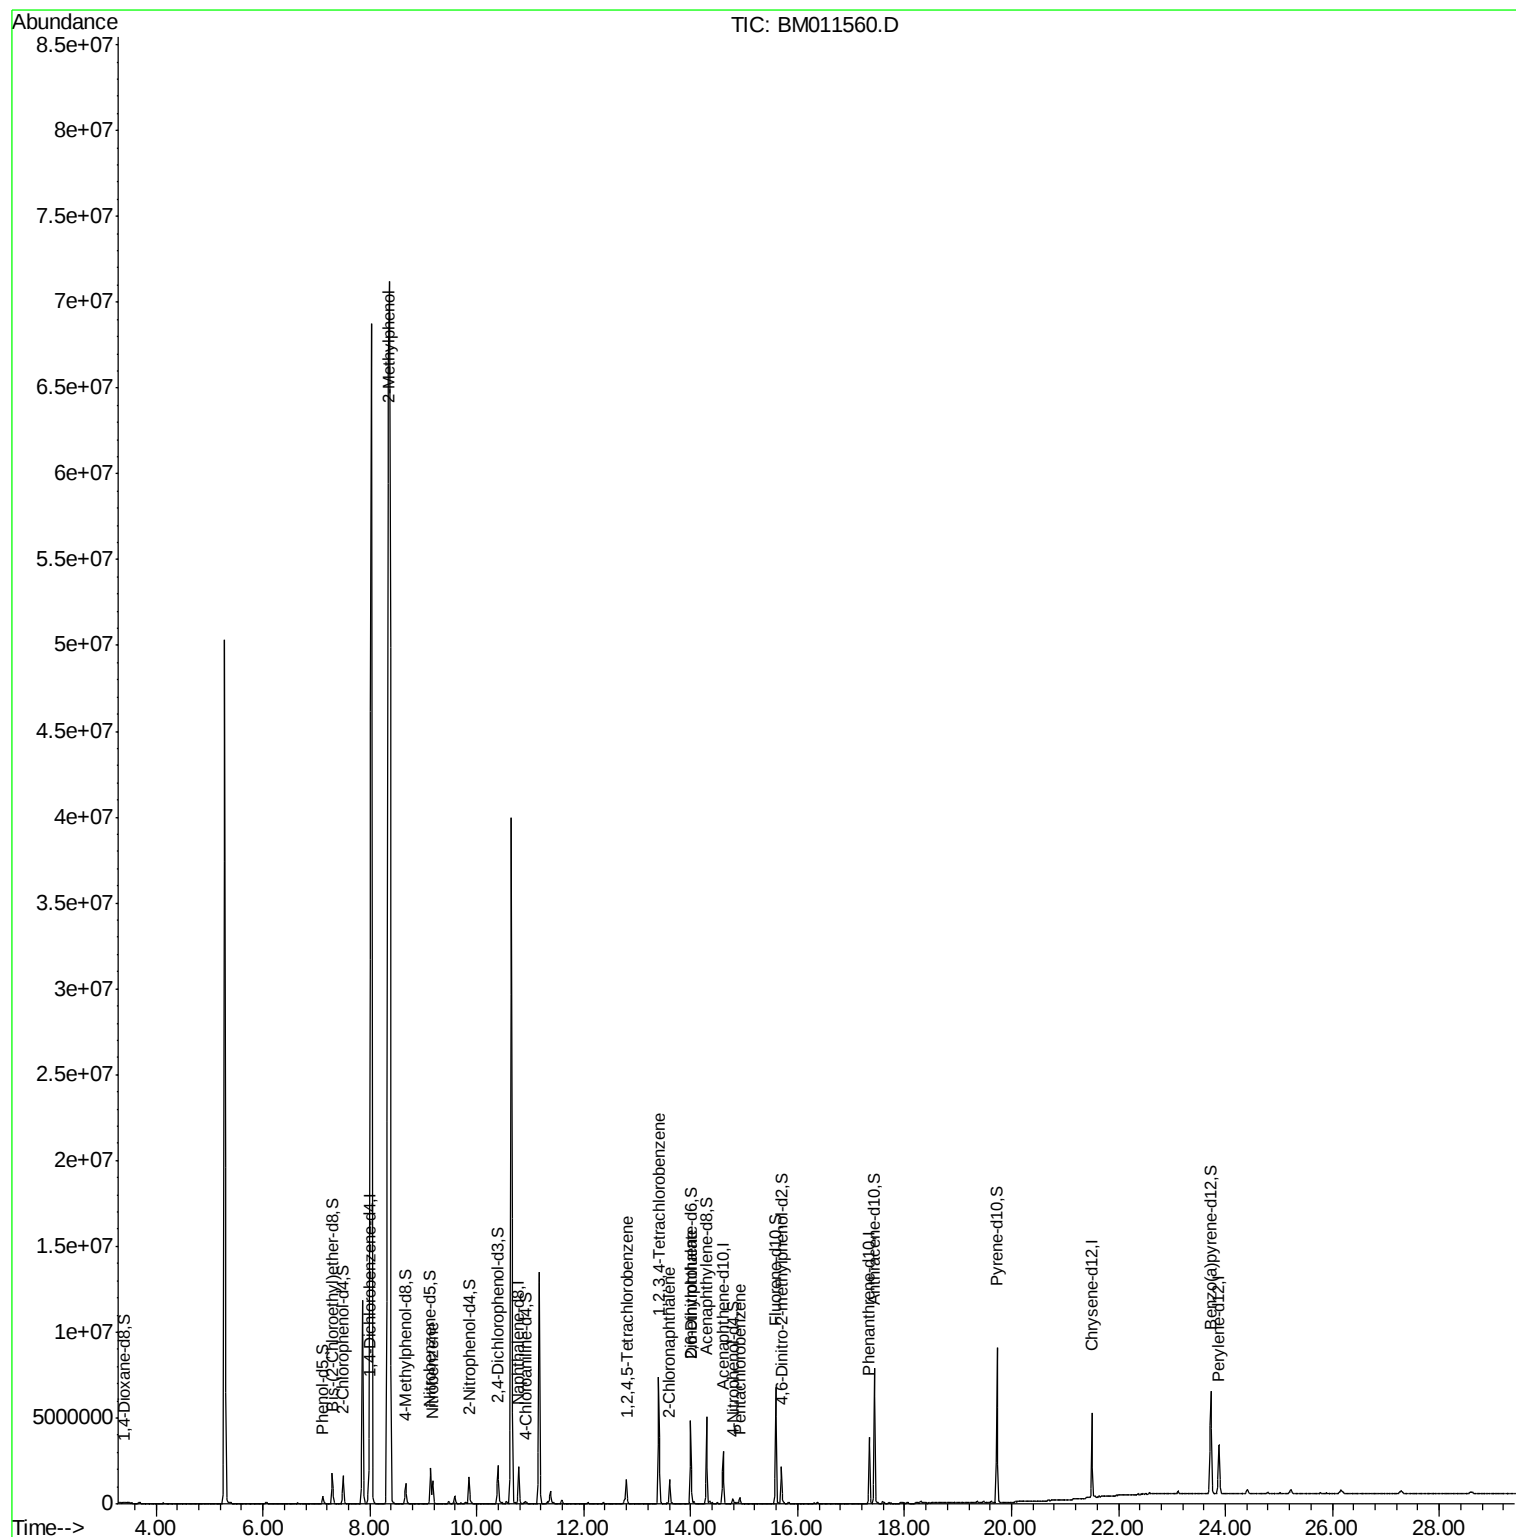

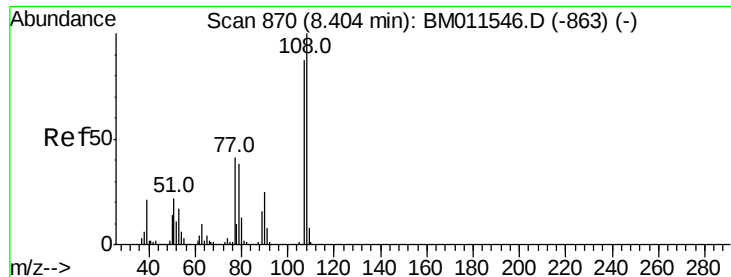

#11

2-Methylphenol

Concen: 12.954 ng/ul

RT: 8.36 min Scan# 862

Delta R.T. -0.05 min

Lab File: BM011560.D

Acq: 15 Sep 2017 02:42

Instrument :

BNA_M

ClientSampleId :





C0AF2

Tot Ion:108 Resp: 371438

Ion Ratio Lower Upper

108 100

107 88.9 74.1 111.1

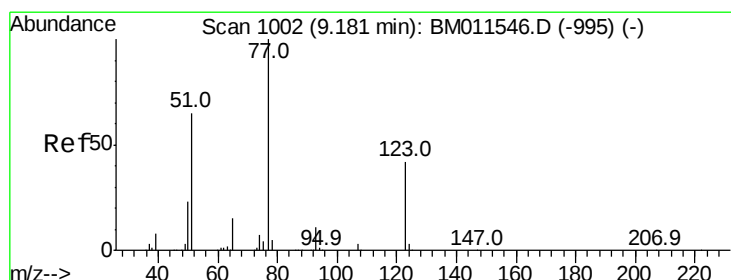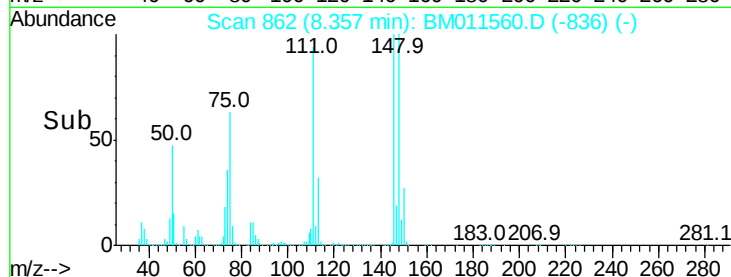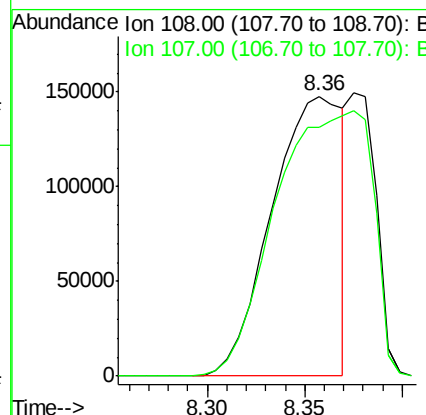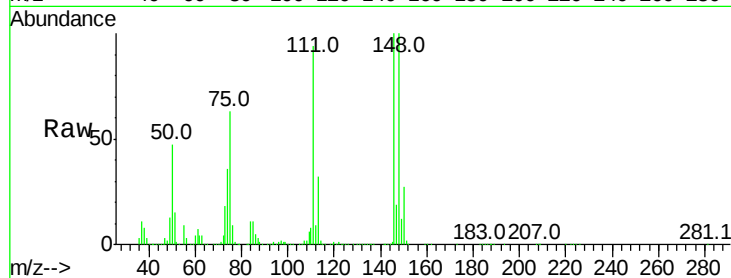

#20

Nitrobenzene

Concen: 24.024 ng/ul

RT: 9.18 min Scan# 1002

Delta R.T. 0.00 min

Lab File: BM011560.D

Acq: 15 Sep 2017 02:42




Tgt Ion: 77 Resp: 705855


Ion Ratio Lower Upper

77 100

123 42.7 31.8 47.8

65 14.6 10.6 16.0


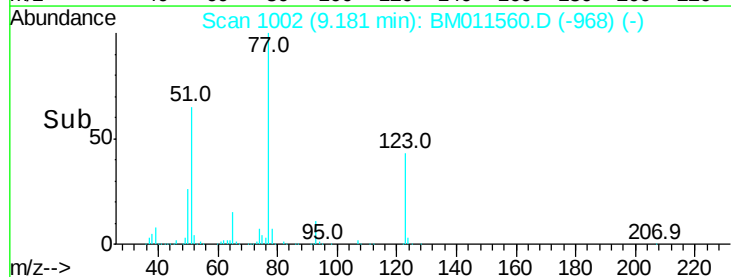
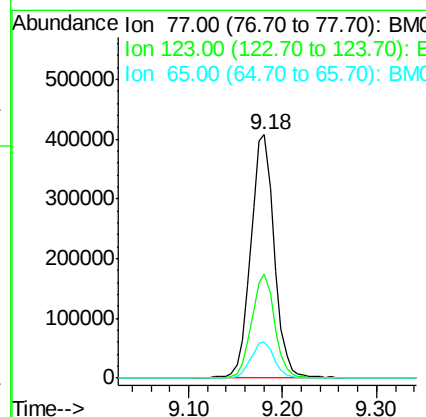
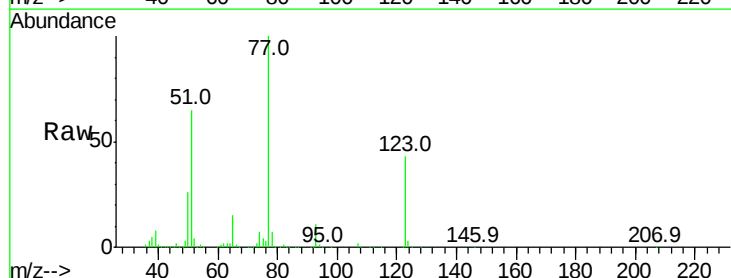


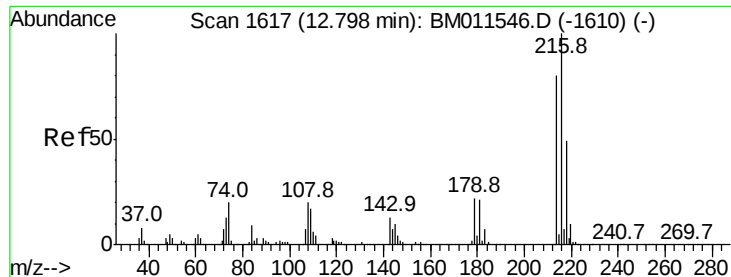

#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 14.755 ng/ul
 RT: 12.80 min Scan# 1617
 Delta R.T. 0.00 min
 Lab File: BM011560.D
 Acq: 15 Sep 2017 02:42




Instrument :
 BNA_M
 ClientSampleId :
 C0AF2


Tot Ion:	216	Resp:	413720
Ion	Ratio	Lower	Upper
216	100		
214	78.7	64.1	96.1
179	21.8	14.5	21.7#
108	19.0	10.4	15.6#

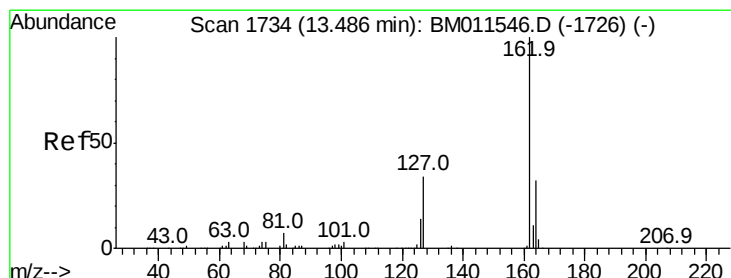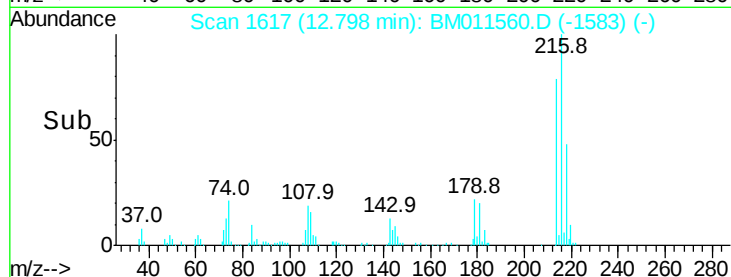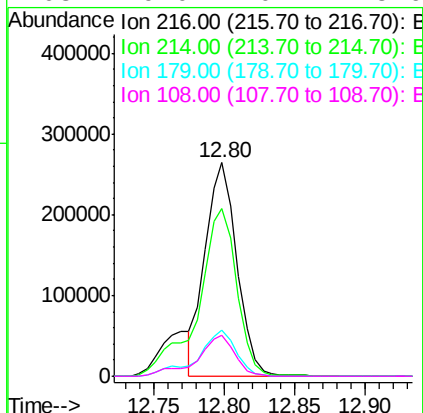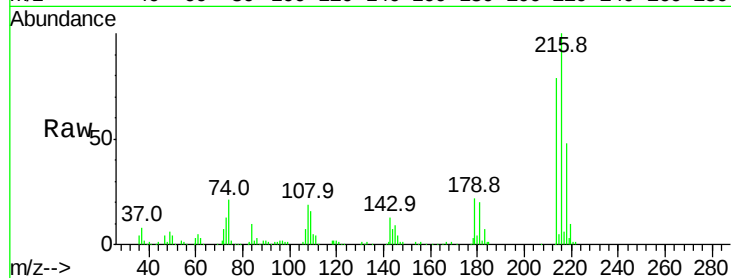

#42
 2-Chloronaphthalene
 Concen: 5.676 ng/ul
 RT: 13.60 min Scan# 1754
 Delta R.T. 0.12 min
 Lab File: BM011560.D
 Acq: 15 Sep 2017 02:42

Tgt Ion:	162	Resp:	335936
Ion	Ratio	Lower	Upper
162	100		
164	62.6	26.2	39.4#
127	2.6	29.5	44.3#


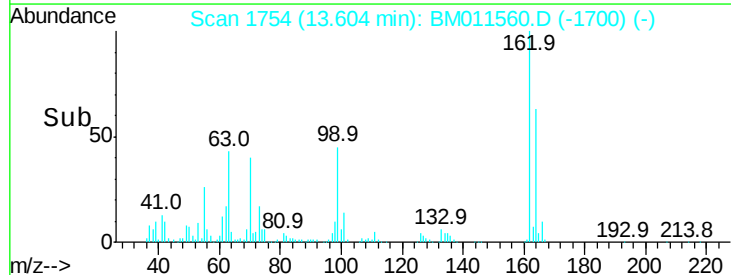
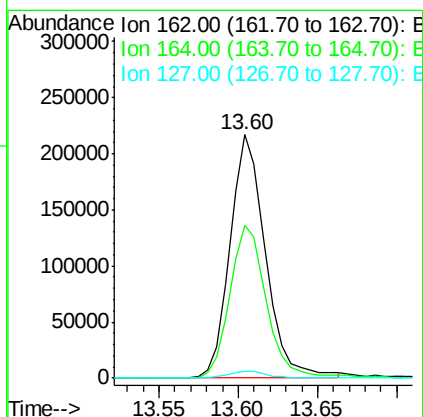
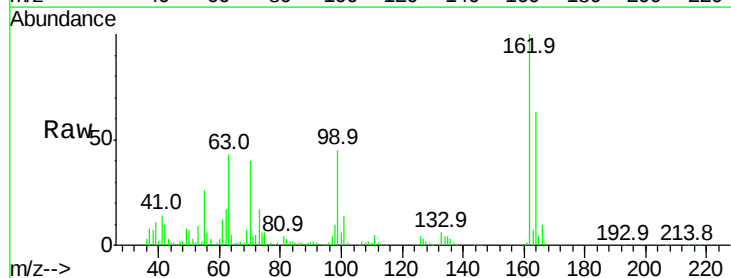


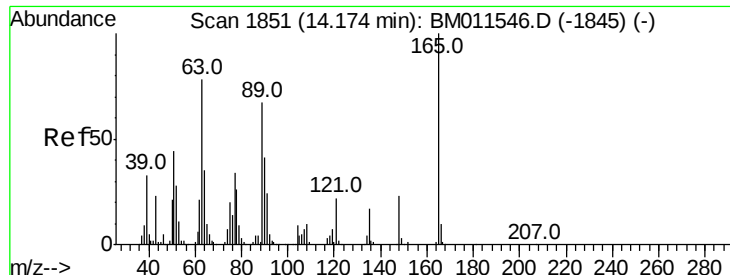

#46
 2,6-Dinitrotoluene
 Concen: 1.068 ng/ul
 RT: 14.01 min Scan# 1823
 Delta R.T. -0.16 min
 Lab File: BM011560.D
 Acq: 15 Sep 2017 02:42




Instrument :
 BNA_M
 ClientSampleId :
 C0AF2


Tot Ion:165 Resp: 14436
 Ion Ratio Lower Upper
 165 100
 89 0.0 43.8 65.8#
 121 45.9 17.8 26.6#

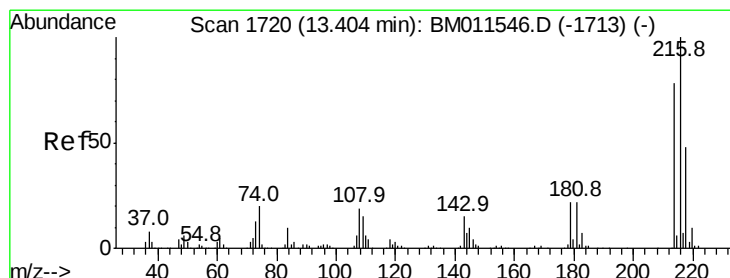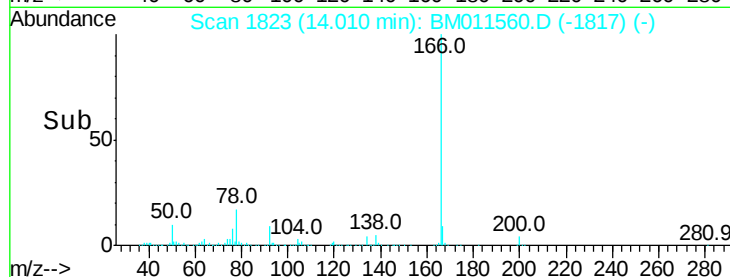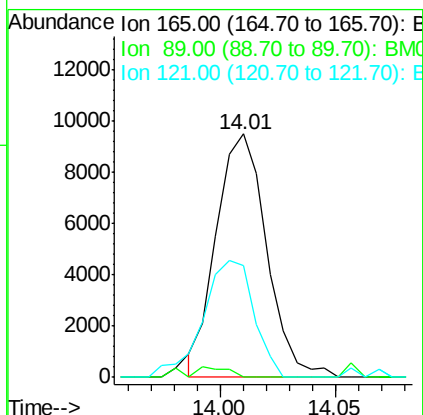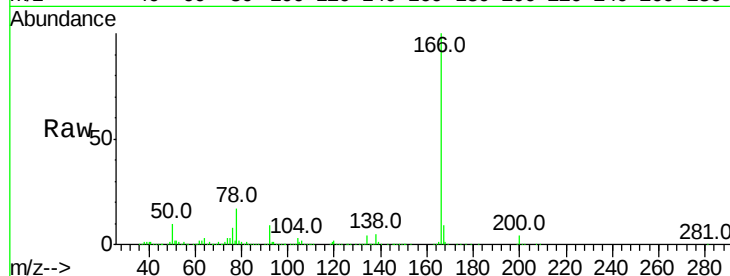

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 66.551 ng/uL
 RT: 13.40 min Scan# 1720
 Delta R.T. 0.00 min
 Lab File: BM011560.D
 Acq: 15 Sep 2017 02:42

Tgt Ion:216 Resp: 1834962
 Ion Ratio Lower Upper
 216 100
 214 79.0 64.1 96.1
 218 48.3 39.4 59.0

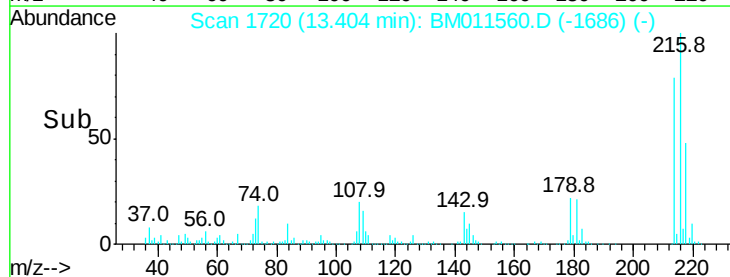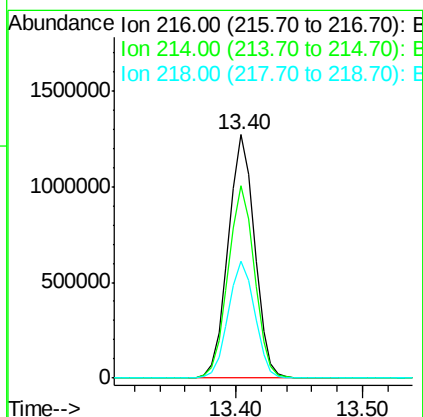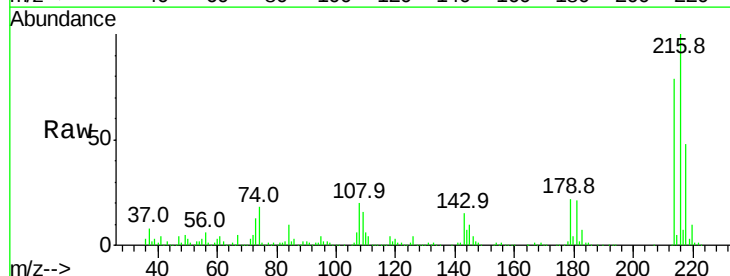

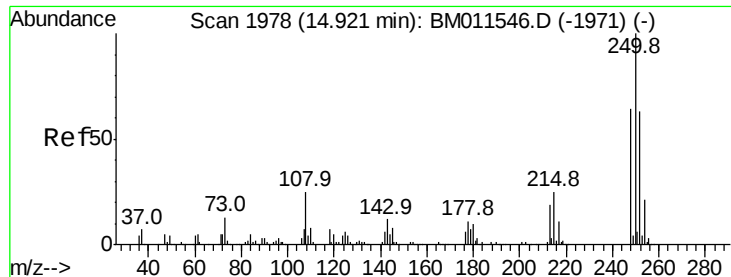

#74

Pentachlorobenzene

Concen: 3.216 ng/uL

RT: 14.92 min Scan# 1977

Delta R.T. -0.01 min

Lab File: BM011560.D

Acq: 15 Sep 2017 02:42

Instrument :

BNA_M

ClientSampleId :

C0AF2


Tot Ion:250 Resp: 89945

Ion Ratio Lower Upper

250 100

248 62.1 51.4 77.2

252 66.4 49.8 74.6

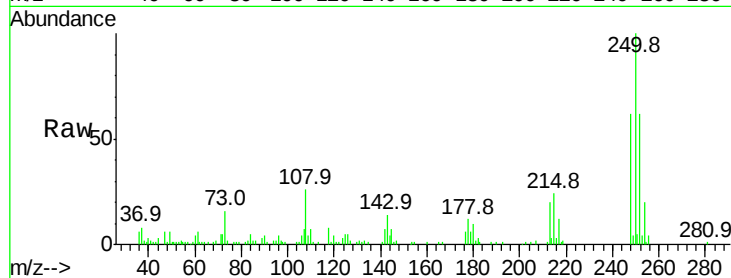

Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

