

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091520\
 Data File : BM027430.D
 Acq On : 16 Sep 2020 02:42
 Operator : JU/CG
 Sample : L3995-11
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG0P3

Quant Time: Sep 16 05:19:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 16 01:07:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	122375	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	425046	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	259170	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	544810	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	569071	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	674850	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	21235	7.72	ng/uL	0.00
5) Phenol-d5	6.75	99	55179	5.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	167912	25.07	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	161423	21.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	96762	11.76	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	91872	28.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	99936	28.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	181930	24.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	16364	1.83	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	584707	28.35	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	718150	30.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	7839	2.16	ng/ul	0.00
58) Fluorene-d10	15.19	176	530651	28.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	81252	23.30	ng/ul	0.00
71) Anthracene-d10	17.04	188	897724	34.84	ng/ul	0.00
79) Pyrene-d10	19.34	212	1039192	40.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1196517	33.05	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.66	163	56205	2.586	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091520\
Data File : BM027430.D
Acq On : 16 Sep 2020 02:42
Operator : JU/CG
Sample : L3995-11
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG0P3

Quant Time: Sep 16 05:19:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 16 01:07:14 2020
Response via : Initial Calibration

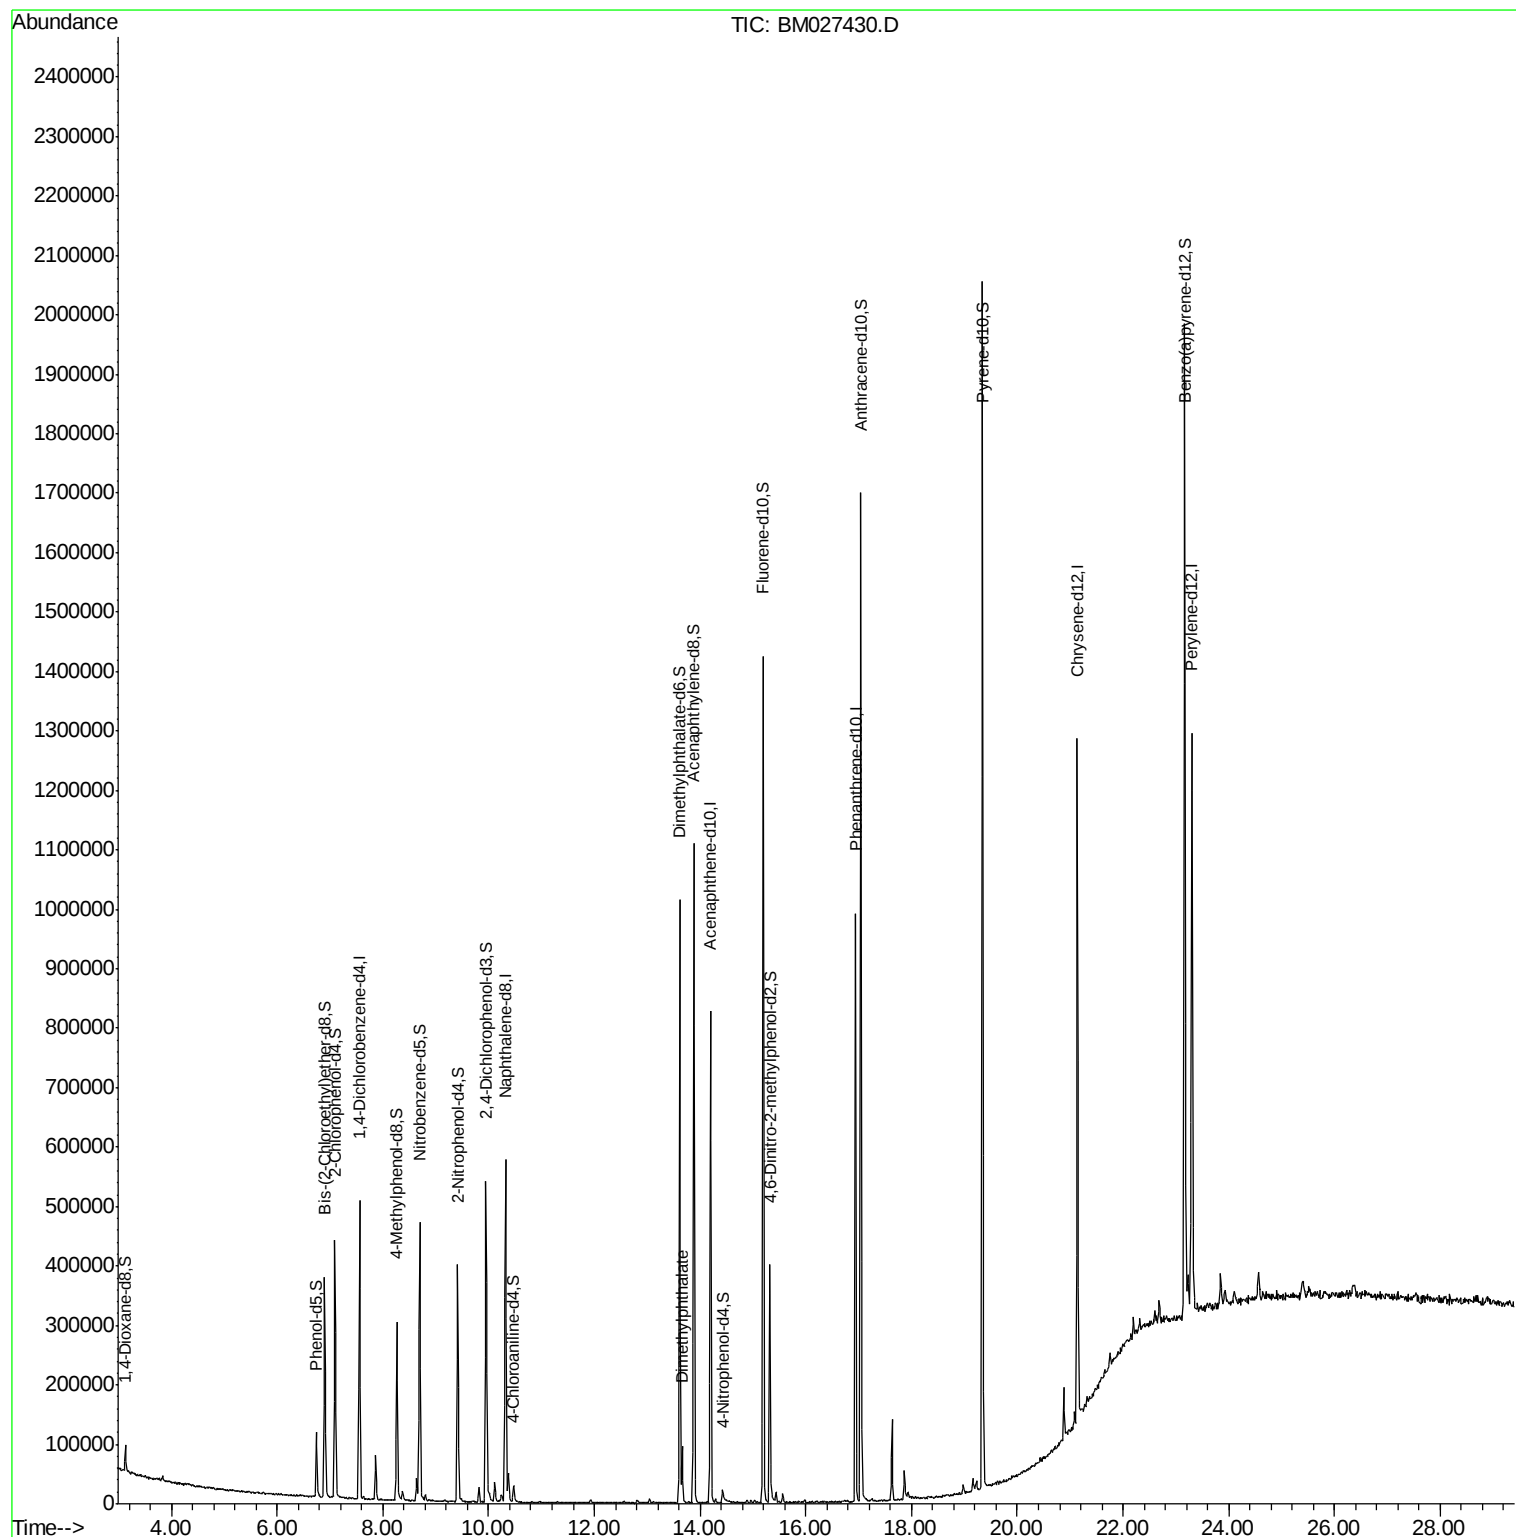

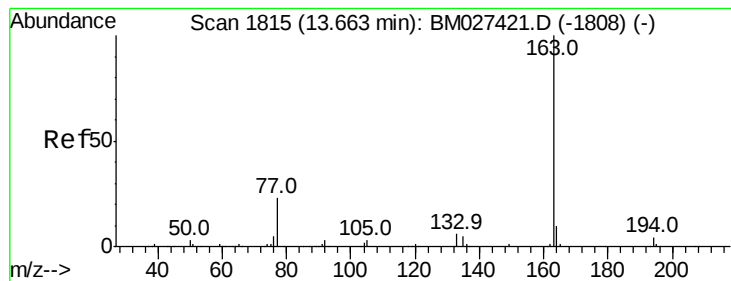

#45

Dimethylphthalate

Concen: 2.586 ng/ul

RT: 13.66 min Scan# 1815

Delta R.T. 0.00 min

Lab File: BM027430.D

Acq: 16 Sep 2020 02:42

Instrument :

BNA_M

ClientSampleId :

BG0P3


Tot Ion:163 Resp: 56205

Ion Ratio Lower Upper

163 100

194 5.5 3.3 4.9#

164 8.9 8.1 12.1

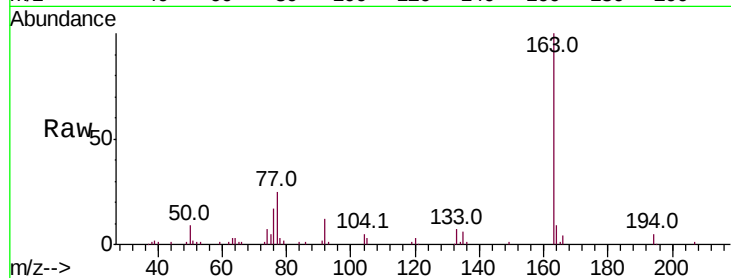

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

