

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091520\
 Data File : BM027434.D
 Acq On : 16 Sep 2020 05:06
 Operator : JU/CG
 Sample : L3995-17
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG0P0

Quant Time: Sep 16 05:40:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 16 01:07:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	123331	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	425811	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	261582	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	559155	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	589392	20.00	ng/ul	0.00
86) Perylene-d12	23.30	264	680849	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	20134	7.26	ng/uL	0.00
5) Phenol-d5	6.75	99	64851	6.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	189573	28.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	184174	24.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	112505	13.57	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	103621	32.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	114161	32.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	206066	27.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	12468	1.39	ng/ul	0.02
44) Dimethylphthalate-d6	13.62	166	661092	31.76	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	792108	33.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	6478	1.77	ng/ul	0.00
58) Fluorene-d10	15.19	176	563341	30.22	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	77667	21.70	ng/ul	0.00
71) Anthracene-d10	17.04	188	906621	34.29	ng/ul	0.00
79) Pyrene-d10	19.34	212	1054315	40.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.17	264	1225822	33.57	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.66	163	82508	3.761	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091520\
Data File : BM027434.D
Acq On : 16 Sep 2020 05:06
Operator : JU/CG
Sample : L3995-17
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG0P0

Quant Time: Sep 16 05:40:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 16 01:07:14 2020
Response via : Initial Calibration

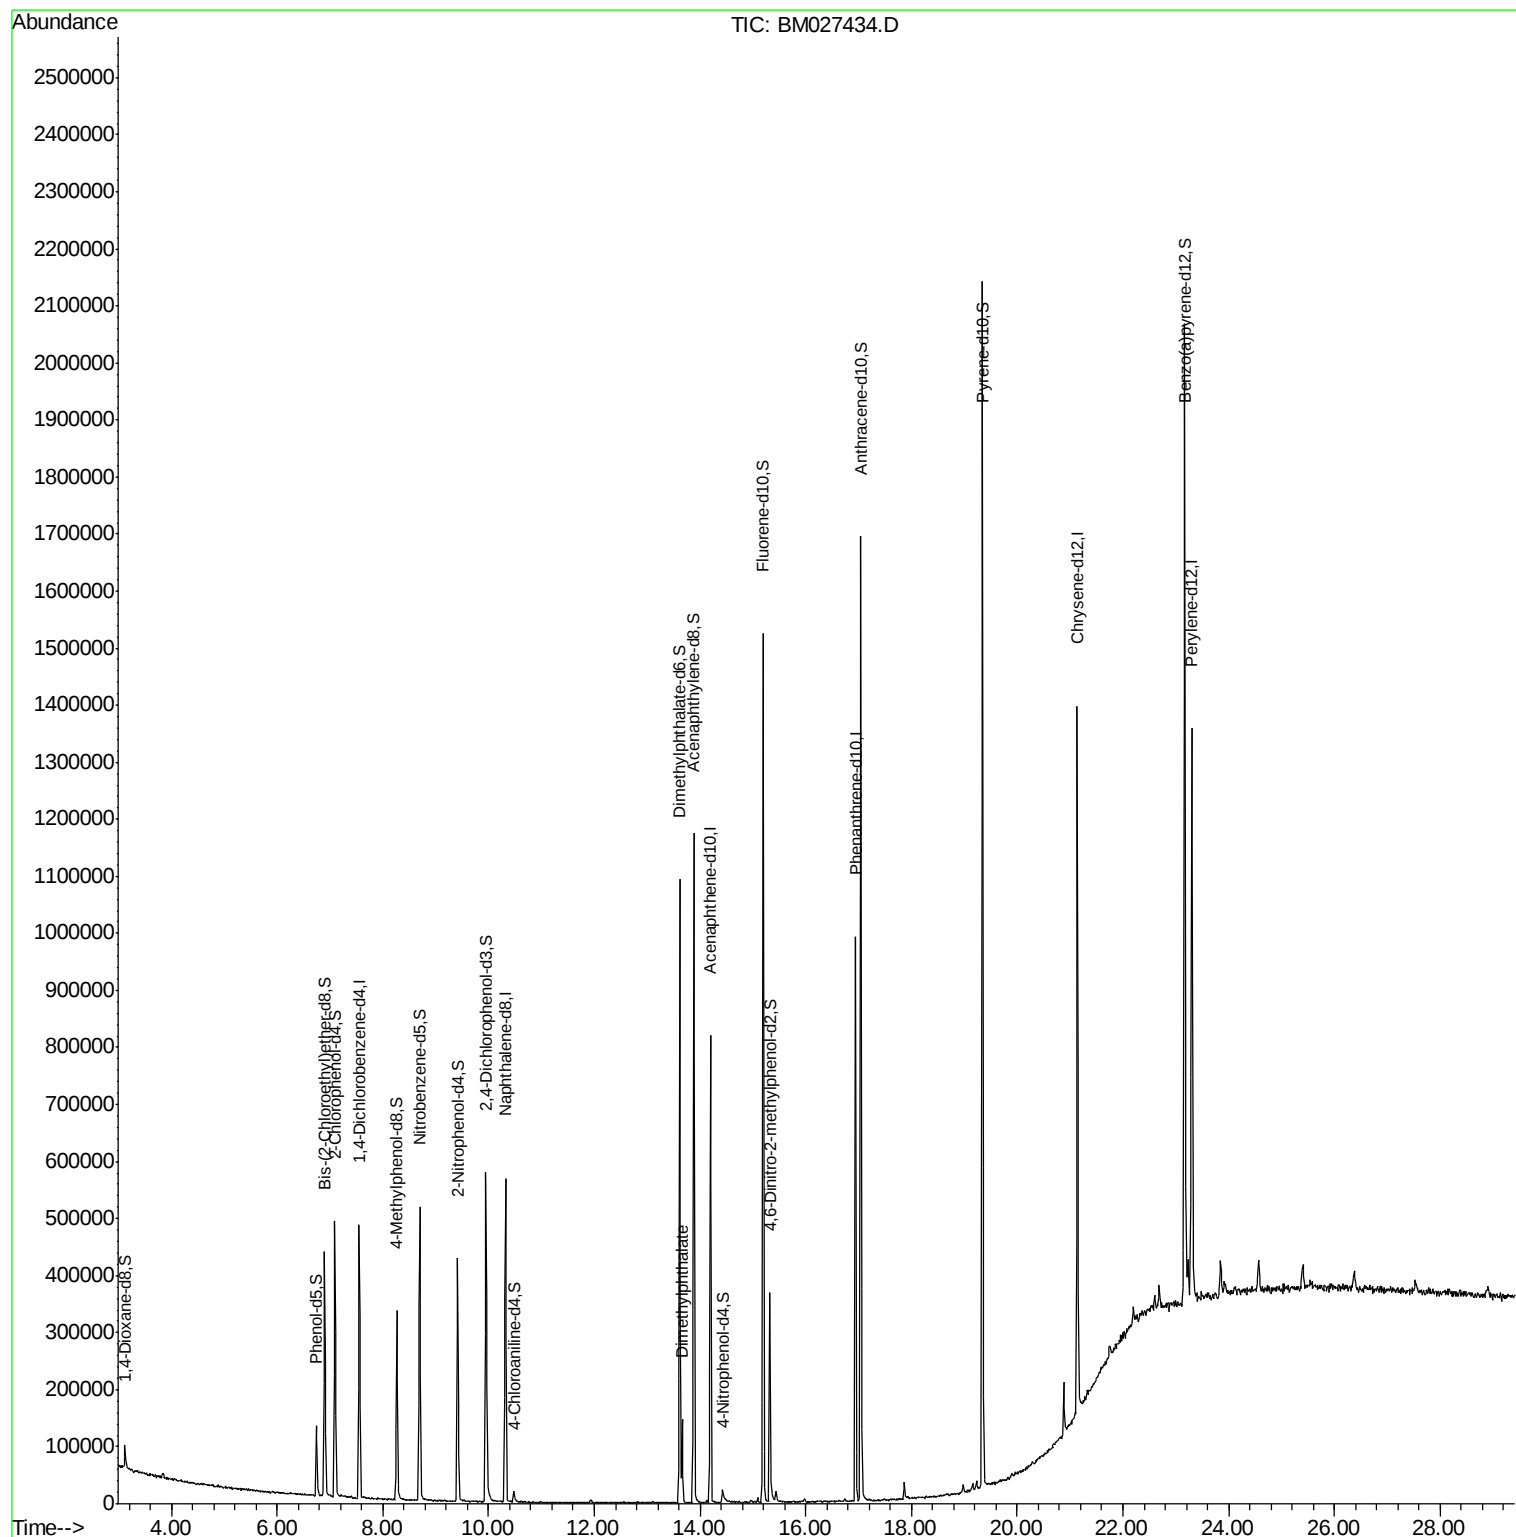

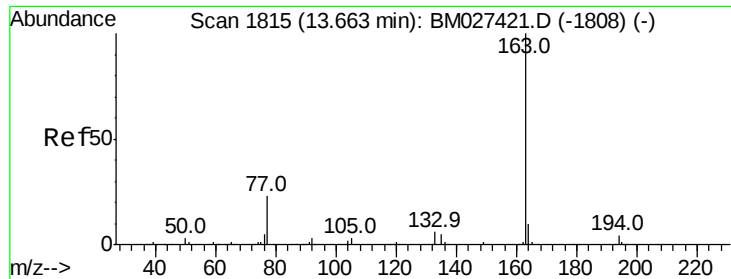

#45

Dimethylphthalate

Concen: 3.761 ng/ul

RT: 13.66 min Scan# 1815

Delta R.T. 0.00 min

Lab File: BM027434.D

Acq: 16 Sep 2020 05:06

Instrument :

BNA_M

ClientSampleId :

BG0P0


Tot Ion:163 Resp: 82508

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.6 8.1 12.1

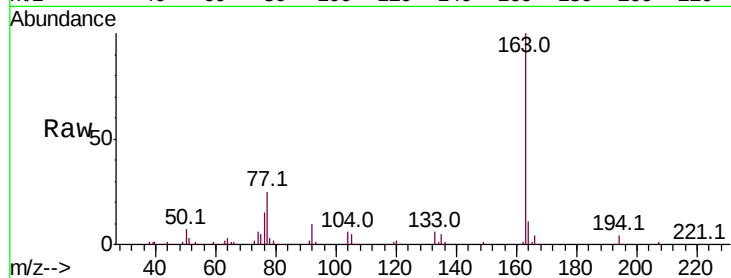

Abundance Ion 163.00 (162.70 to 163.70): E

80000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

