


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
Data File : BM022685.D
Acq On : 16 Sep 2019 11:30
Operator : HP/JU
Sample : K4780-13
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BN9

Manual Integrations
APPROVED

mohammad
9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:42:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

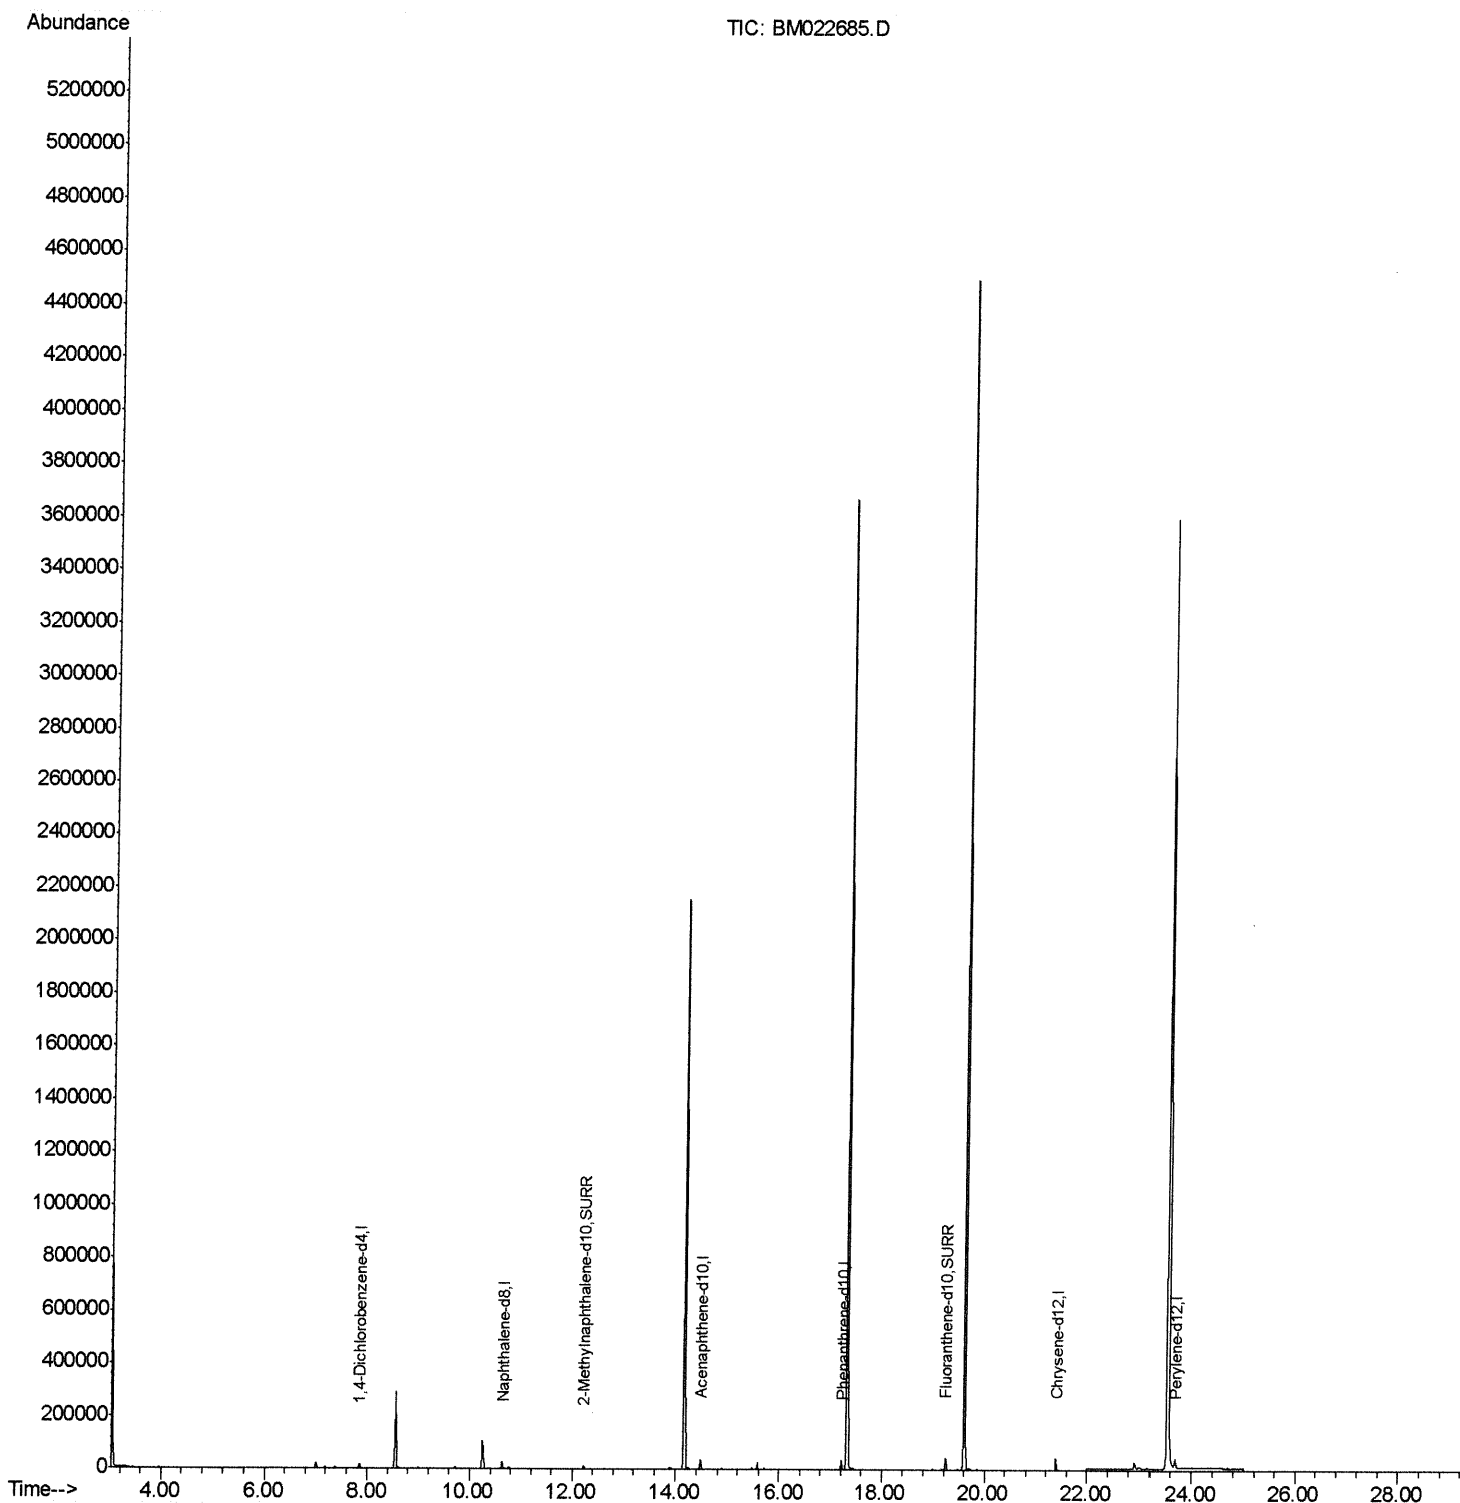

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9

Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:33:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

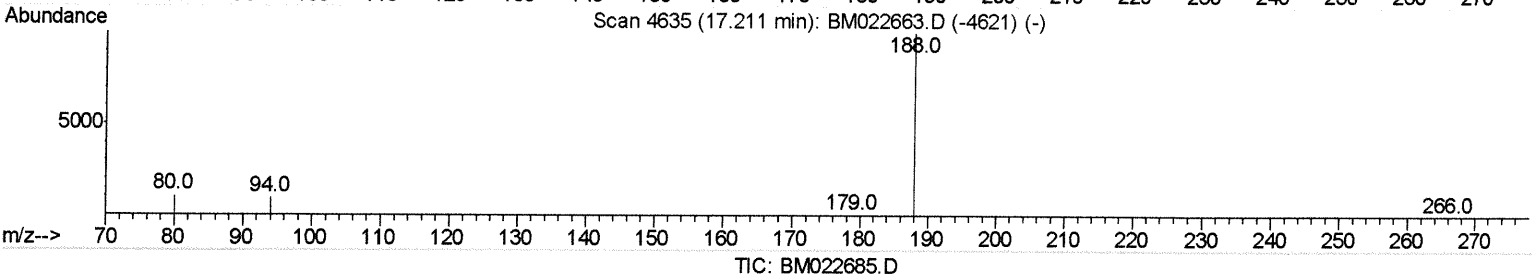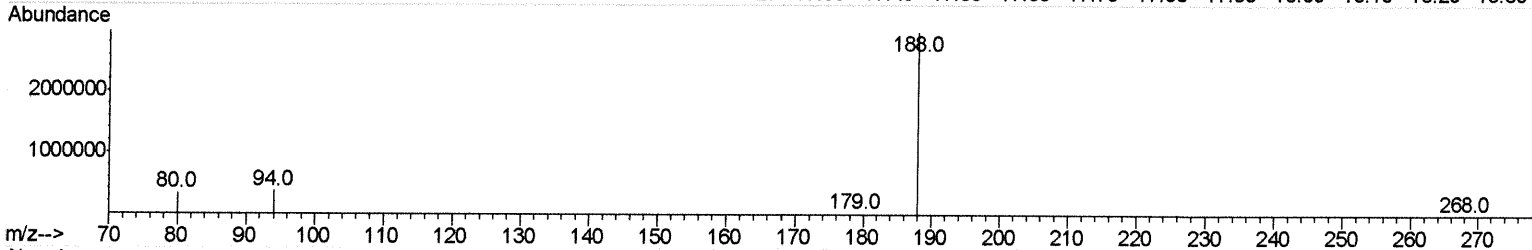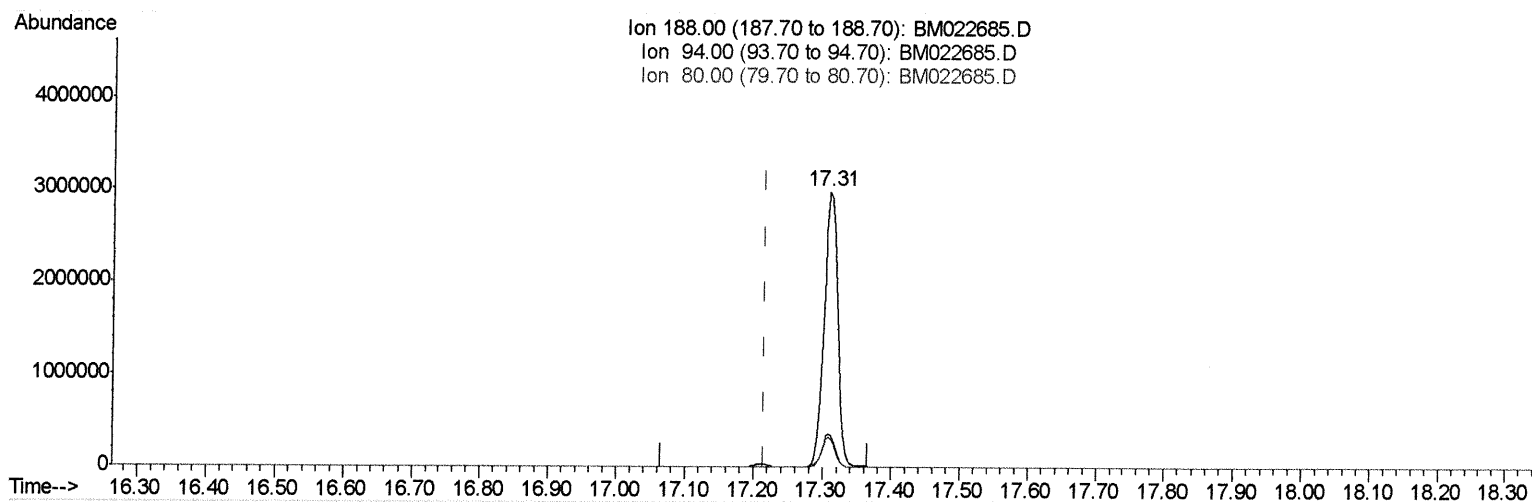

TIC: BM022685.D

(10) Phenanthrene-d10 (I)

17.308min (+0.092) 0.40ng/ul

response 4139323

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	12.22#
80.00	11.00	10.79
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9


Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:33:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

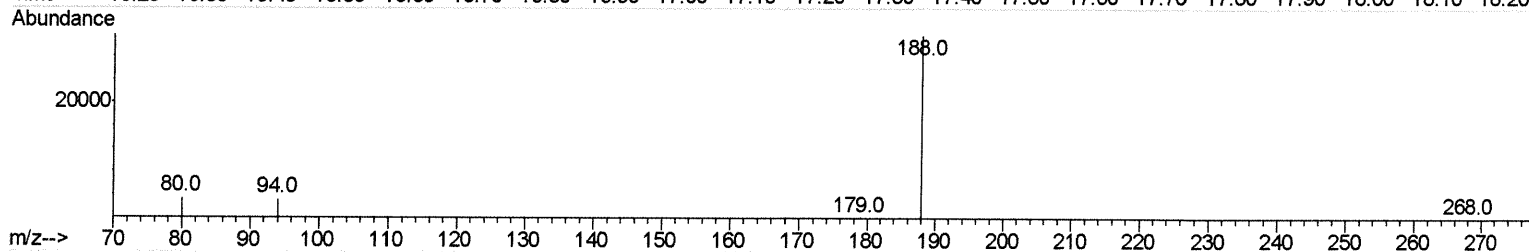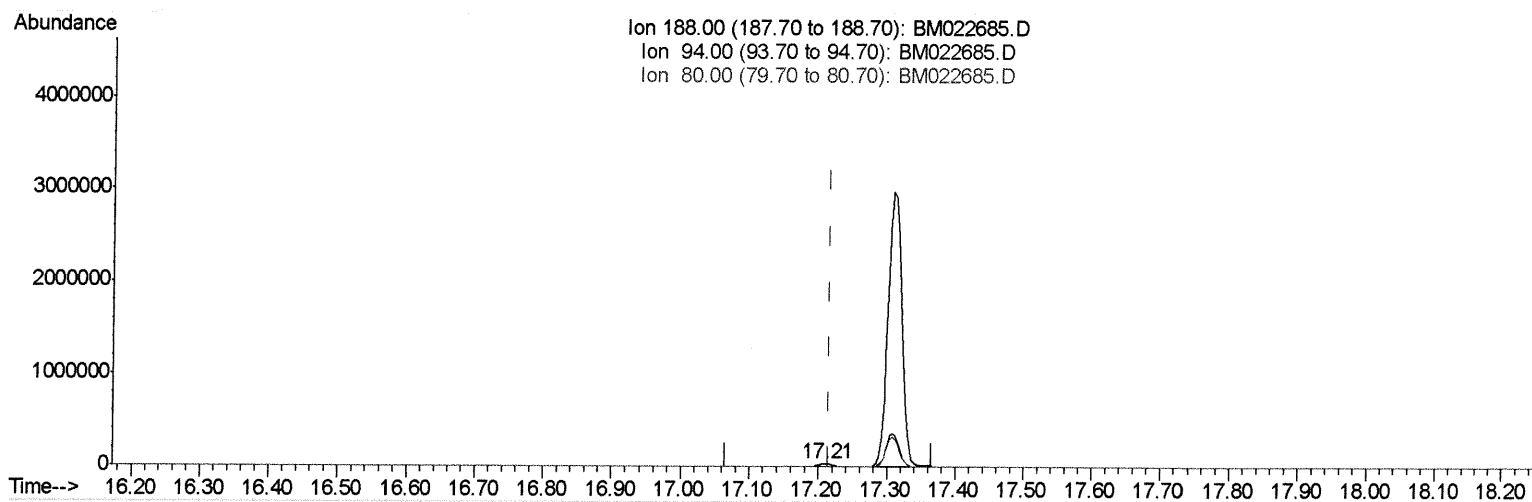

Scan 4635 (17.211 min): BM022685.D (-4621) (-)

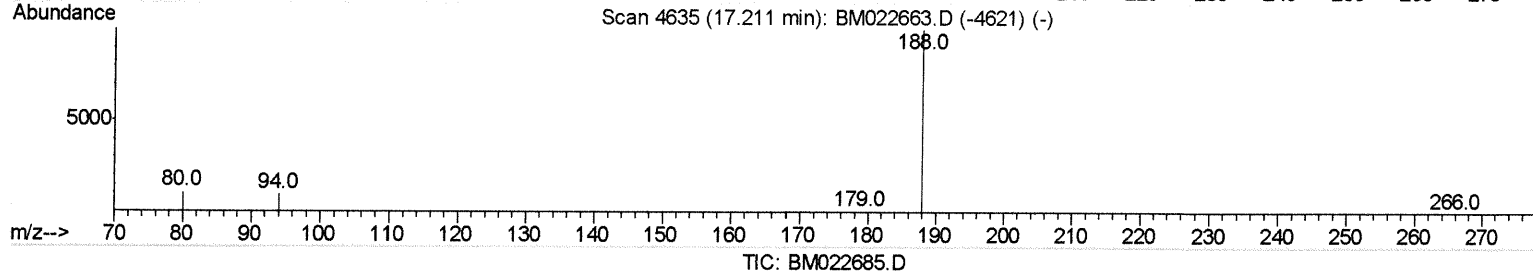

(10) Phenanthrene-d10 (I)

17.211min (-0.005) 0.40ng/ul m *JU* 09/17/19

response 44311

Ion	Exp%	Act%
188.00	100	100
94.00	9.80	9.89
80.00	11.00	10.66
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9

Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:39:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

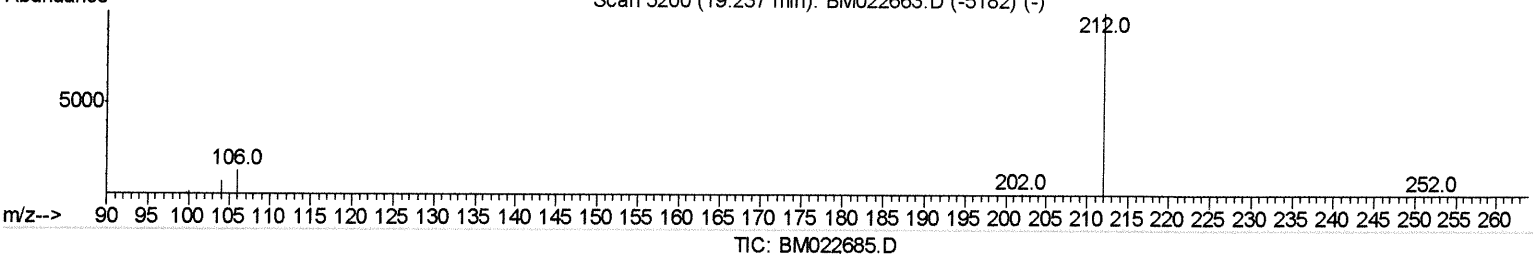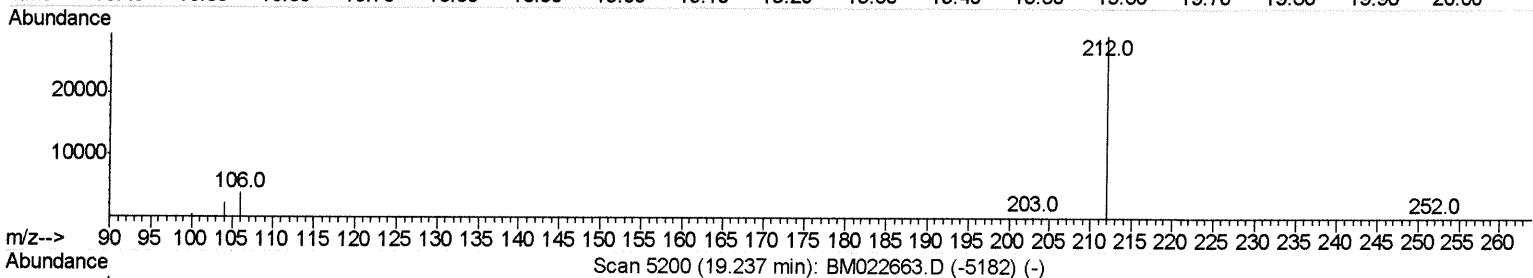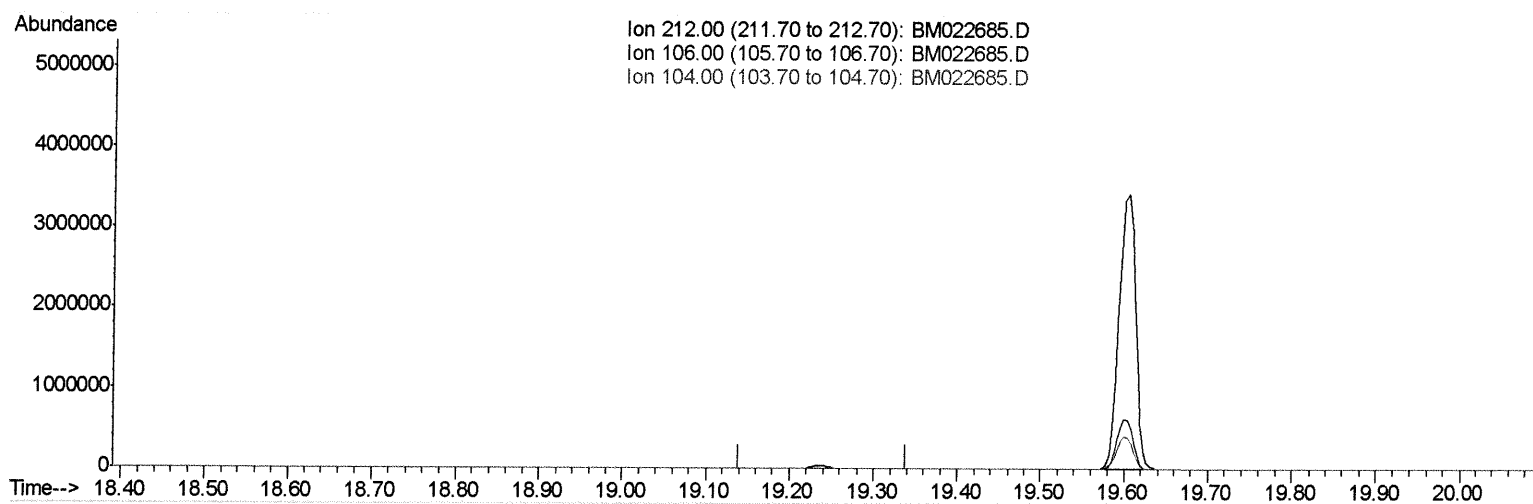

(14) Fluoranthene-d10 (SURR)

19.240min (-19.240) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	14.00	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9

Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:39:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

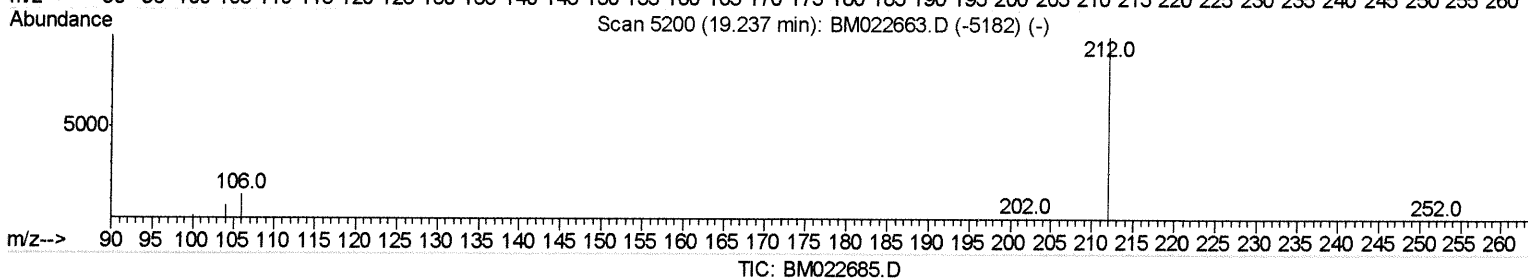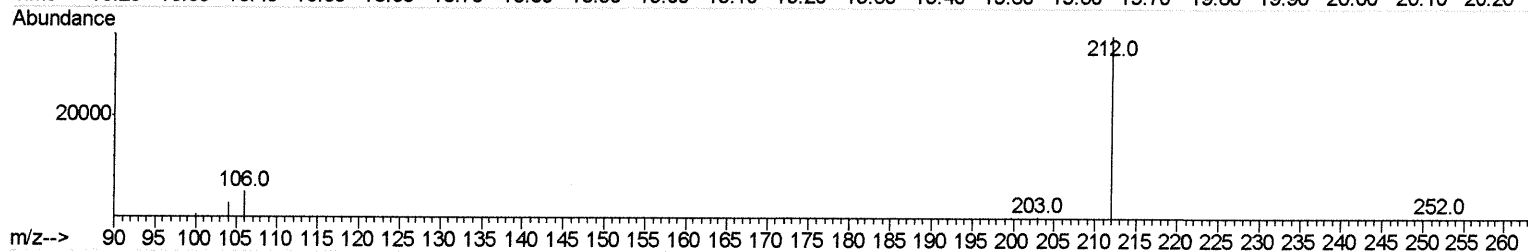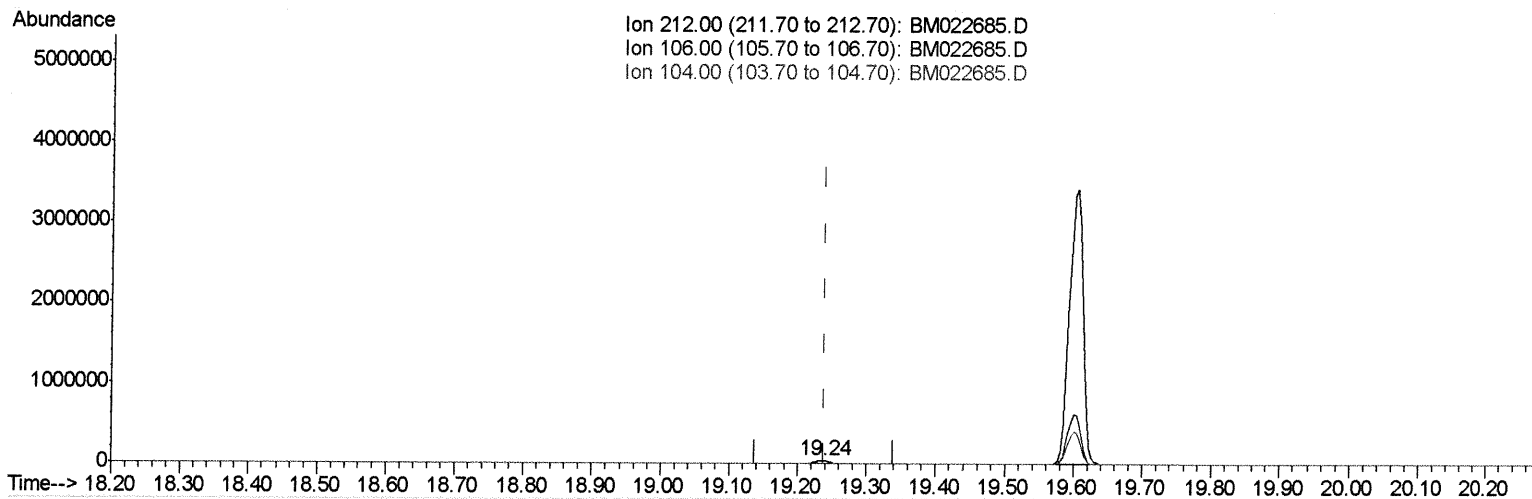

(14) Fluoranthene-d10 (SURR)

19.237min (-0.002) 0.40ng/ul m *JU* 09/17/19

response 48836

Ion	Exp%	Act%
212.00	100	100
106.00	14.00	0.00#
104.00	8.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9

Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:40:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

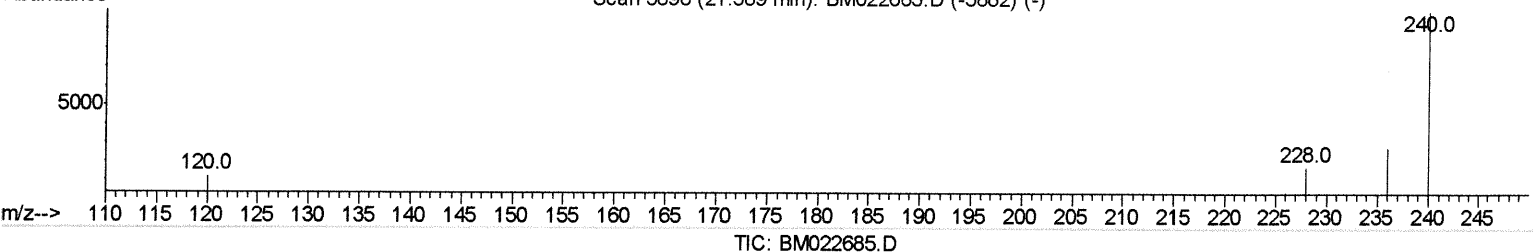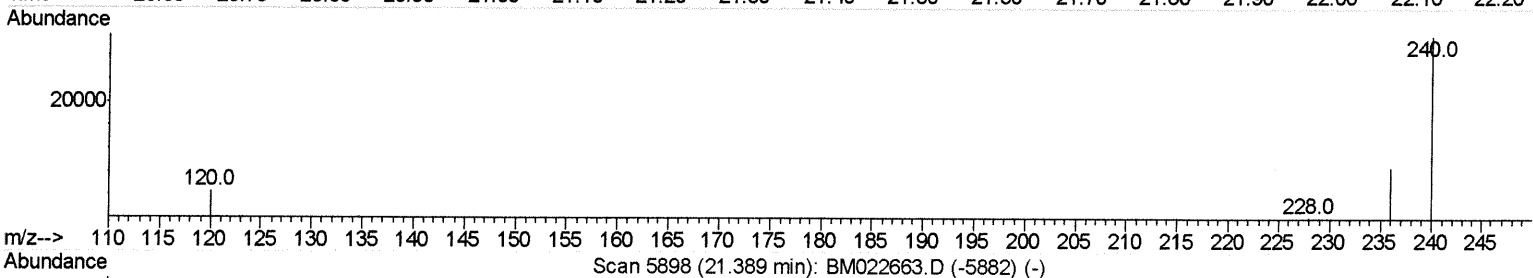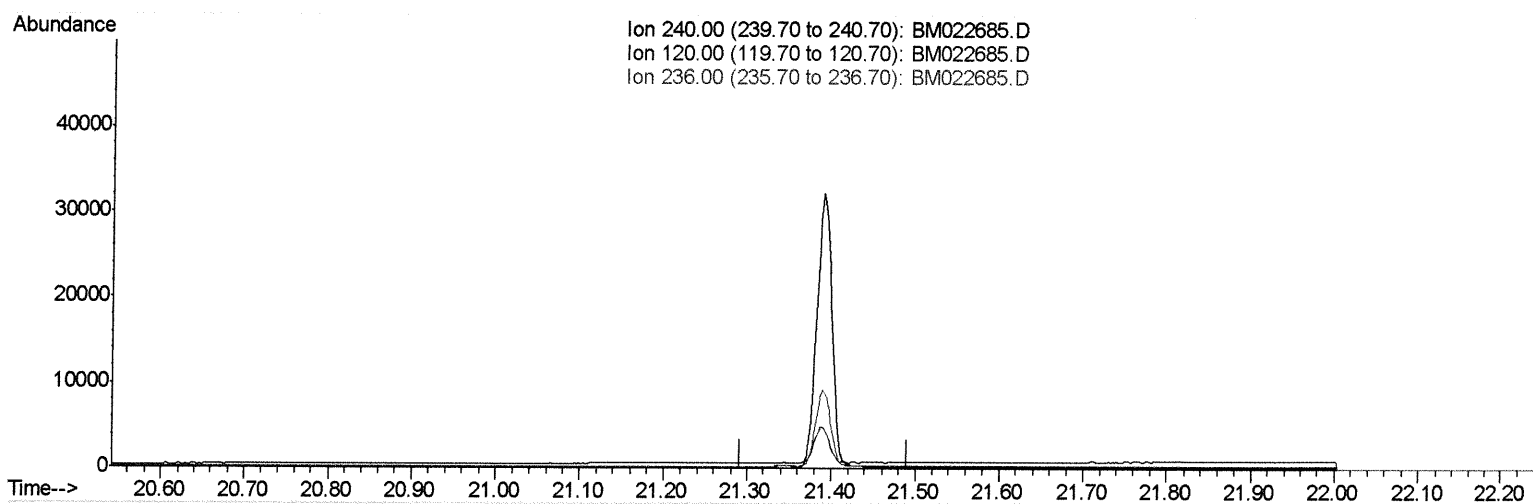

(16) Chrysene-d12 (I)

21.391min (-21.391) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	14.60	0.00#
236.00	28.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9

Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:40:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

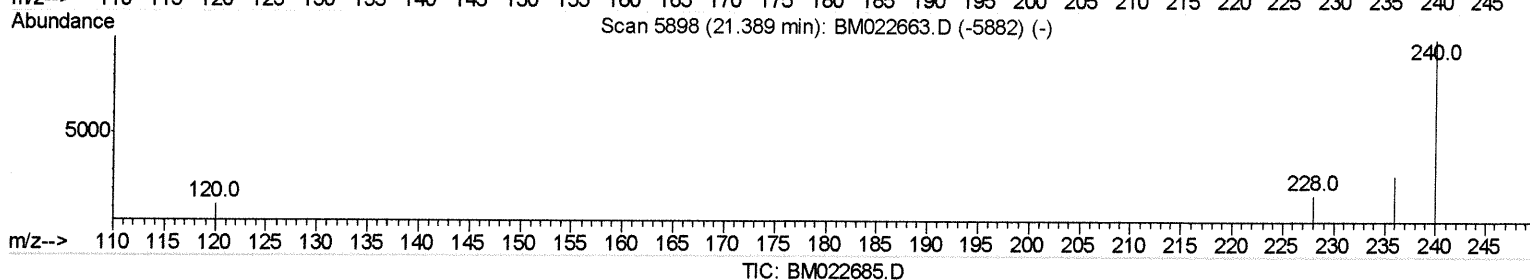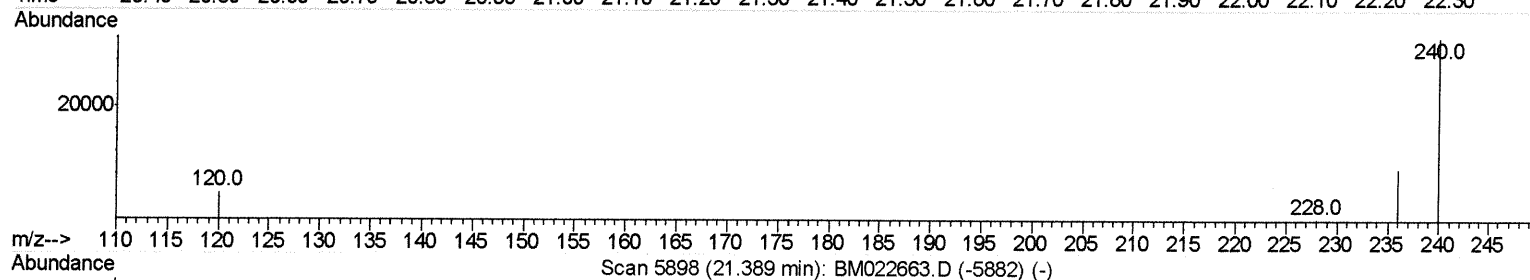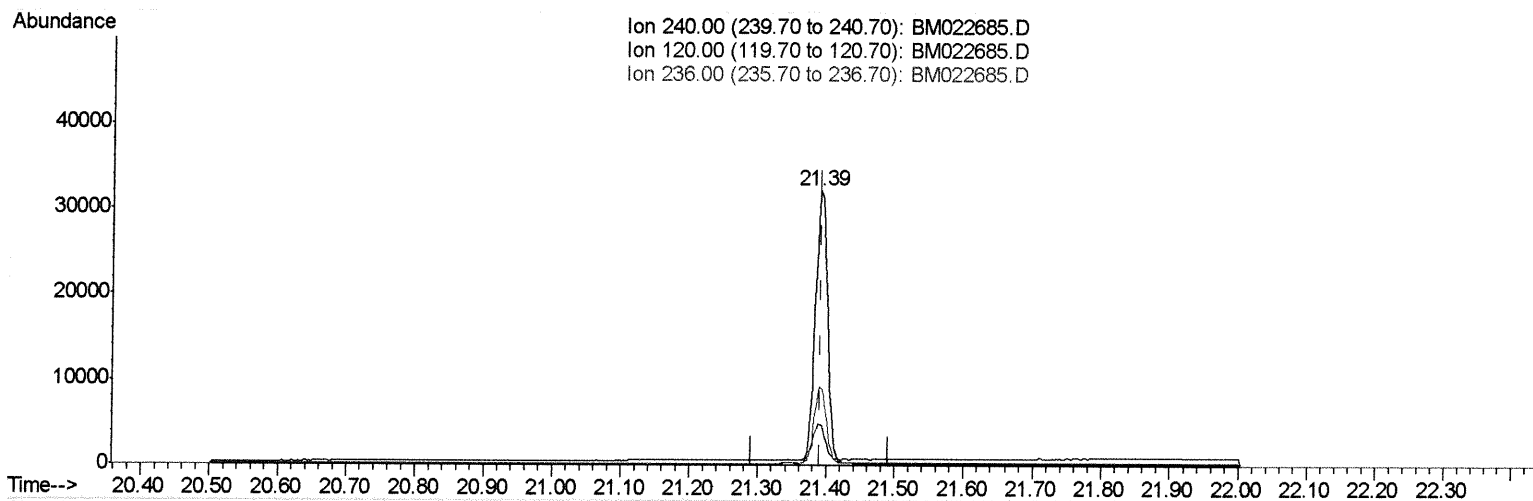

(16) Chrysene-d12 (I)

21.389min (-0.002) 0.40ng/ul m ^{JU} 09/17/19

response 39782

Ion	Exp%	Act%
240.00	100	100
120.00	14.60	15.13
236.00	28.80	28.67
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091619\
 Data File : BM022685.D
 Acq On : 16 Sep 2019 11:30
 Operator : HP/JU
 Sample : K4780-13
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BN9

Manual Integrations
 APPROVED

mohammad
 9/17/2019 4:11:17 PM

Quant Time: Sep 17 01:42:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	8674	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	35902	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	20906	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	44311m →	0.40	ng/ul →	0.00
16) Chrysene-d12	21.39	240	39782m →	0.40	ng/ul →	0.00
20) Perylene-d12	23.67	264	42969	0.40	ng/ul	0.00

JU
 09/17/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.22	152	16518	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	48836m →	0.40	ng/ul →	0.00

JU 09/17/19

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed