
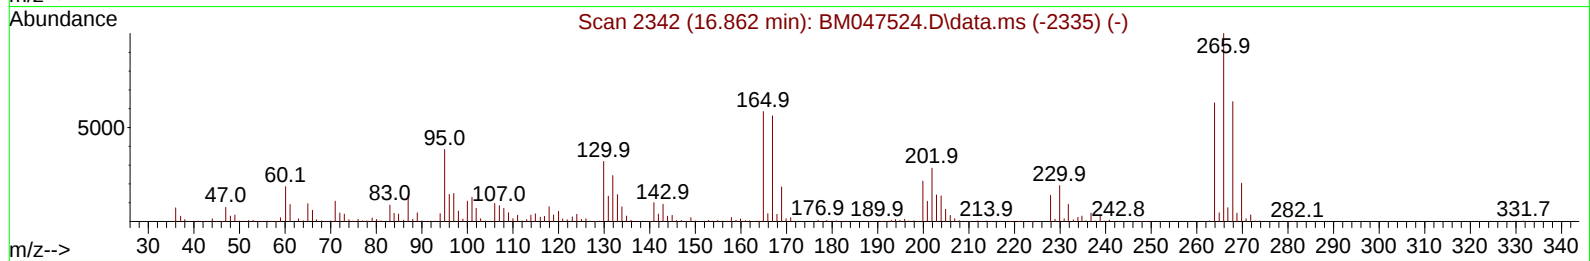
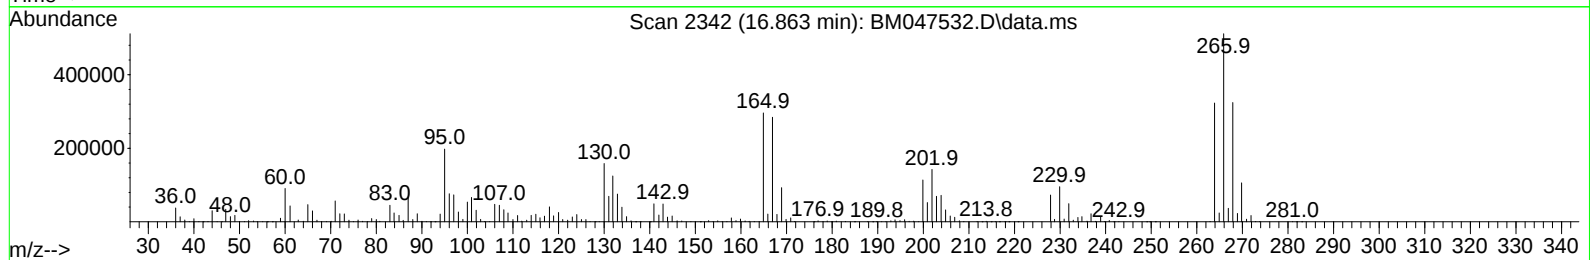


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091624\
Data File : BM047532.D
Acq On : 16 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 11:33:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

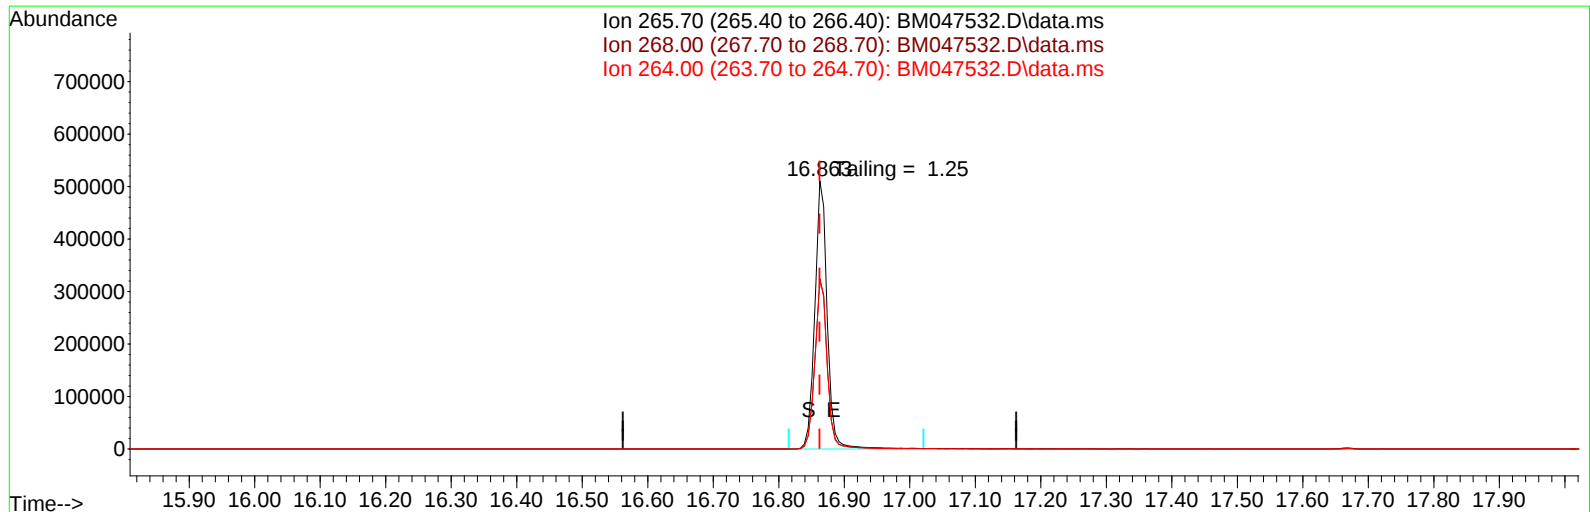

TIC: BM047532.D\data.ms

(70) Pentachlorophenol (C)




16.863min (+ 0.000) 1952988.49 ng

response 672937

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.45
264.00	63.00	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091624\
Data File : BM047532.D
Acq On : 16 Sep 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 11:33:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

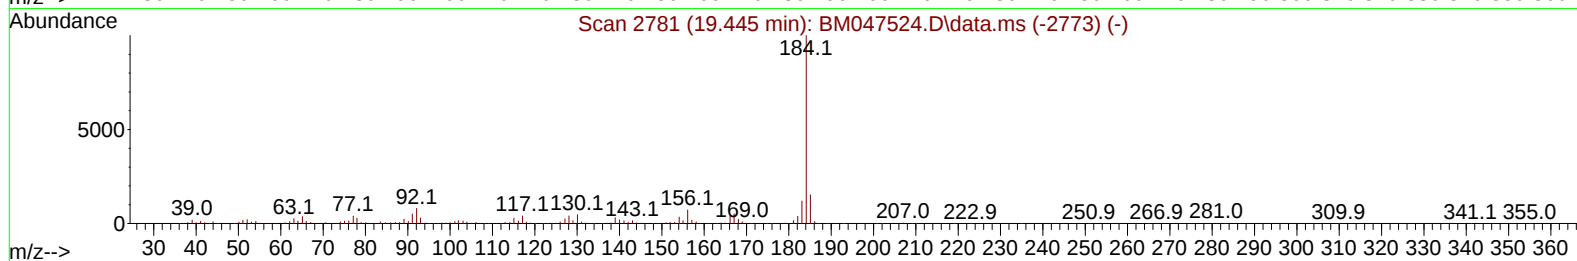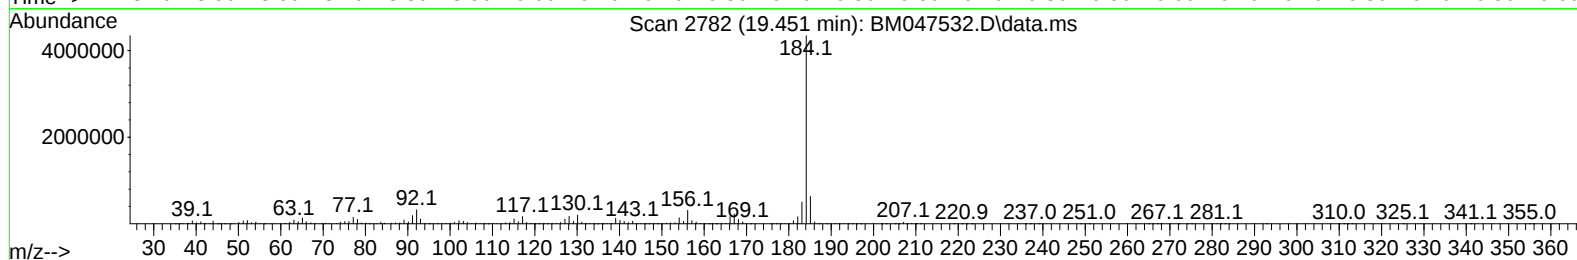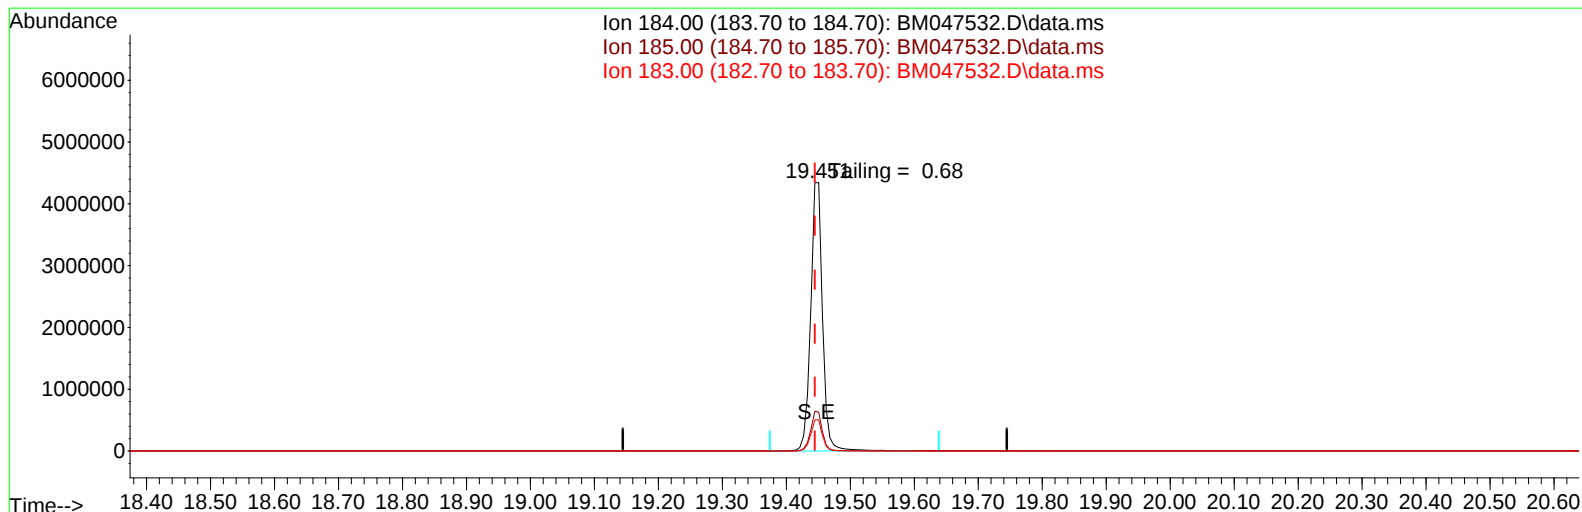

TIC: BM047532.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 33612.78 ng

response 5649482

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.49
183.00	12.00	11.57
0.00	0.00	0.00