

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091719\
 Data File : BM022705.D
 Acq On : 17 Sep 2019 14:06
 Operator : HP/JU
 Sample : K4780-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BM4

Quant Time: Sep 17 17:52:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	11108	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	46625	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	28407	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	4478528	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.39
20) Perylene-d12	23.66	264	46025	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	20816	0.27	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.46	166	7849	0.062	ng/ul#	13
21) Benzo(b)fluoranthene	22.98	252	9503	0.048	ng/ul#	1
22) Benzo(k)fluoranthene	22.98	252	9483	0.046	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM091719\
Data File : BM022705.D
Acq On : 17 Sep 2019 14:06
Operator : HP/JU
Sample : K4780-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BM4

Quant Time: Sep 17 17:52:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

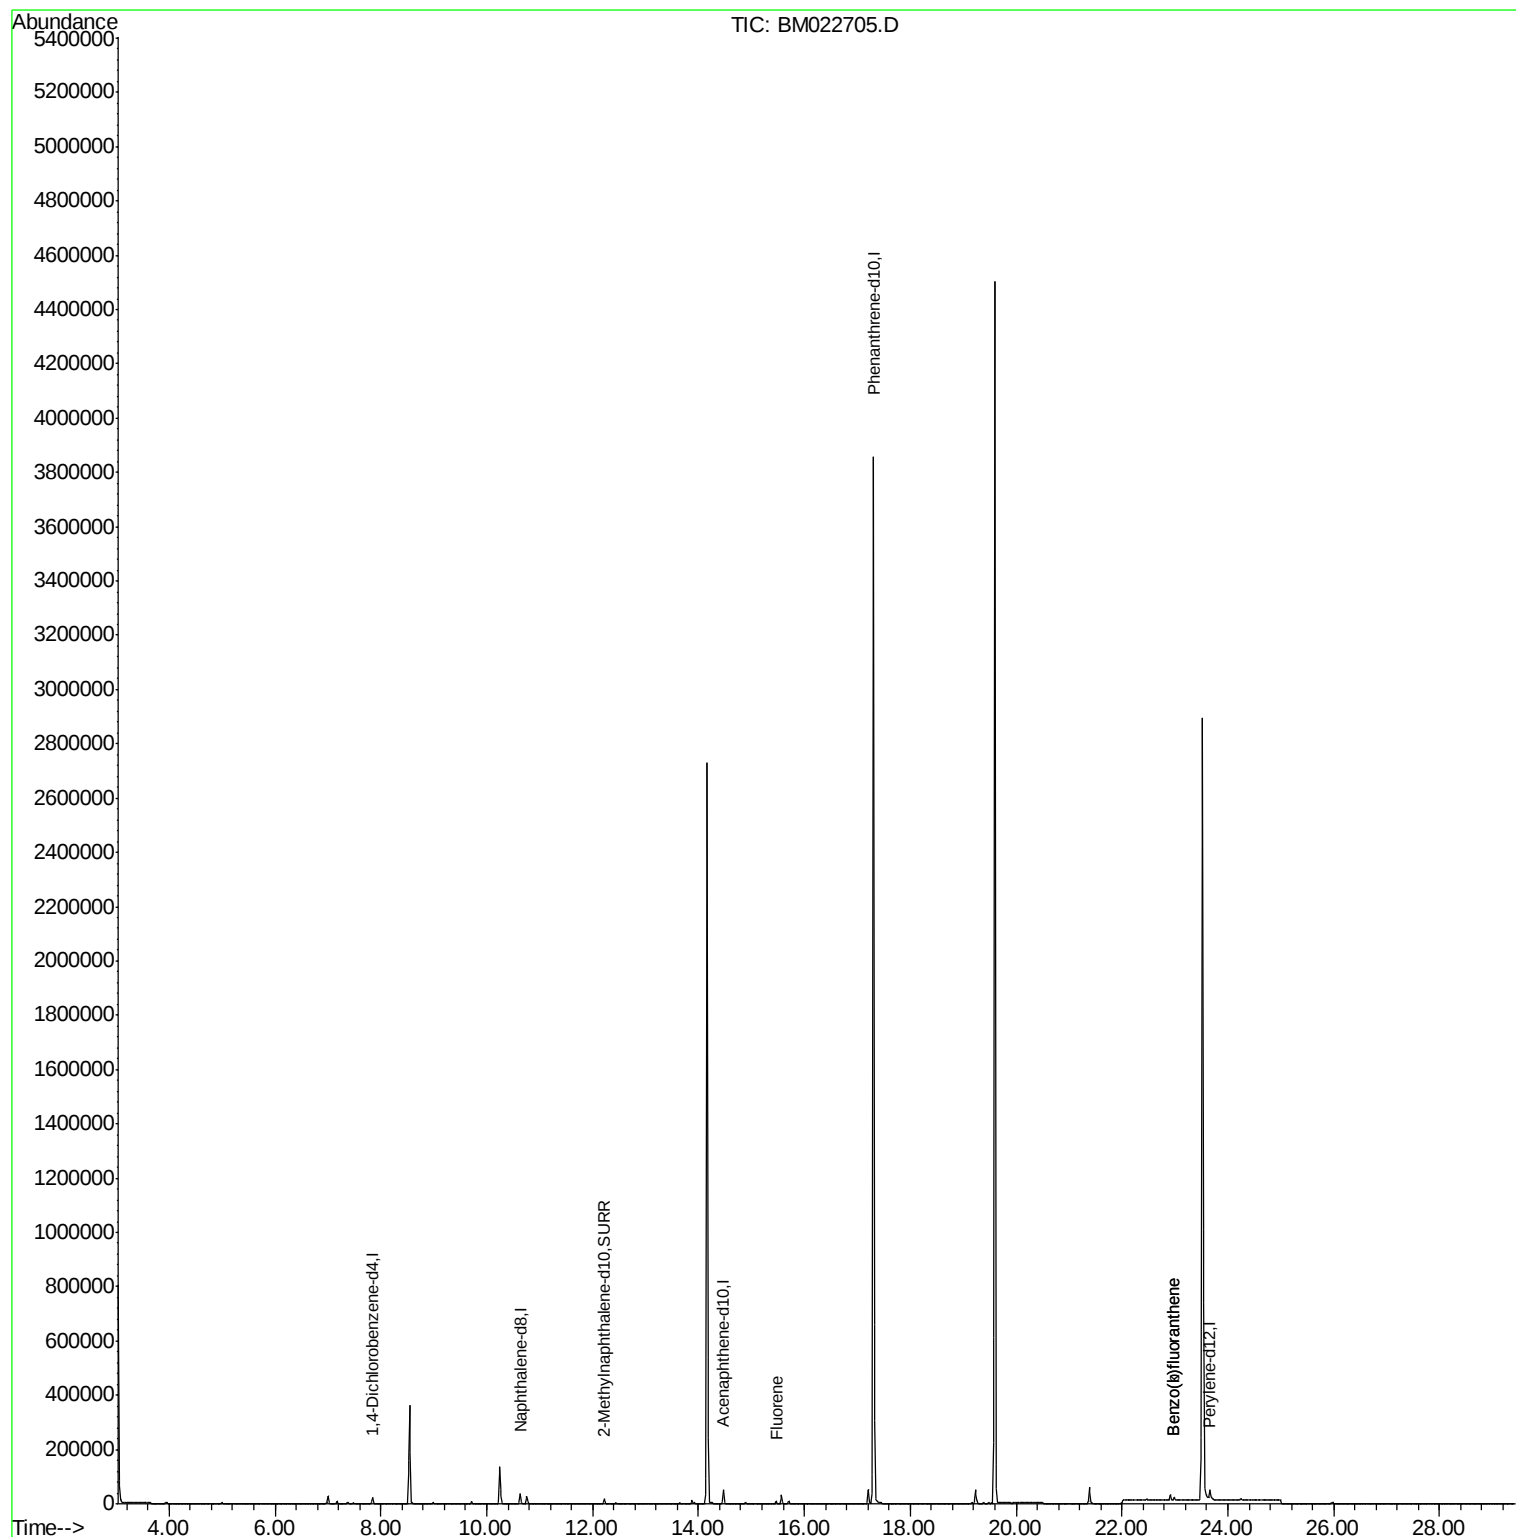

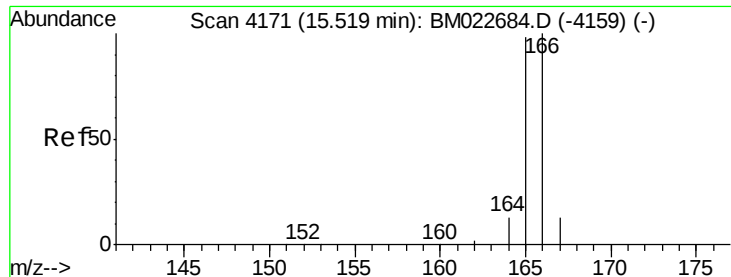

#9

Fluorene

Concen: 0.062 ng/ul

RT: 15.46 min Scan# 4156

Delta R.T. -0.06 min

Lab File: BM022705.D

Acq: 17 Sep 2019 14:06

Instrument :

BNA_M

ClientSampleId :

H0BM4


Tgt Ion:166 Resp: 7849

Ion Ratio Lower Upper

166 100

165 5.3 78.2 117.2#




167 30.7 10.8 16.2#

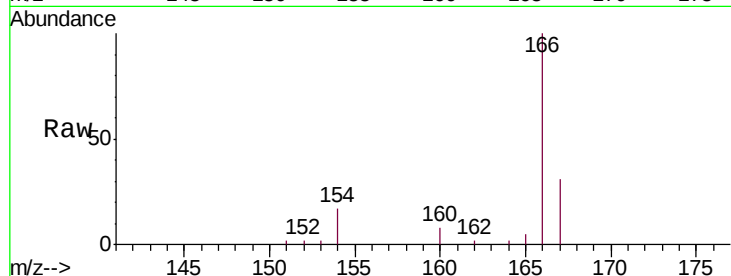

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

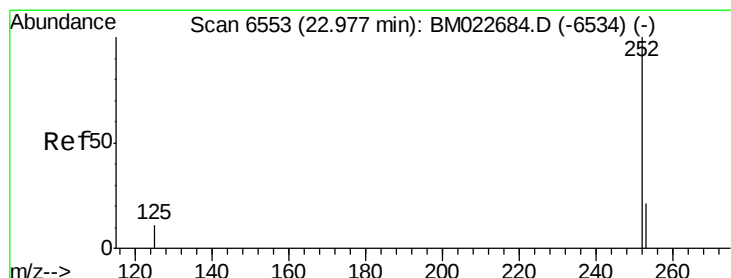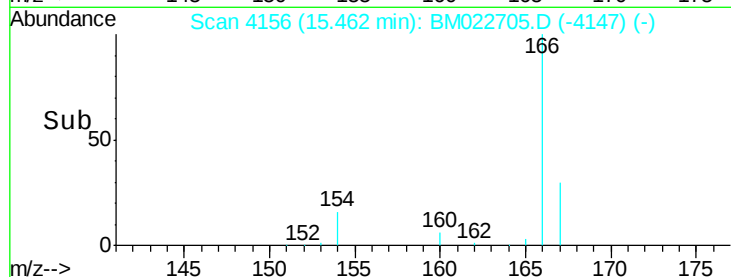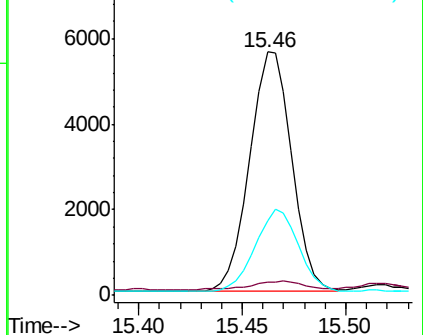

#21

Benzo(b)fluoranthene

Concen: 0.048 ng/ul

RT: 22.98 min Scan# 6553

Delta R.T. -0.01 min

Lab File: BM022705.D

Acq: 17 Sep 2019 14:06


Tgt Ion:252 Resp: 9503

Ion Ratio Lower Upper

252 100

253 54.0 0.0 48.4#



125 113.3 0.0 31.2#



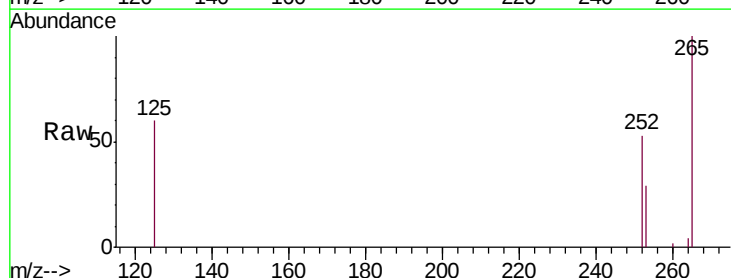


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

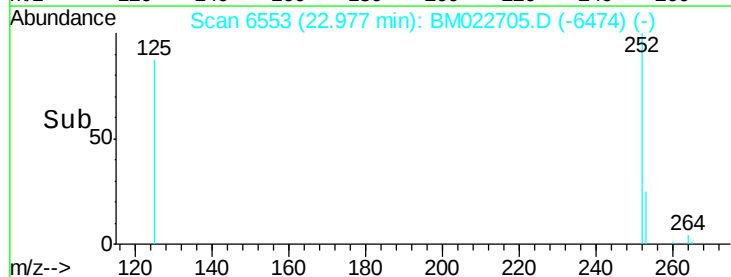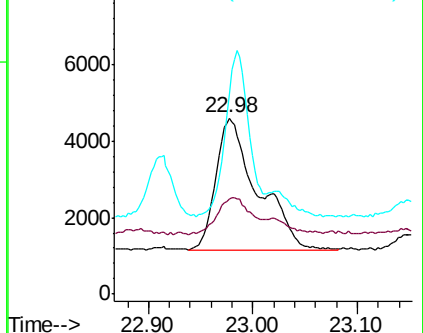

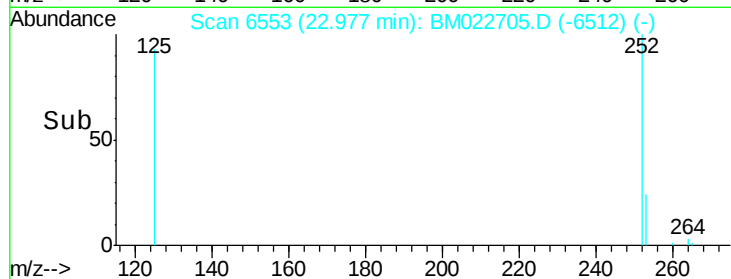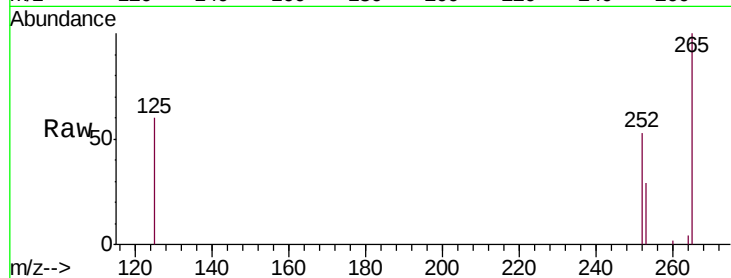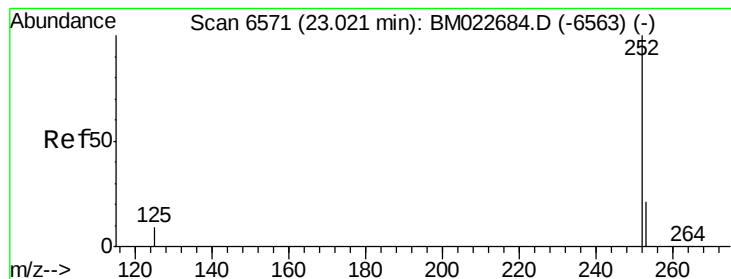

#22

Benzo(k)fluoranthene

Concen: 0.046 ng/ul

RT: 22.98 min Scan# 6553

Delta R.T. -0.05 min

Lab File: BM022705.D

Acq: 17 Sep 2019 14:06

Instrument :

BNA_M

ClientSampleId :

H0BM4

Tgt Ion: 252 Resp: 9483

Ion Ratio Lower Upper

252 100

253 54.0 19.5 29.3#

125 113.3 11.2 16.8#

