



Benzoic acid

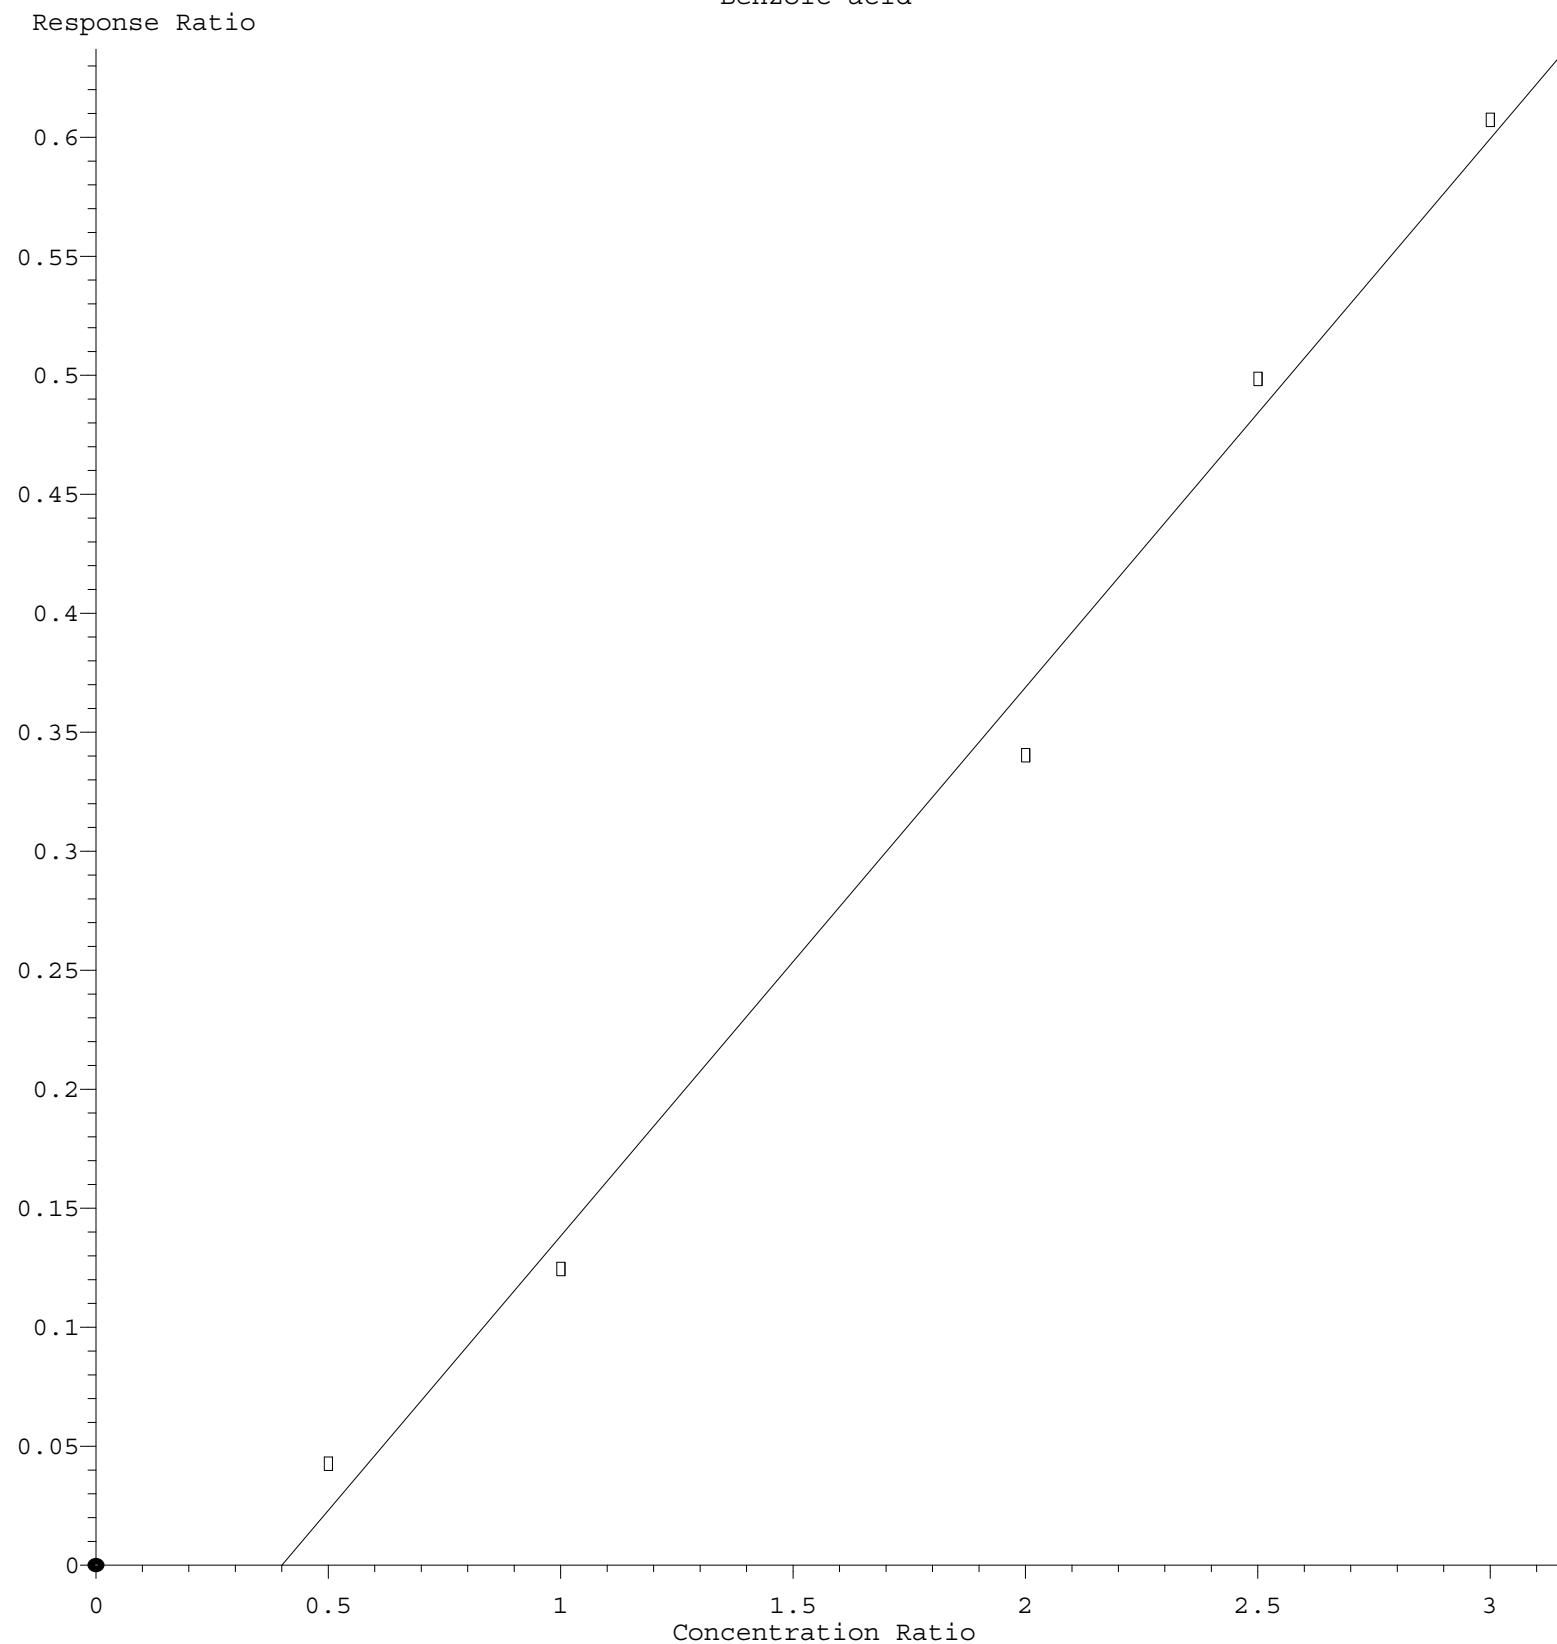

Response = 2.304e-001 * Amt - 9.212e-002
 Coef of Det (r^2) = 0.992794 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM091720.M
 Calibration Table Last Updated: Thu Sep 17 20:07:45 2020


2,4-Dinitrophenol

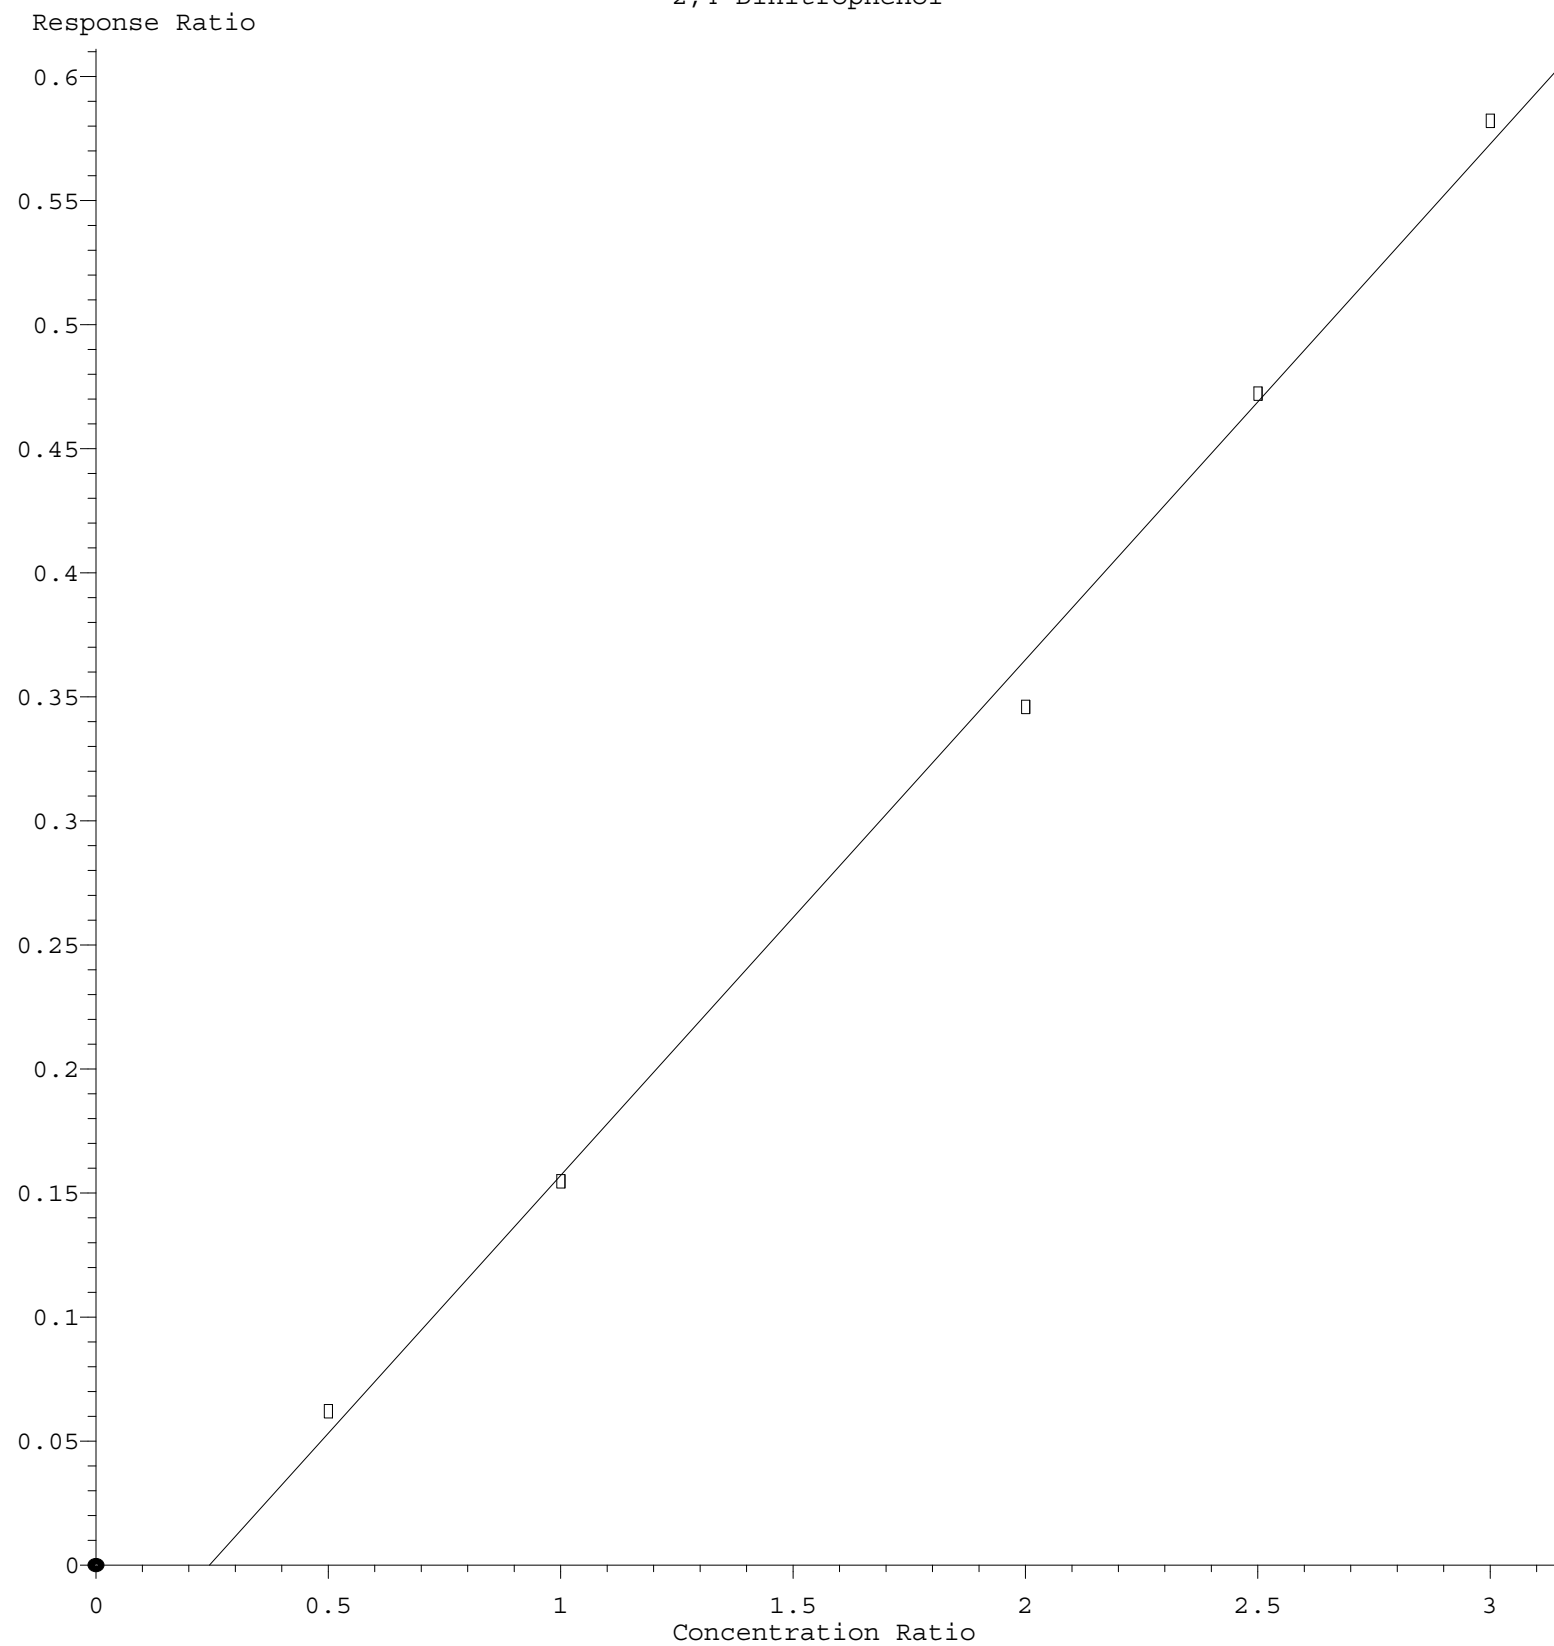

Response = $2.079 \times 10^{-1} \times \text{Amt} - 5.079 \times 10^{-2}$
Coef of Det (r^2) = 0.997072 Curve Fit: Linear
Method Name: Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM091720.M
Calibration Table Last Updated: Thu Sep 17 20:07:45 2020

4-Nitroaniline

Response Ratio

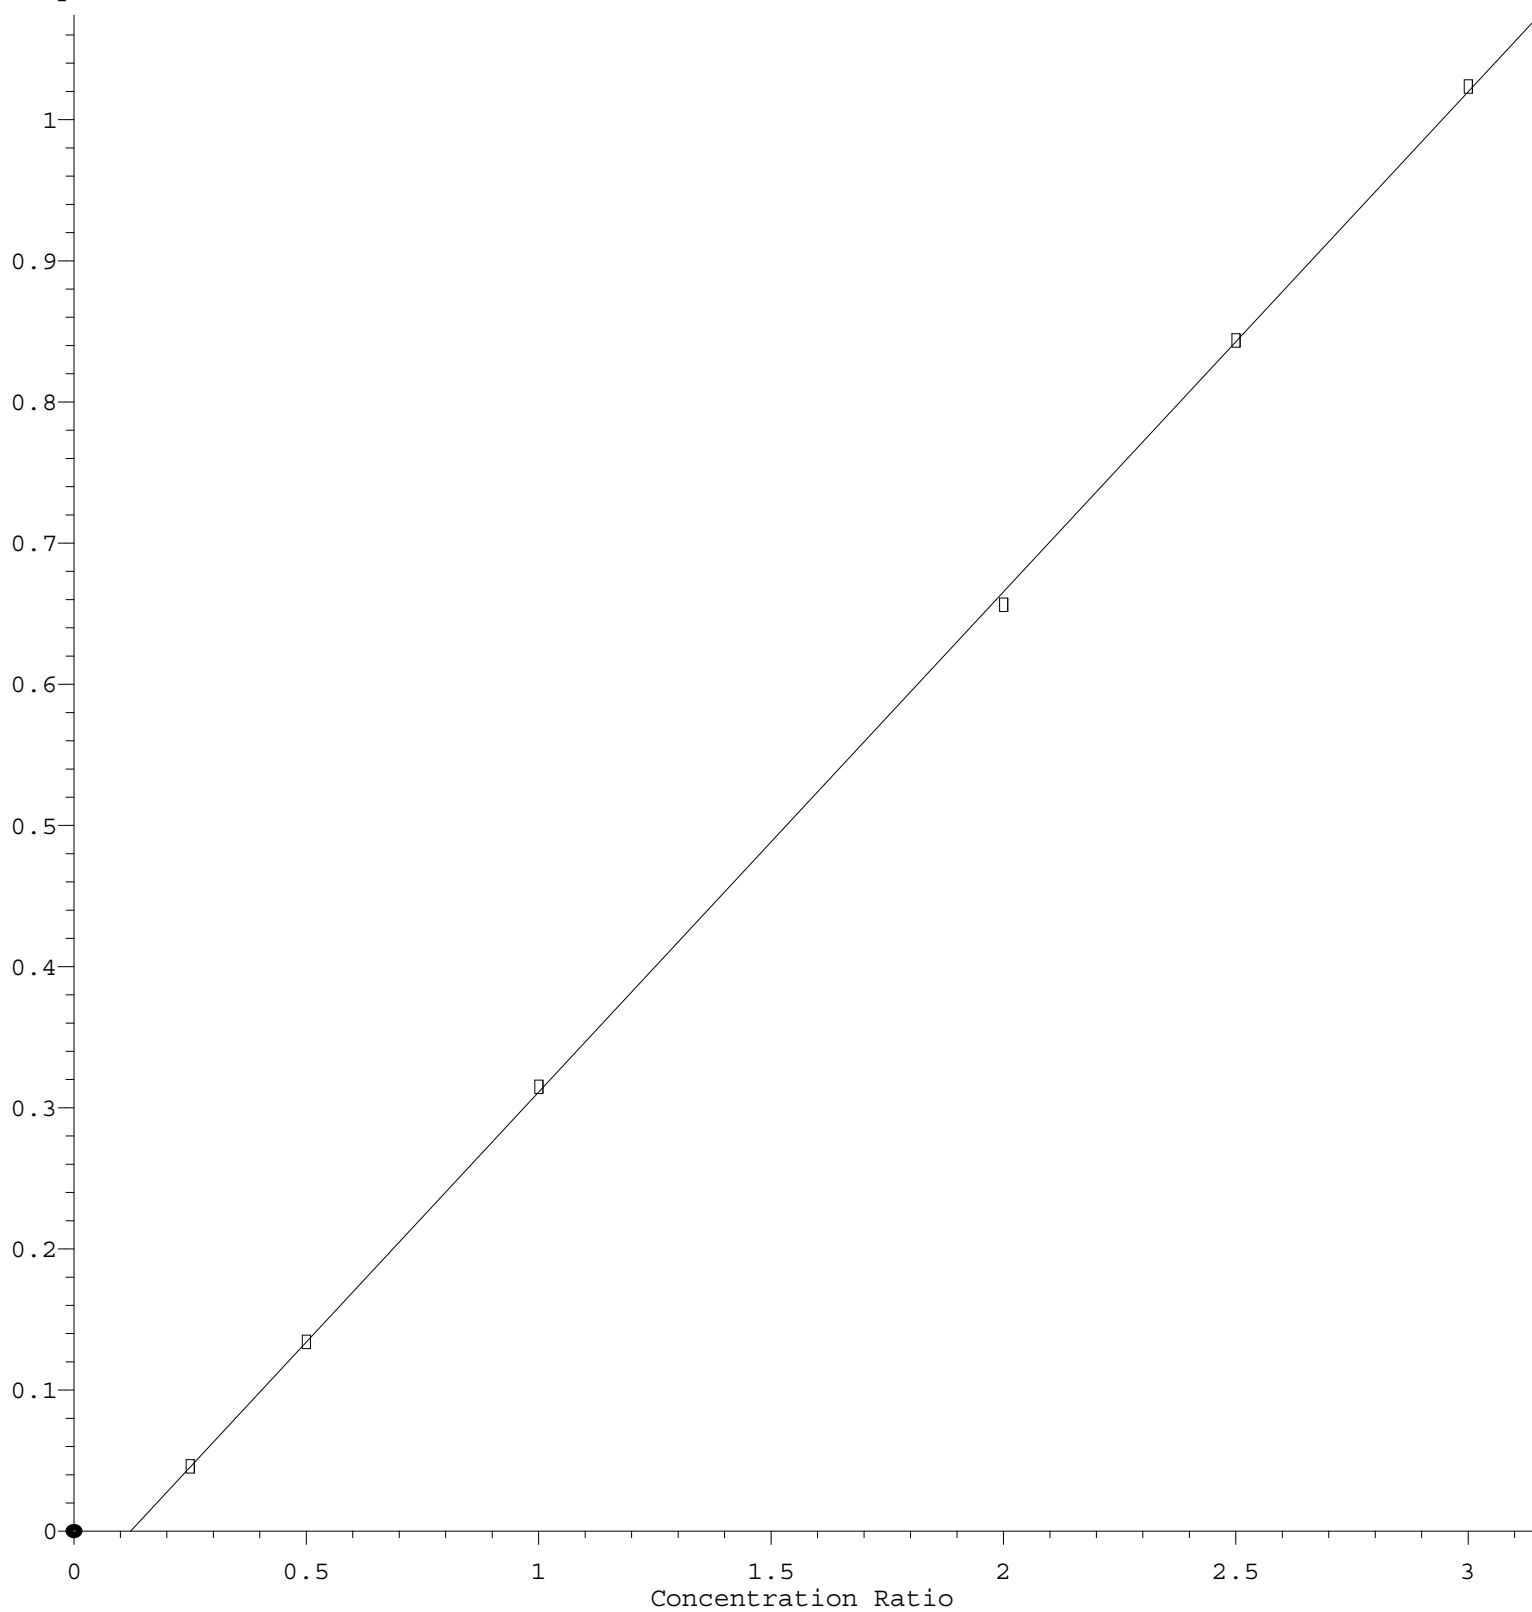

$$\text{Response} = 3.542\text{e-}001 * \text{Amt} - 4.304\text{e-}002$$


Coef of Det (r^2) = 0.999858 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM091720.M

Calibration Table Last Updated: Thu Sep 17 20:07:45 2020

Benzidine

Response Ratio

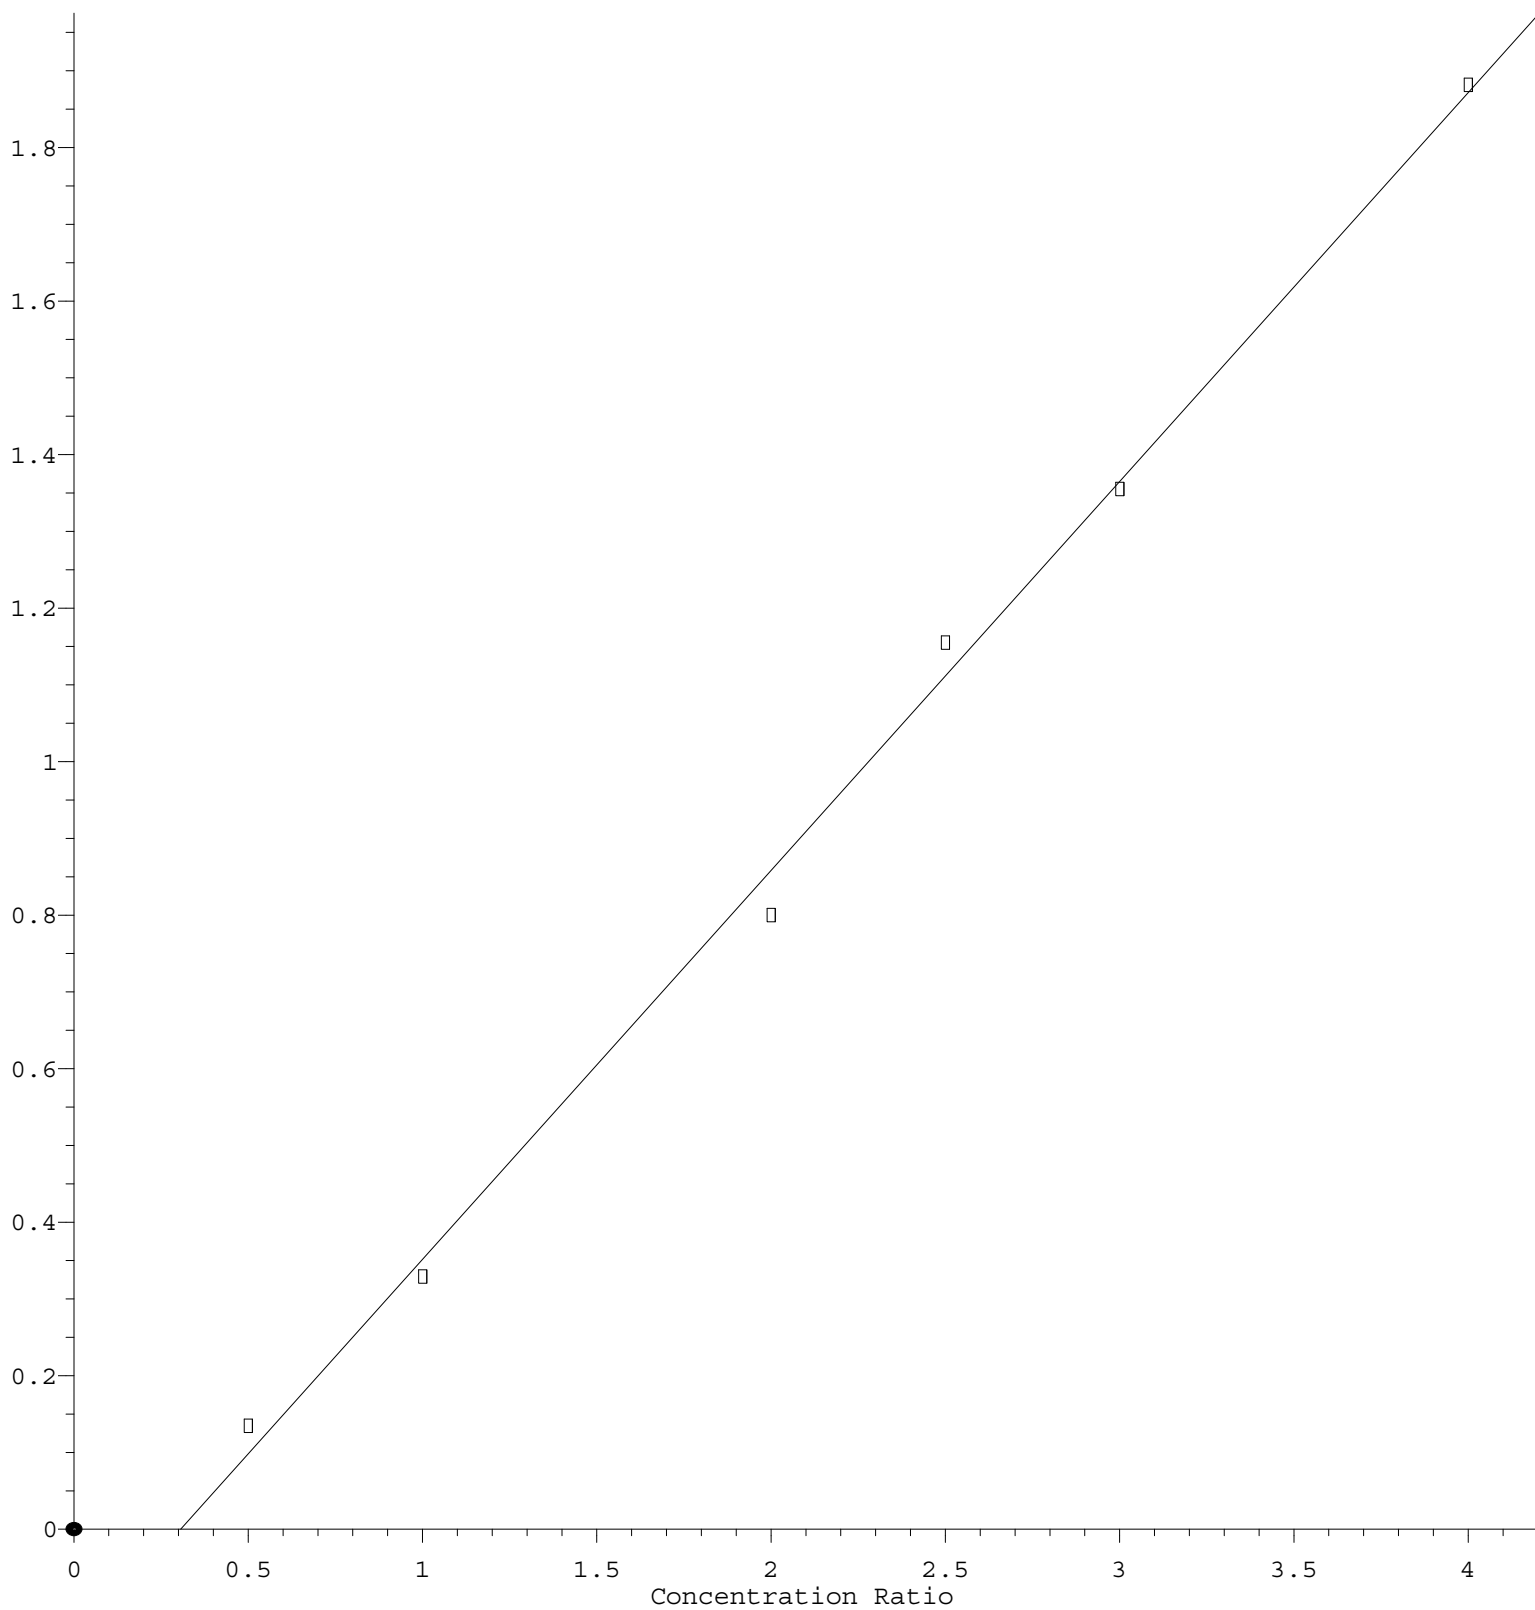

$$\text{Response} = 5.066\text{e-}001 * \text{Amt} - 1.551\text{e-}001$$

Coef of Det (r^2) = 0.996589 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM091720.M

Calibration Table Last Updated: Thu Sep 17 20:07:45 2020