


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091720\
Data File : BM027447.D
Acq On : 17 Sep 2020 15:03
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM091720.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 17 20:07:45 2020

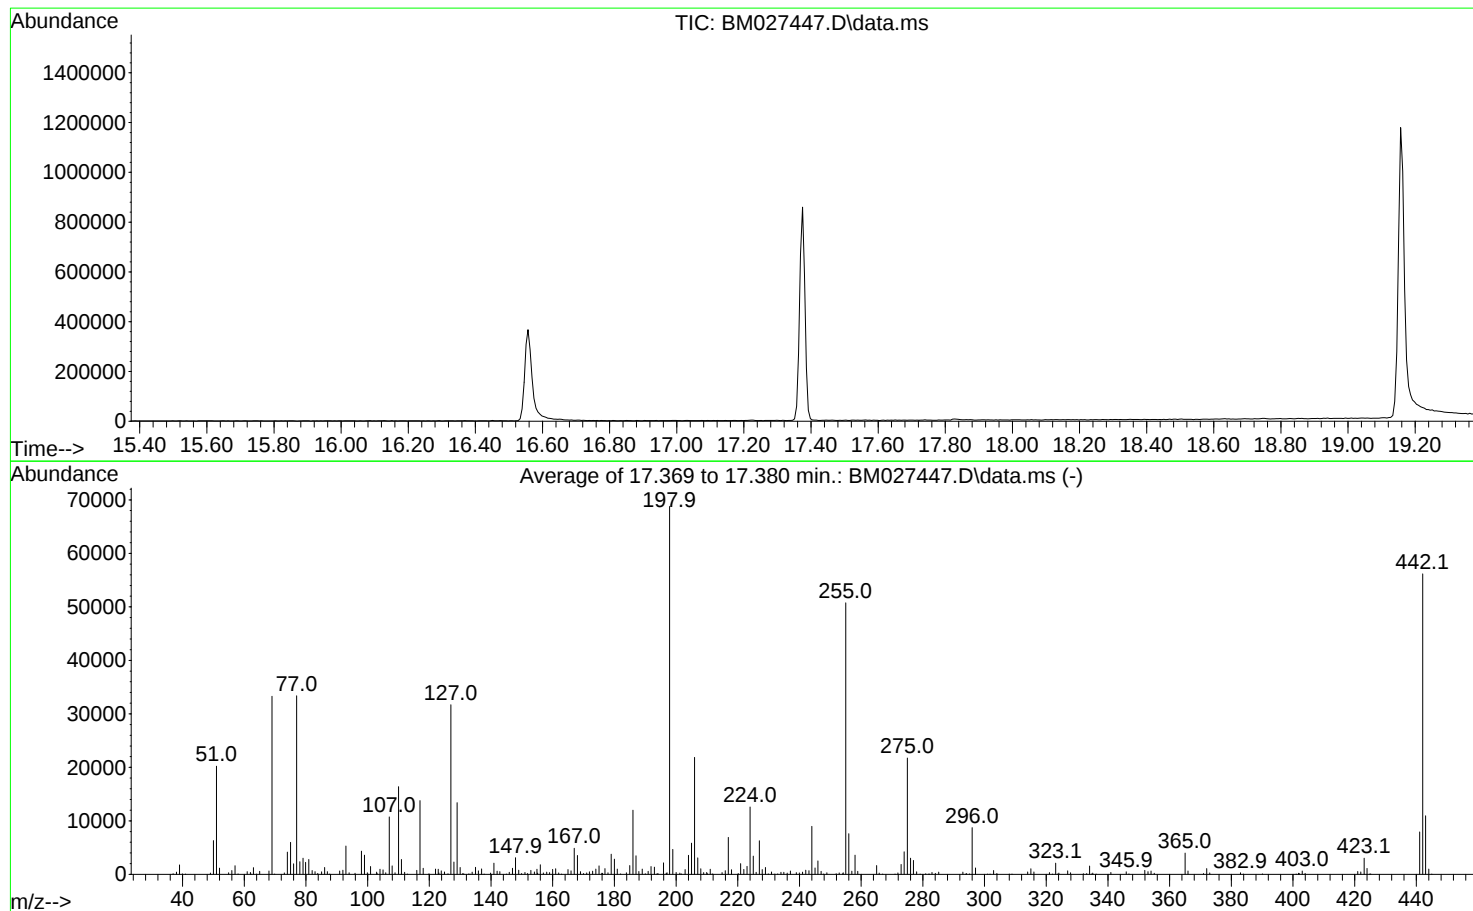

AutoFind: Scans 2445, 2446, 2447; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	20223	PASS
68	69	0.00	2	1.9	620	PASS
69	198	0.00	100	48.4	33299	PASS
70	69	0.00	2	0.2	65	PASS
127	198	10	80	46.1	31701	PASS
197	198	0.00	2	0.4	306	PASS
198	198	100	100	100.0	68765	PASS
199	198	5	9	6.8	4666	PASS
275	198	10	60	31.6	21739	PASS
365	198	1	100	5.8	3968	PASS
441	198	0.01	100	11.5	7941	PASS
442	198	50	100	81.7	56187	PASS
443	442	15	24	19.5	10952	PASS