
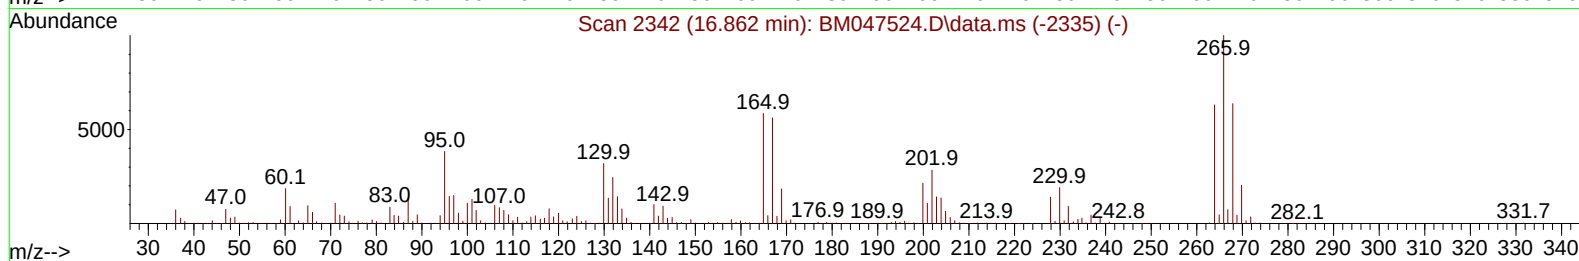
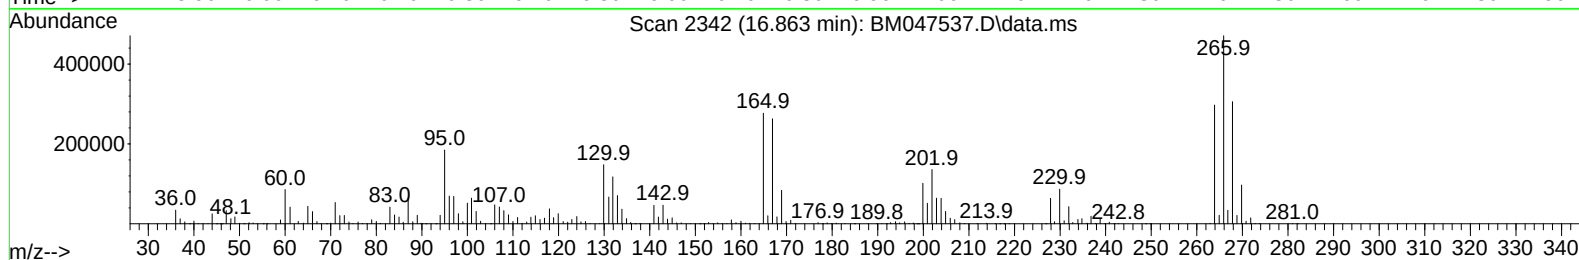


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM091724\  
Data File : BM047537.D  
Acq On : 17 Sep 2024 08:05  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 11:12:06 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM091424.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Sep 15 08:56:37 2024  
Response via : Initial Calibration

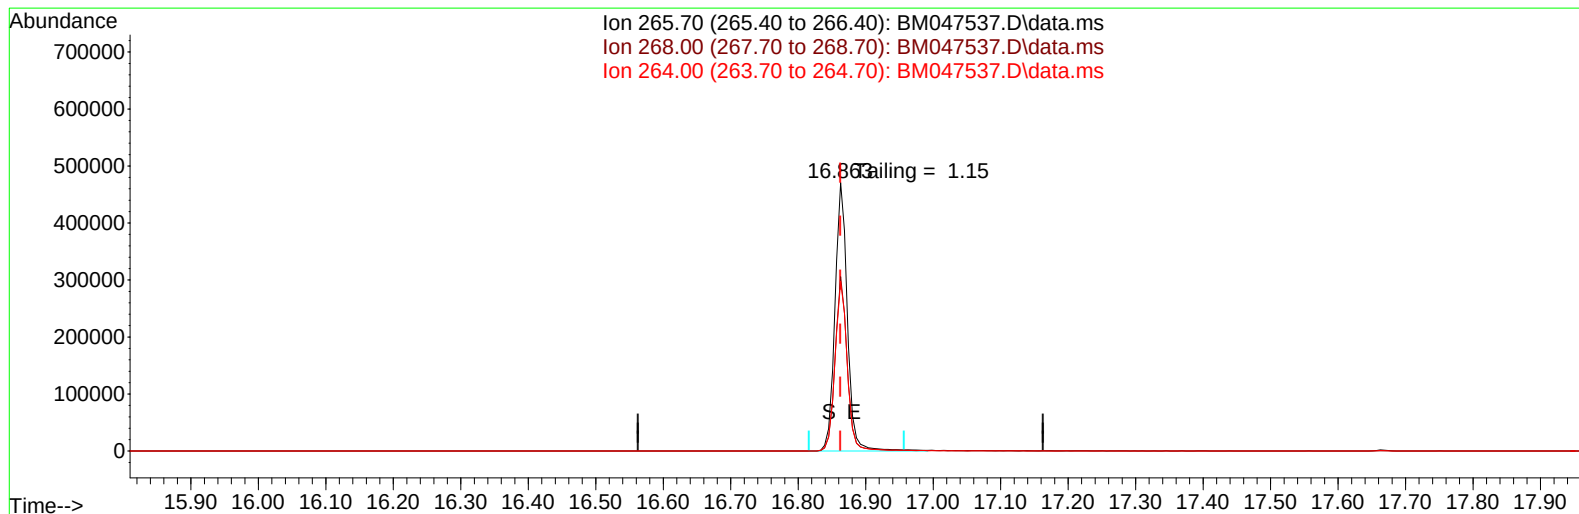

TIC: BM047537.D\data.ms

**(70) Pentachlorophenol (C)**




16.863min (+ 0.000) 1274585.83 ng

response 601841

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.70  | 64.96  |
| 264.00 | 63.00  | 63.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM091724\  
Data File : BM047537.D  
Acq On : 17 Sep 2024 08:05  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 11:12:06 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM091424.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sun Sep 15 08:56:37 2024  
Response via : Initial Calibration

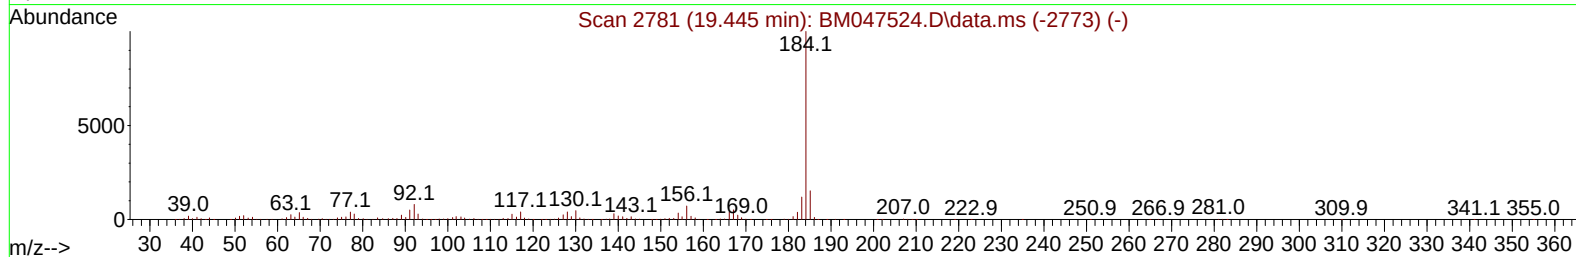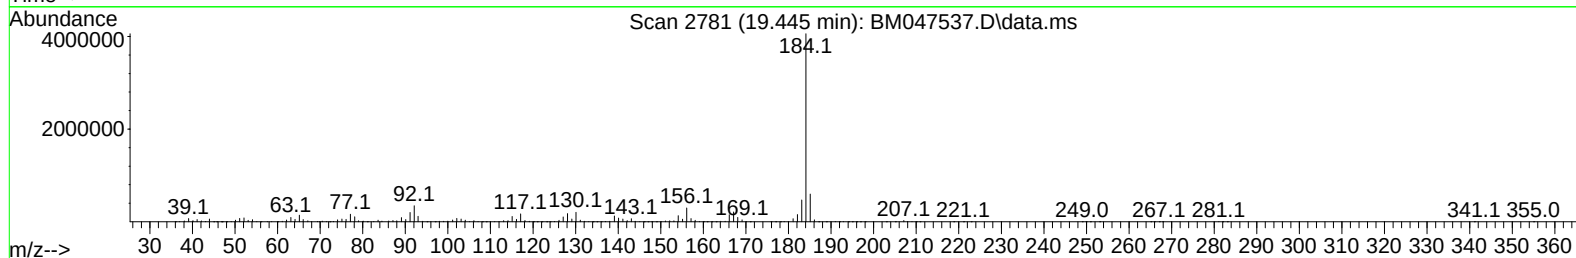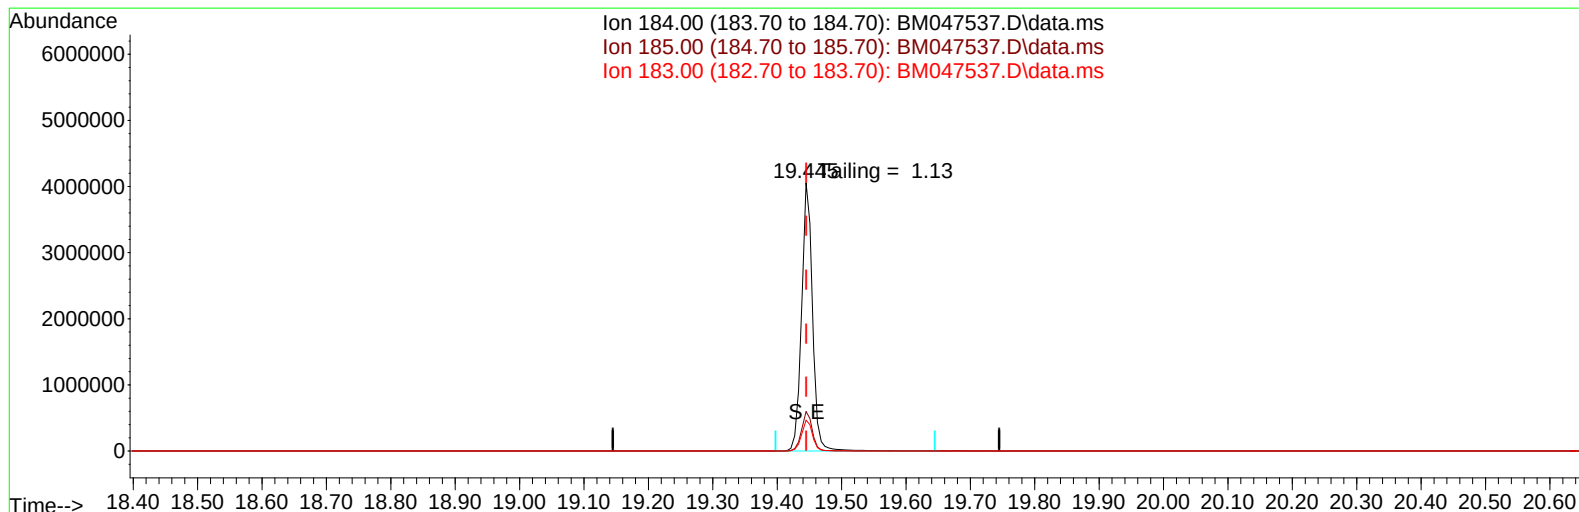

TIC: BM047537.D\data.ms

**(77) Benzidine**

19.445min (-0.000) 68077.98 ng m

response 4801635

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.73  |
| 183.00 | 12.00  | 11.55  |
| 0.00   | 0.00   | 0.00   |