
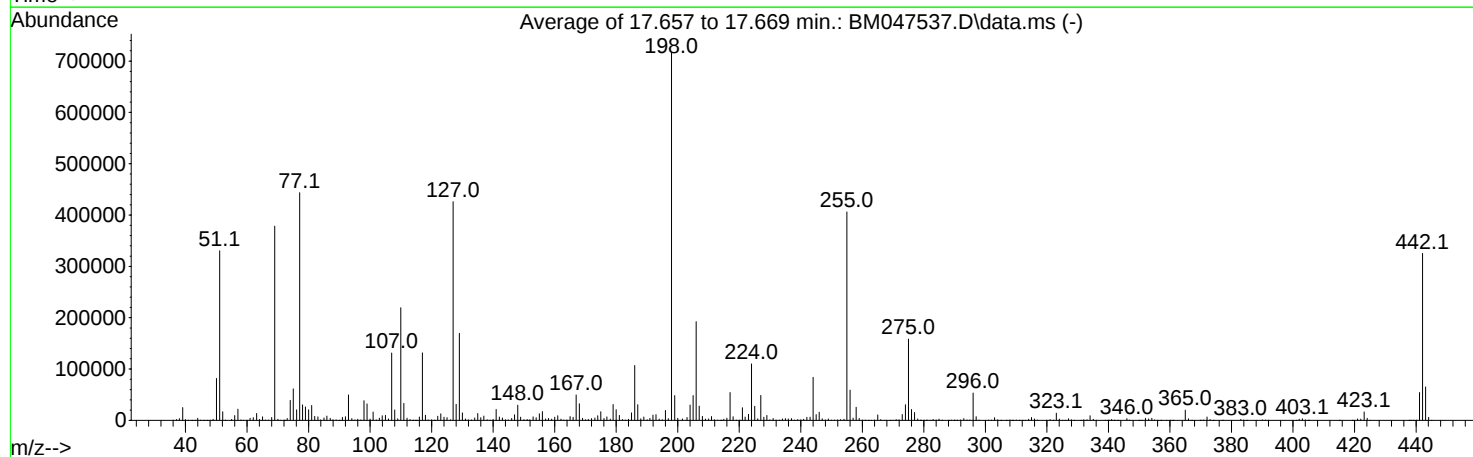


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091724\
Data File : BM047537.D
Acq On : 17 Sep 2024 08:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Sep 15 08:56:37 2024

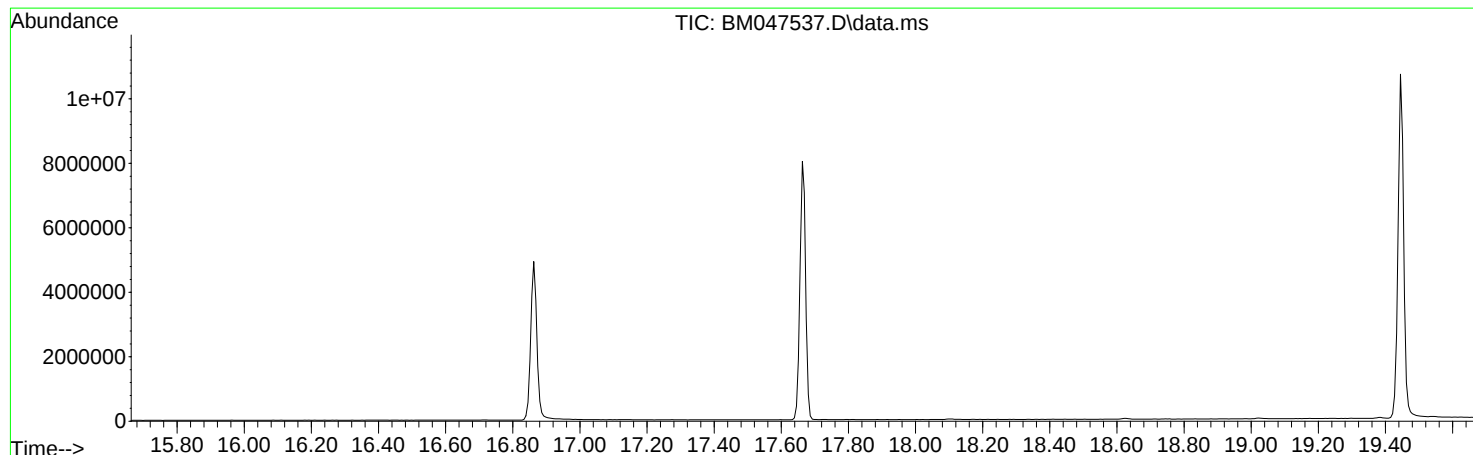

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	330476	PASS
68	69	0.00	2	1.5	5626	PASS
69	198	0.00	100	52.8	378517	PASS
70	69	0.00	2	0.6	2146	PASS
127	198	10	80	59.4	426069	PASS
197	198	0.00	2	0.5	3503	PASS
198	198	100	100	100.0	716715	PASS
199	198	5	9	6.8	48507	PASS
275	198	10	60	22.1	158253	PASS
365	198	1	100	2.8	19878	PASS
441	198	0.01	100	7.6	54272	PASS
442	442	50	100	100.0	325461	PASS
443	442	15	24	20.0	65093	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/17/2024	BNA_M	<u>BM047537.D</u>
Compound Name	Response	Retention Time
DDT	2033083	20.68
DDD	16098	20.298
DDE	1245	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17343	2050426	0.85

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091724\
Data File : BM047537.D
Acq On : 17 Sep 2024 08:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 17 11:12:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

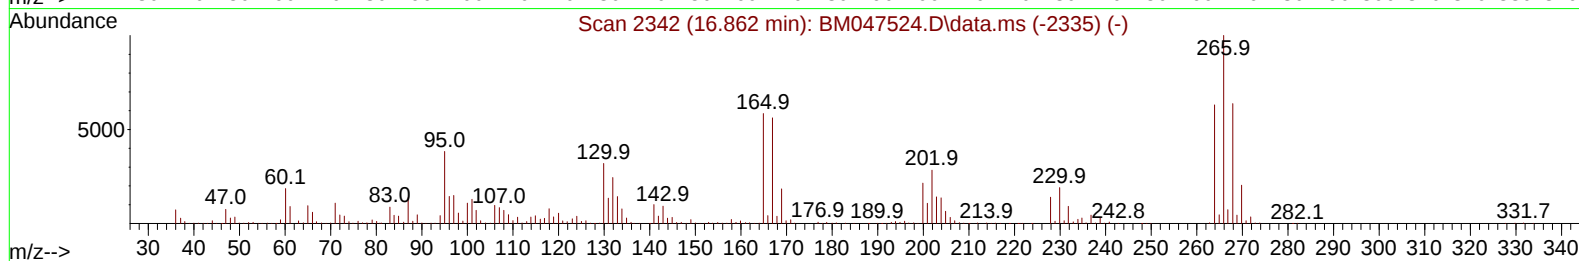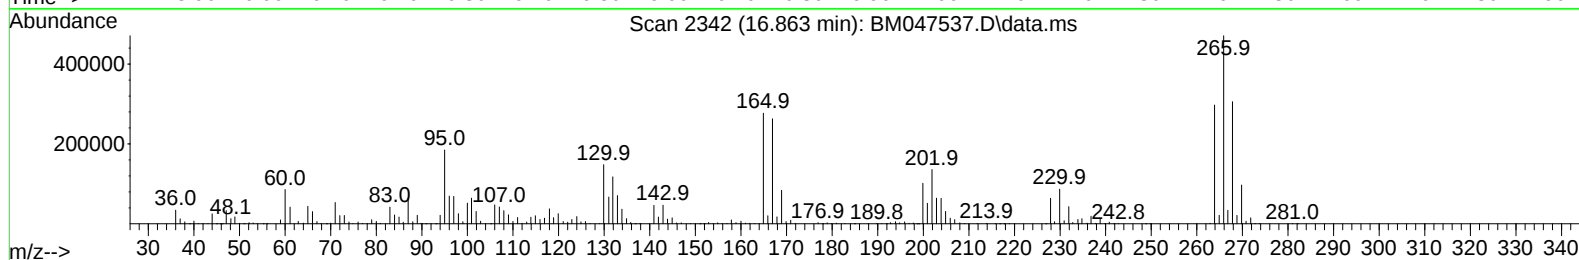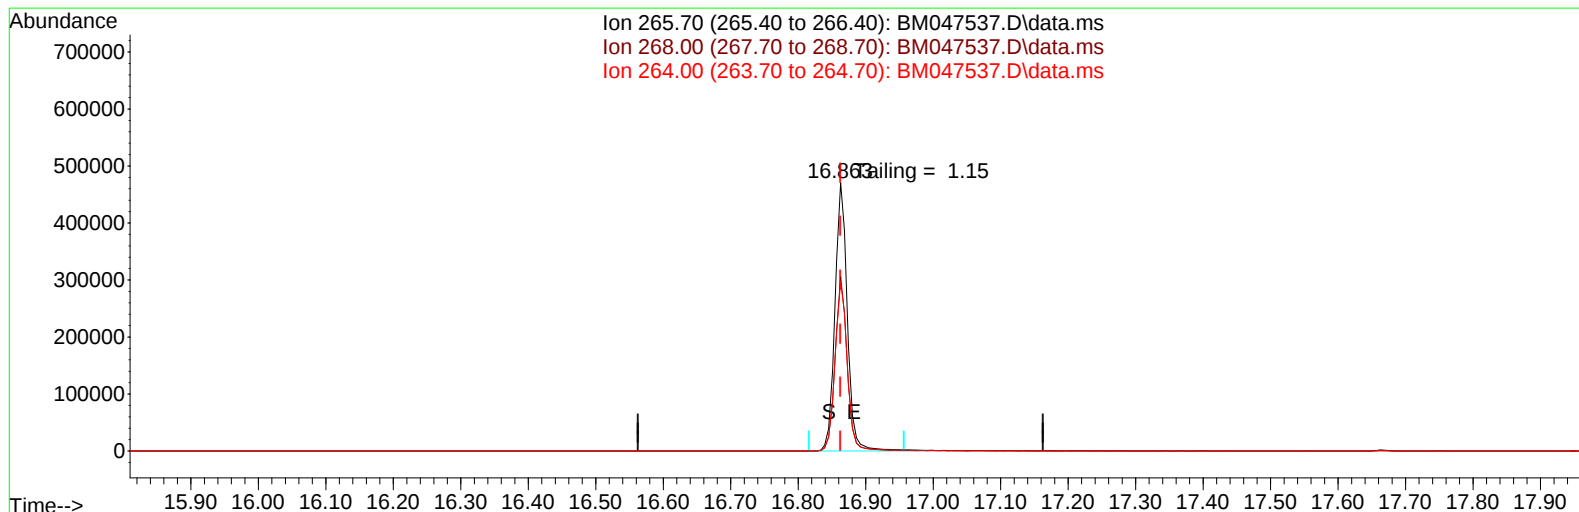

TIC: BM047537.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.000) 1274585.83 ng




response 601841

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.96
264.00	63.00	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091724\
Data File : BM047537.D
Acq On : 17 Sep 2024 08:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 17 11:12:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

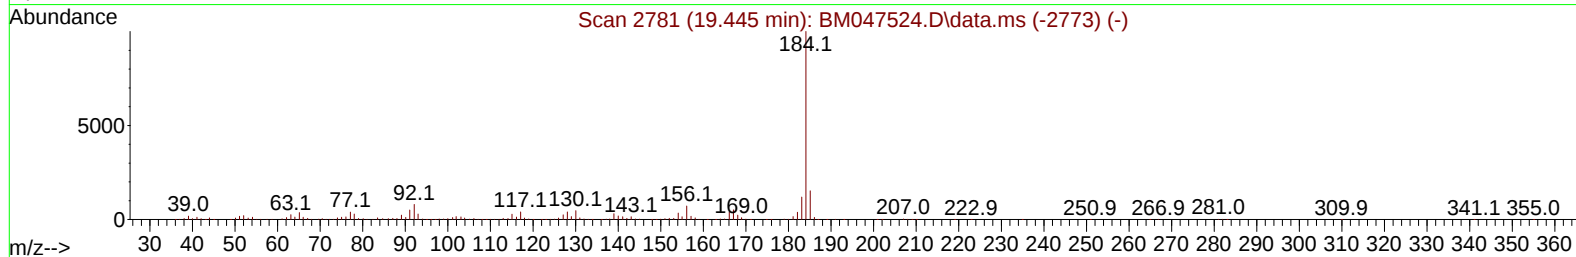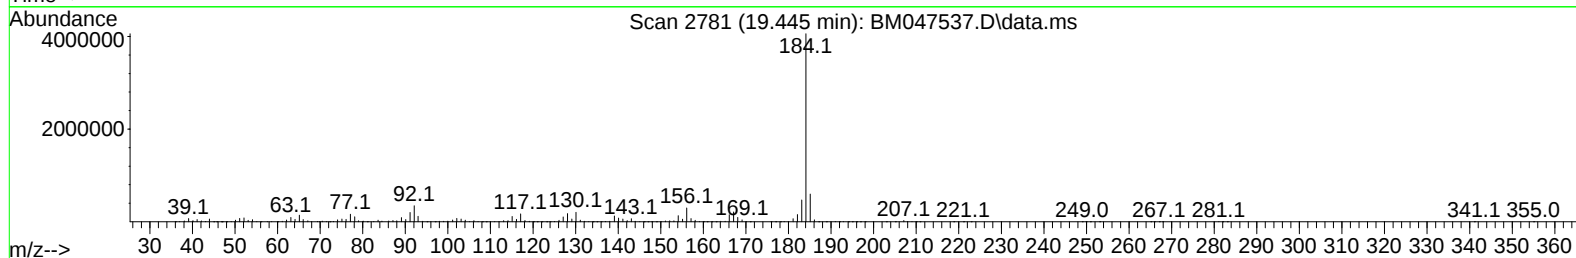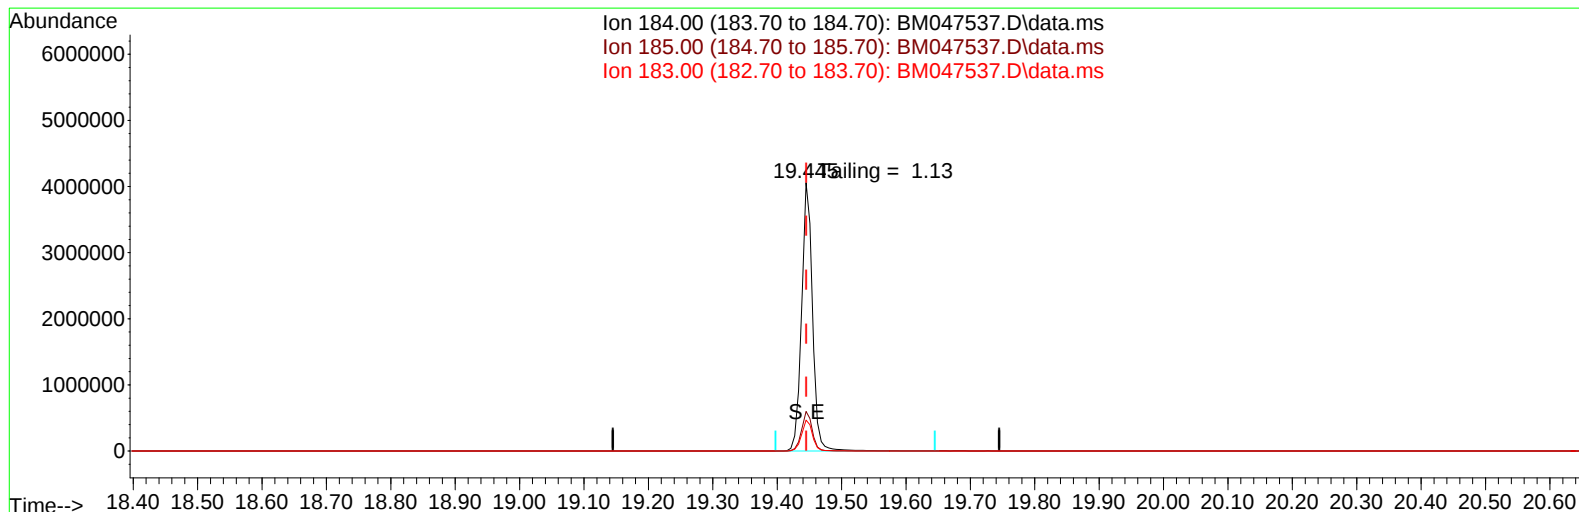

TIC: BM047537.D\data.ms

(77) Benzidine

19.445min (-0.000) 68077.98 ng m

response 4801635

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.73
183.00	12.00	11.55
0.00	0.00	0.00