

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091817\
 Data File : BM011576.D
 Acq On : 18 Sep 2017 19:24
 Operator : SJ/JU
 Sample : I5234-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.393	14	18	29	rVB	101220	137114	1.37%	0.117%
2	4.146	140	146	153	rVB4	15191	28562	0.29%	0.024%
3	5.281	332	339	360	rBV	1694115	2805400	28.09%	2.399%
4	7.122	646	652	668	rBV	322875	632879	6.34%	0.541%
5	7.292	674	681	694	rBV	1272531	2072494	20.75%	1.772%
6	7.498	709	716	740	rBV	1252385	2106552	21.09%	1.801%
7	7.857	770	777	788	rBV	731945	1221776	12.23%	1.045%
8	7.969	789	796	799	rVV	1851350	3044210	30.48%	2.603%
9	8.004	799	802	816	rVB	1678442	2705774	27.09%	2.313%
10	8.322	846	856	872	rBV	1843068	3106064	31.10%	2.656%
11	8.663	907	914	926	rBV	926427	1636155	16.38%	1.399%
12	8.745	926	928	934	rVB6	9839	13450	0.13%	0.011%
13	9.133	986	994	1007	rBV	1585943	2719586	27.23%	2.325%
14	9.228	1007	1010	1016	rVV6	23579	45761	0.46%	0.039%
15	9.528	1057	1061	1065	rVV3	13743	18991	0.19%	0.016%
16	9.857	1109	1117	1132	rBV	1136940	2020506	20.23%	1.728%
17	10.392	1200	1208	1223	rBV	1631392	2951689	29.55%	2.524%
18	10.569	1233	1238	1243	rBV5	11324	29552	0.30%	0.025%
19	10.633	1243	1249	1263	rVV	1033416	1836895	18.39%	1.571%
20	10.775	1265	1273	1284	rVB	2788114	4649084	46.55%	3.975%
21	10.922	1292	1298	1305	rBV	56051	116128	1.16%	0.099%
22	11.157	1331	1338	1350	rVB	698669	1188227	11.90%	1.016%
23	11.380	1369	1376	1384	rBV2	49089	105942	1.06%	0.091%
24	11.592	1404	1412	1418	rBV9	12780	34130	0.34%	0.029%
25	11.969	1471	1476	1481	rBV4	6542	12632	0.13%	0.011%
26	12.016	1481	1484	1488	rVB4	12516	17086	0.17%	0.015%
27	12.363	1537	1543	1548	rBV2	22662	37904	0.38%	0.032%
28	12.768	1604	1612	1614	rBV4	27583	51265	0.51%	0.044%
29	12.792	1614	1616	1624	rVB2	40132	65330	0.65%	0.056%
30	12.957	1639	1644	1648	rBV4	16649	24670	0.25%	0.021%
31	13.204	1680	1686	1693	rBV3	23876	41297	0.41%	0.035%
32	13.280	1693	1699	1702	rBV4	9180	16972	0.17%	0.015%
33	13.404	1715	1720	1730	rVB	143907	233673	2.34%	0.200%
34	14.004	1815	1822	1826	rBV	3598007	5096453	51.03%	4.357%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091817\
 Data File : BM011576.D
 Acq On : 18 Sep 2017 19:24
 Operator : SJ/JU
 Sample : I5234-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

35	14.045	1826	1829	1837	rVV	321318	483239	4.84%	0.413%
36	14.121	1837	1842	1846	rVB5	8266	15915	0.16%	0.014%
37	14.233	1859	1861	1865	rBV5	6152	10525	0.11%	0.009%
38	14.292	1865	1871	1886	rVV	3898247	5734287	57.41%	4.903%
39	14.480	1898	1903	1908	rVB3	19042	27895	0.28%	0.024%
40	14.598	1917	1923	1938	rVB2	3941904	6200082	62.08%	5.301%
41	14.786	1949	1955	1965	rBV2	147806	342030	3.42%	0.292%
42	14.915	1973	1977	1983	rVB3	47876	70990	0.71%	0.061%
43	15.086	2001	2006	2015	rBV8	10342	21229	0.21%	0.018%
44	15.380	2051	2056	2059	rBV2	18742	28600	0.29%	0.024%
45	15.427	2059	2064	2071	rVB2	50417	69716	0.70%	0.060%
46	15.586	2082	2091	2103	rBV	5375105	7586598	75.96%	6.487%
47	15.698	2103	2110	2126	rVV	1689415	2384115	23.87%	2.038%
48	15.827	2126	2132	2139	rVB3	71691	112608	1.13%	0.096%
49	15.986	2155	2159	2164	rBV5	9186	15887	0.16%	0.014%
50	16.045	2167	2169	2172	rVB3	9172	10644	0.11%	0.009%
51	16.286	2206	2210	2219	rBV	65552	109503	1.10%	0.094%
52	16.368	2221	2224	2228	rVB6	7758	12826	0.13%	0.011%
53	16.468	2237	2241	2247	rVB6	14349	20661	0.21%	0.018%
54	16.639	2265	2270	2276	rBV9	13329	26287	0.26%	0.022%
55	16.792	2293	2296	2300	rVV5	10794	11900	0.12%	0.010%
56	17.074	2341	2344	2349	rBV	43222	57355	0.57%	0.049%
57	17.133	2350	2354	2359	rVB2	21242	29604	0.30%	0.025%
58	17.339	2382	2389	2398	rBV2	5097572	7300332	73.09%	6.242%
59	17.439	2399	2406	2423	rVB	6245935	8708440	87.19%	7.446%
60	17.609	2432	2435	2440	rVB3	13061	15200	0.15%	0.013%
61	17.703	2445	2451	2459	rBV6	47652	86349	0.86%	0.074%
62	17.815	2466	2470	2473	rBV2	20843	22432	0.22%	0.019%
63	17.992	2495	2500	2506	rVB	43450	62974	0.63%	0.054%
64	18.209	2532	2537	2542	rBV	242463	349307	3.50%	0.299%
65	18.292	2548	2551	2558	rVB	22730	39455	0.40%	0.034%
66	18.503	2584	2587	2591	rBV3	14680	17782	0.18%	0.015%
67	19.062	2680	2682	2684	rBV3	11193	10901	0.11%	0.009%
68	19.133	2690	2694	2695	rBV4	20443	23038	0.23%	0.020%
69	19.156	2695	2698	2702	rVB2	62967	70416	0.71%	0.060%
70	19.286	2718	2720	2723	rVB4	13571	13389	0.13%	0.011%
71	19.356	2726	2732	2741	rVV2	73803	140481	1.41%	0.120%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091817\
Data File : BM011576.D
Acq On : 18 Sep 2017 19:24
Operator : SJ/JU
Sample : I5234-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Title : SVOA CALIBRATION

72	19.480	2748	2753	2760	rBV	234907	339705	3.40%	0.290%
73	19.615	2772	2776	2782	rVB2	51951	101018	1.01%	0.086%
74	19.721	2788	2794	2804	rBV	7410917	9987849	100.00%	8.540%
75	21.191	3040	3044	3051	rBV	152469	244500	2.45%	0.209%
76	21.503	3091	3097	3110	rBV	6564875	8268138	82.78%	7.069%
77	23.721	3467	3474	3486	rVB2	4678791	9148400	91.60%	7.822%
78	23.874	3493	3500	3510	rVB	3771781	7205990	72.15%	6.161%
79	24.409	3587	3591	3599	rVB	303005	595412	5.96%	0.509%


Sum of corrected areas: 116958207

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091817\
Data File : BM011576.D
Acq On : 18 Sep 2017 19:24
Operator : SJ/JU
Sample : I5234-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
C0AH8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

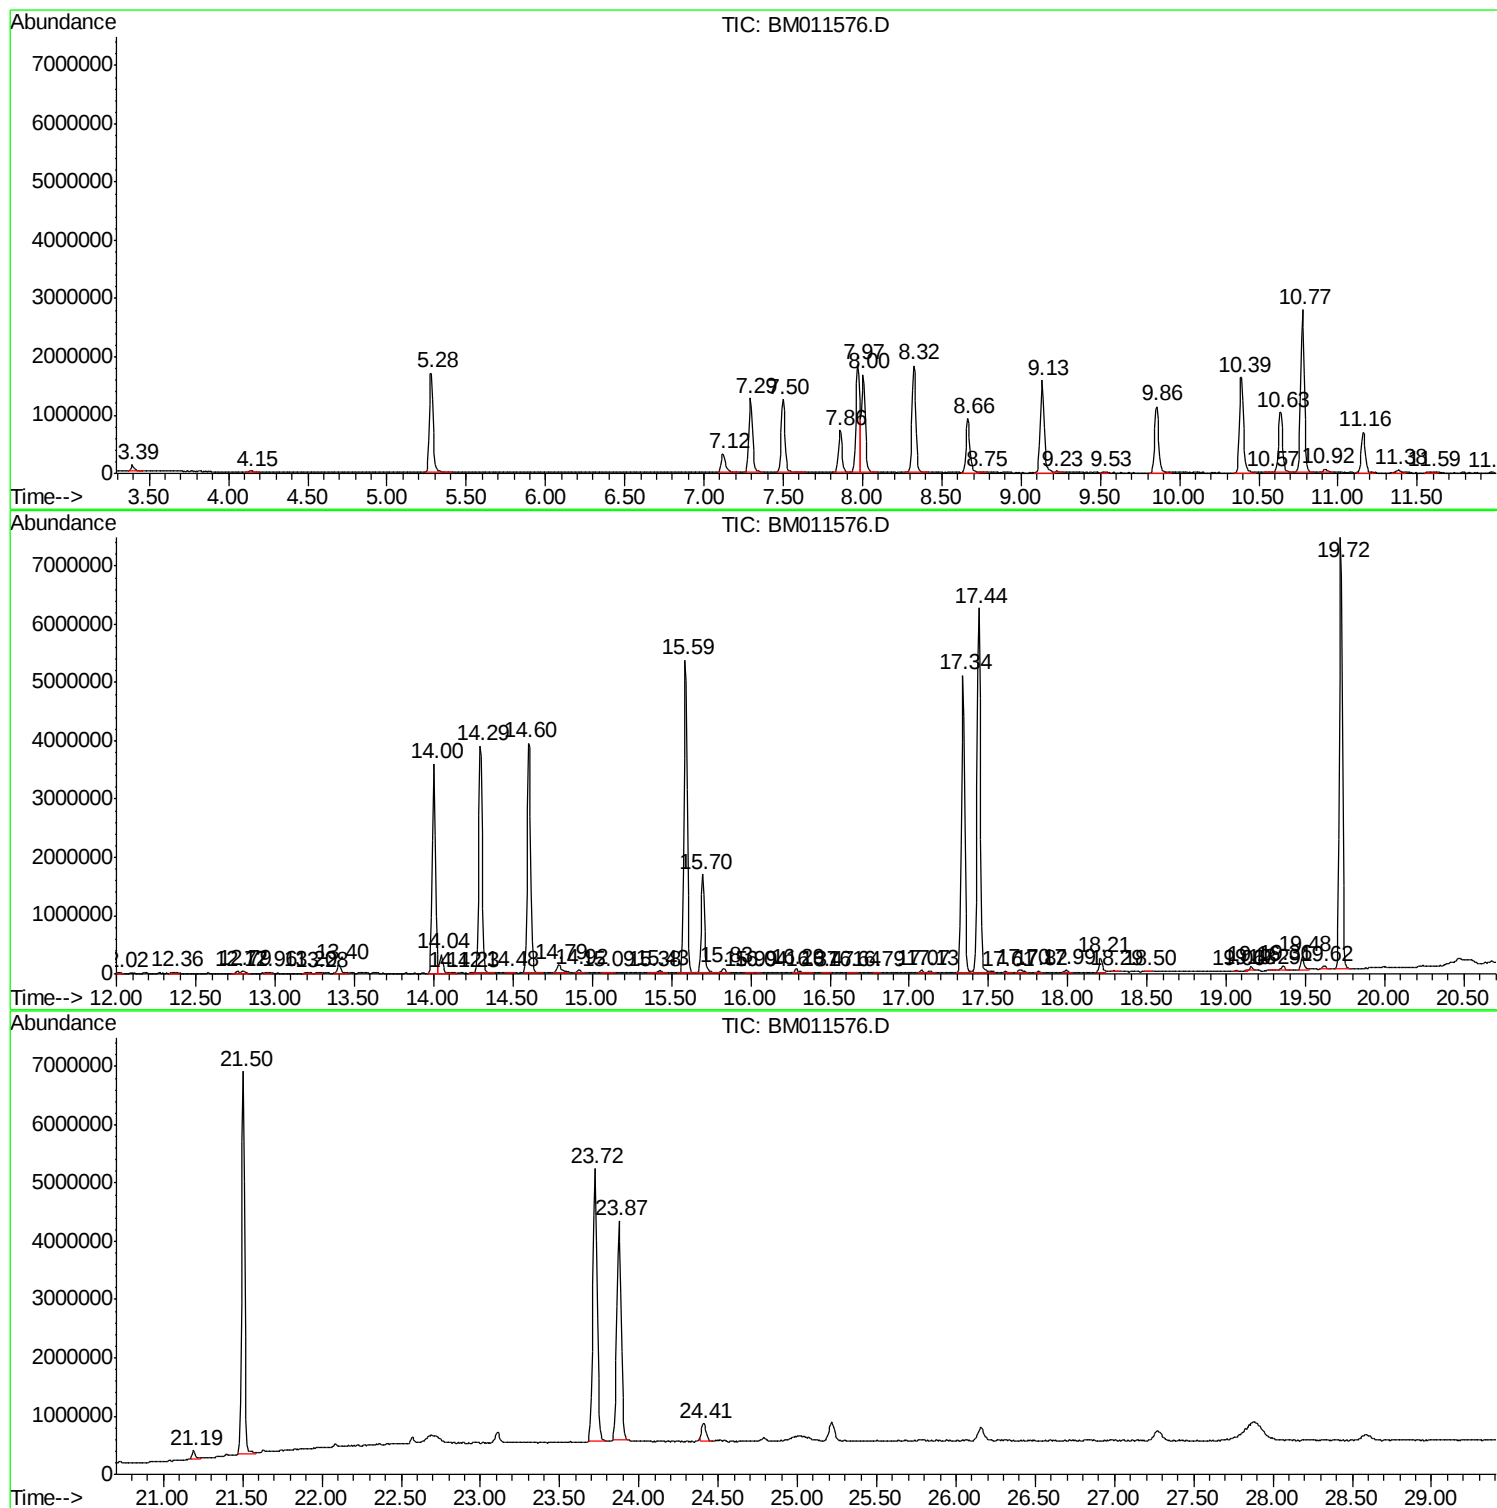

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091817\
Data File : BM011576.D
Acq On : 18 Sep 2017 19:24
Operator : SJ/JU
Sample : I5234-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091817\
Data File : BM011576.D
Acq On : 18 Sep 2017 19:24
Operator : SJ/JU
Sample : I5234-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc