


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091824\
Data File : BM047552.D
Acq On : 18 Sep 2024 08:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Sep 15 08:56:37 2024

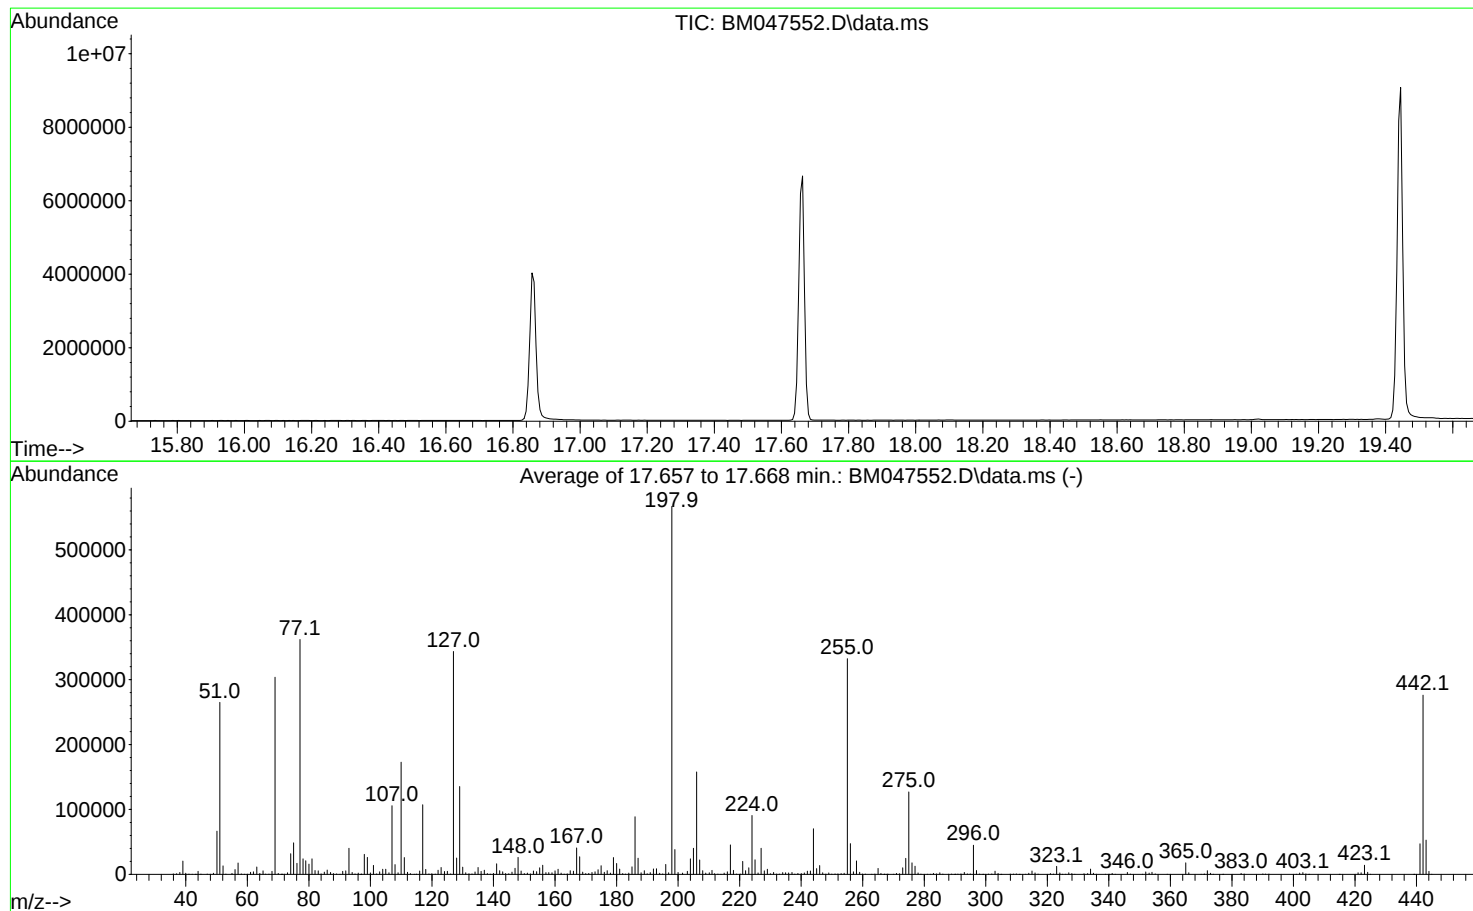




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	265037	PASS
68	69	0.00	2	1.6	4815	PASS
69	198	0.00	100	53.6	303872	PASS
70	69	0.00	2	0.5	1546	PASS
127	198	10	80	60.6	343552	PASS
197	198	0.00	2	0.5	2606	PASS
198	198	100	100	100.0	566891	PASS
199	198	5	9	6.7	38261	PASS
275	198	10	60	22.4	127091	PASS
365	198	1	100	3.1	17685	PASS
441	198	0.01	100	8.3	47040	PASS
442	442	50	100	100.0	276203	PASS
443	442	15	24	19.1	52717	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091824\
Data File : BM047552.D
Acq On : 18 Sep 2024 08:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 18 11:19:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

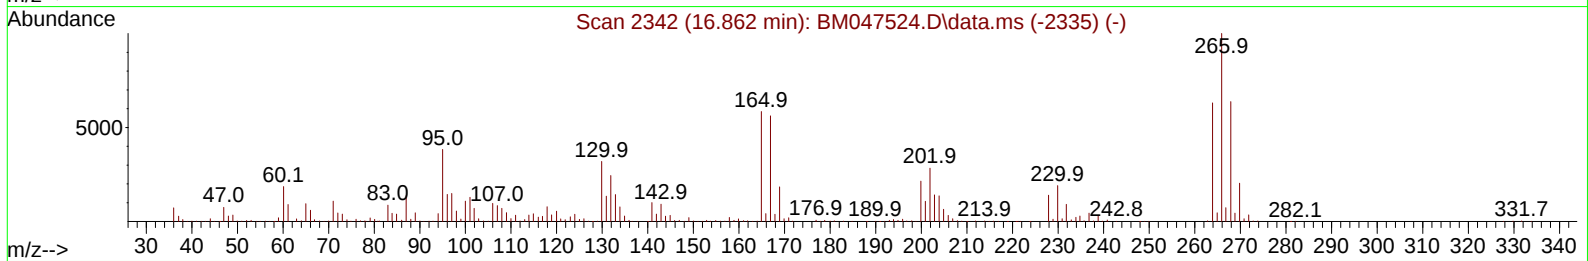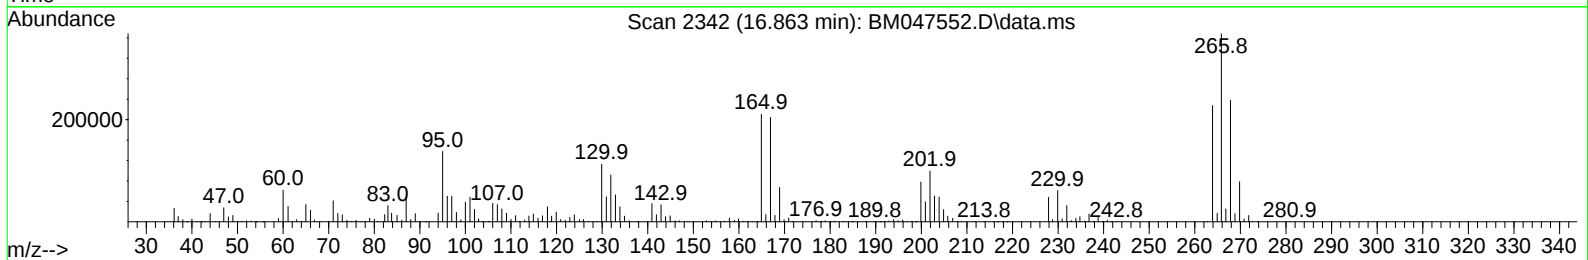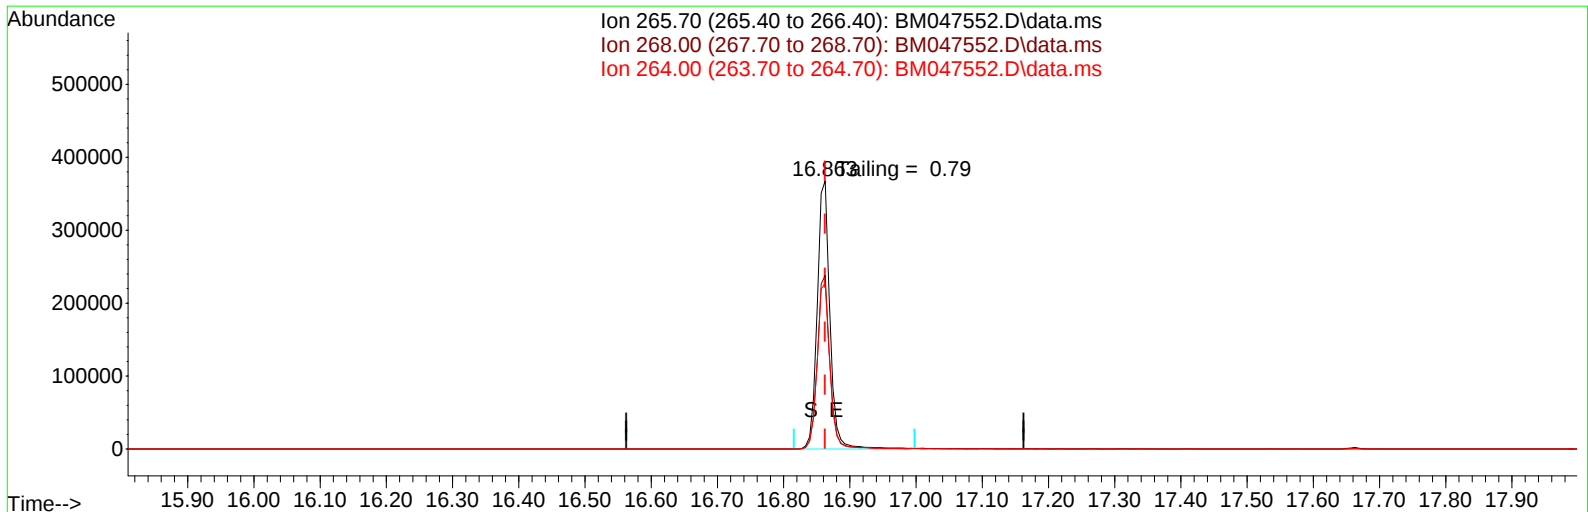

TIC: BM047552.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.000) 0.00 ng




response 492498

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.73
264.00	63.00	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091824\
Data File : BM047552.D
Acq On : 18 Sep 2024 08:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 18 11:19:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

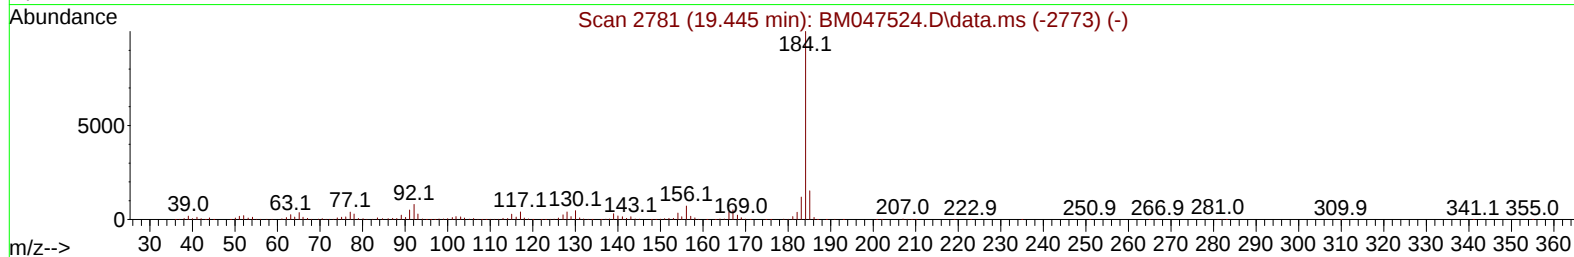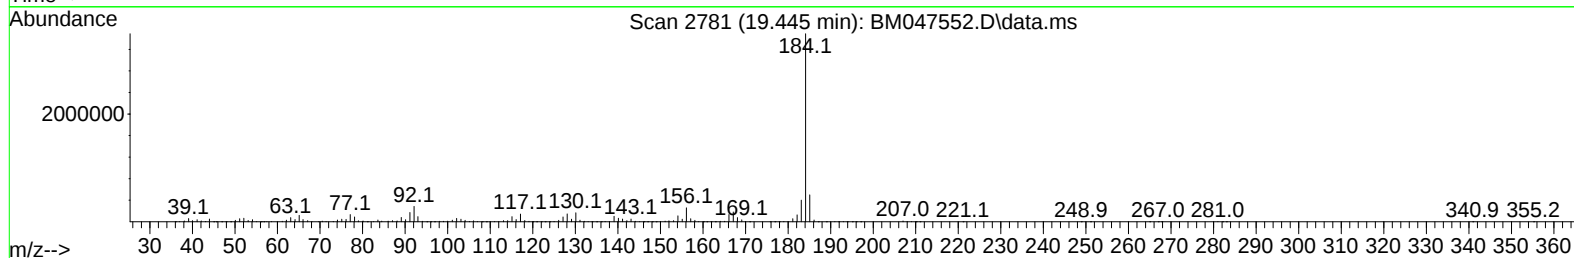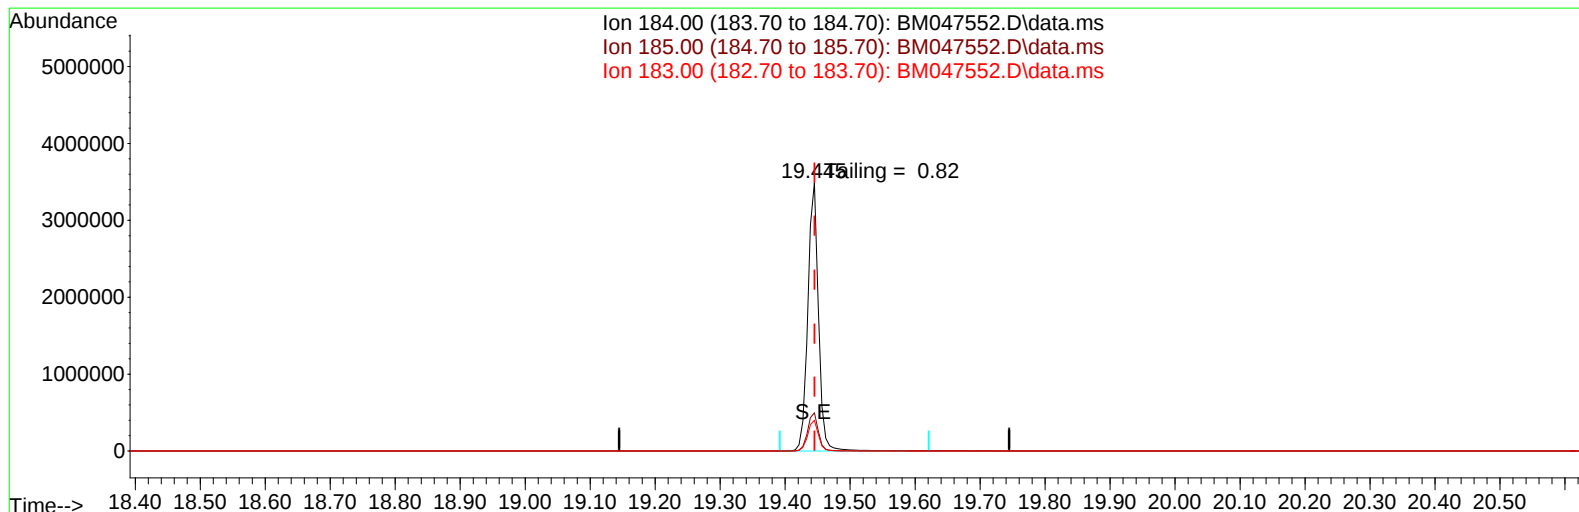

TIC: BM047552.D\data.ms

(77) Benzidine

19.445min (-0.000) 2611153.57 ng

response 3971681

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.28
183.00	12.00	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2024	BNA_M	<u>BM047552.D</u>
Compound Name	Response	Retention Time
DDT	1768642	20.68
DDD	15809	20.292
DDE	687	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16496	1785138	0.92

Instrument :
BNA_M
ClientSampleId :
DFTPP