

Data Path : Z:\HPCHEM1\BNA M\DATA\BM091916\
 Data File : BM007480.D
 Acq On : 19 Sep 2016 18:39
 Operator : UM/SJ
 Sample : PB93451BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.963	737	744	756	rBV	755220	1280871	15.14%	1.941%
2	7.122	765	771	781	rBV	607685	981943	11.61%	1.488%
3	7.322	799	805	819	rBV	805068	1337560	15.82%	2.027%
4	7.786	877	884	894	rBV	560481	929666	10.99%	1.409%
5	8.492	997	1004	1024	rBV	1049773	1743961	20.62%	2.642%
6	8.945	1074	1081	1095	rBV	839233	1404595	16.61%	2.128%
7	9.663	1196	1203	1214	rBV	737247	1224612	14.48%	1.855%
8	10.198	1287	1294	1312	rBV	971243	1800740	21.29%	2.728%
9	10.574	1350	1358	1366	rBV	855566	1475550	17.45%	2.236%
10	10.716	1374	1382	1400	rBV	752476	1472942	17.42%	2.232%
11	13.827	1905	1911	1927	rBV	2338281	3391693	40.10%	5.139%
12	14.110	1952	1959	1972	rBV	2456750	3746159	44.29%	5.676%
13	14.421	2005	2012	2021	rBV	1575693	2345518	27.73%	3.554%
14	14.627	2040	2047	2065	rBV	807816	1668389	19.73%	2.528%
15	15.415	2174	2181	2192	rBV	3404528	4894109	57.87%	7.415%
16	15.539	2196	2202	2217	rVV	1055279	1605614	18.98%	2.433%
17	17.162	2472	2478	2488	rBV2	2160496	3106964	36.74%	4.708%
18	17.262	2489	2495	2508	rVV2	3912759	5729241	67.74%	8.681%
19	19.556	2878	2885	2897	rBV	5265035	7377288	87.23%	11.178%
20	21.344	3183	3189	3204	rBV	3533424	4756166	56.24%	7.206%
21	23.468	3542	3550	3564	rBV2	4474790	8457502	100.00%	12.815%
22	23.609	3567	3574	3584	rVB2	2389760	4763318	56.32%	7.217%
23	24.121	3657	3661	3670	rVB	124882	235471	2.78%	0.357%
24	24.874	3785	3789	3797	rVB	126132	269344	3.18%	0.408%


Sum of corrected areas: 65999216

Data Path : Z:\HPCHEM1\BNA M\DATA\BM091916\
Data File : BM007480.D
Acq On : 19 Sep 2016 18:39
Operator : UM/SJ
Sample : PB93451BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

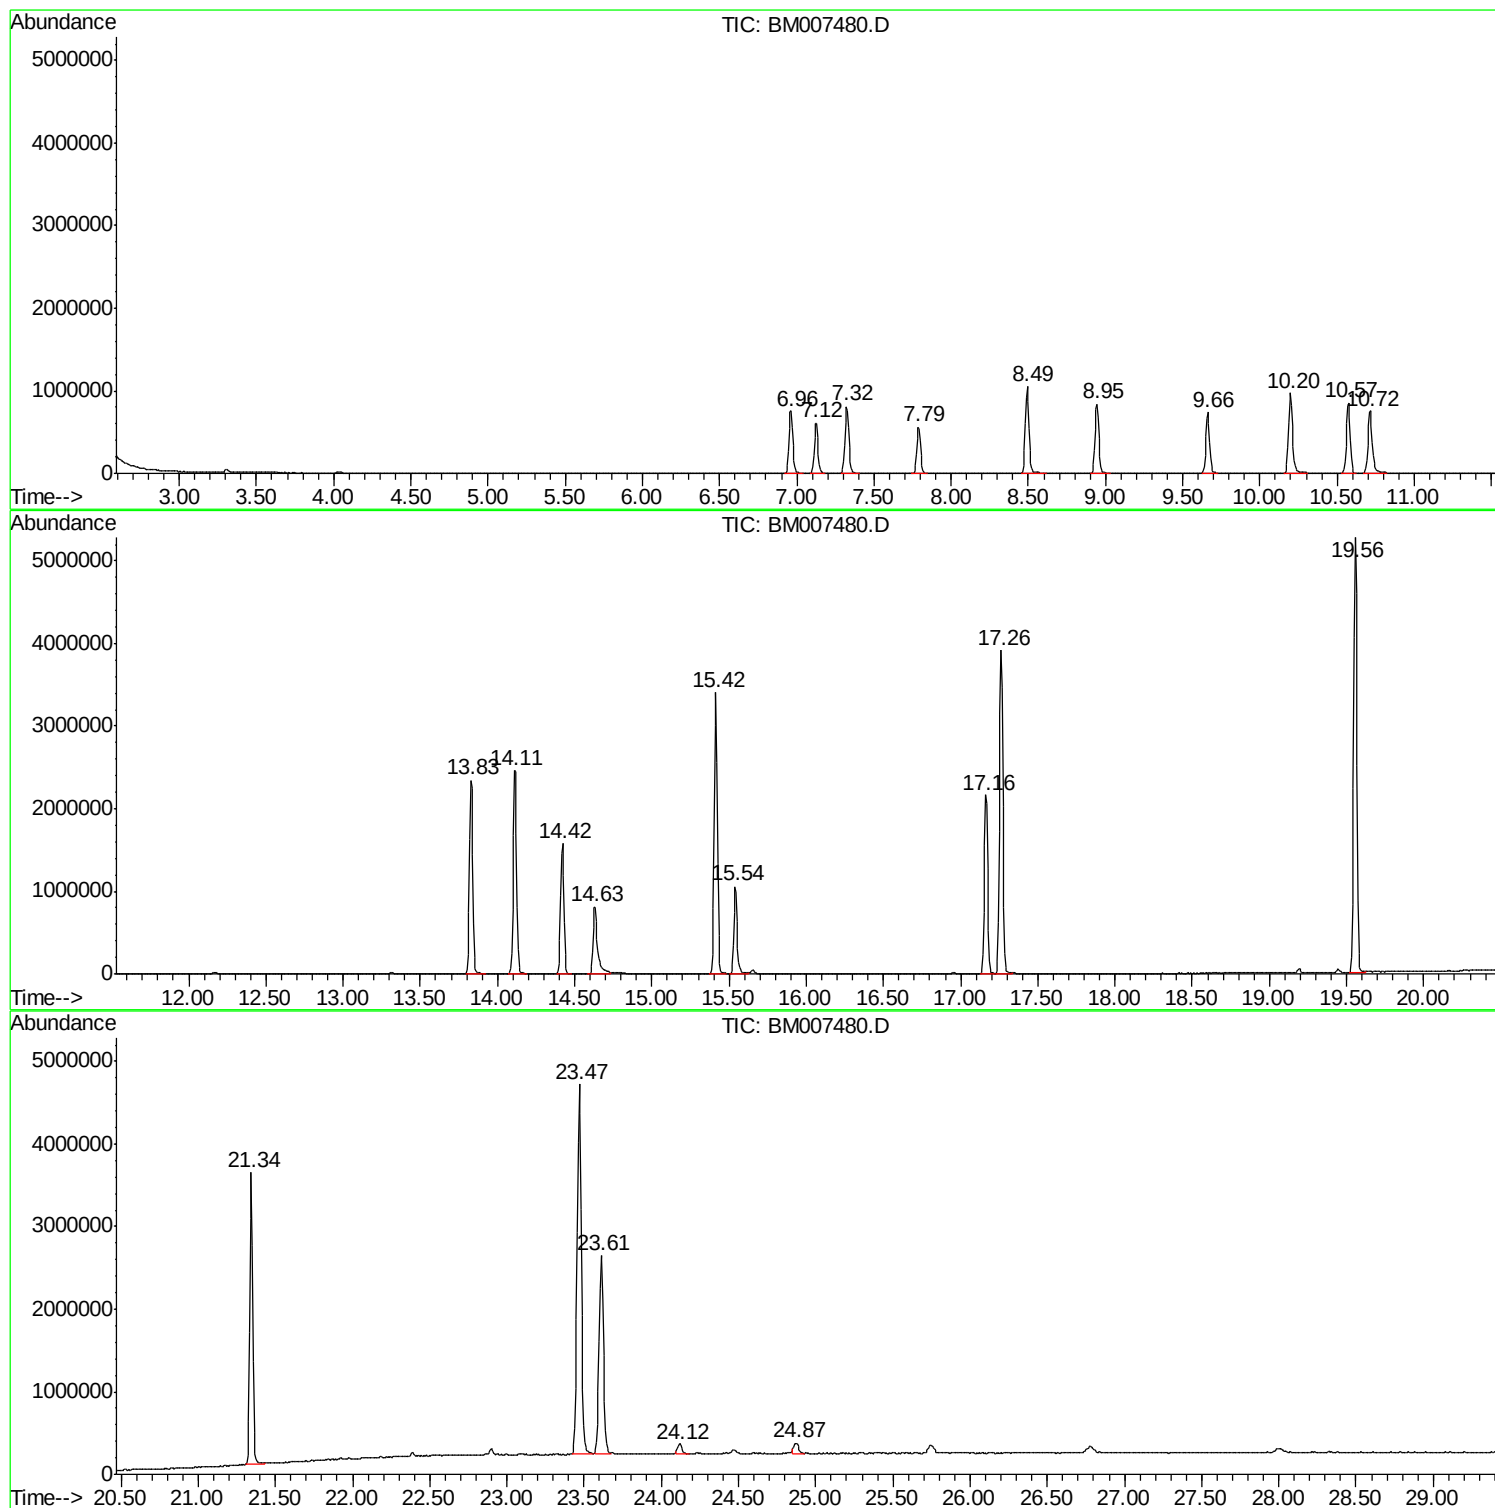

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091916\
Data File : BM007480.D
Acq On : 19 Sep 2016 18:39
Operator : UM/SJ
Sample : PB93451BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM091916\
Data File : BM007480.D
Acq On : 19 Sep 2016 18:39
Operator : UM/SJ
Sample : PB93451BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK51

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM082316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc