

Data Path : Z:\HPCHEM1\BNA M\DATA\BM091917\
 Data File : BM011610.D
 Acq On : 19 Sep 2017 18:37
 Operator : SJ/JU
 Sample : I5271-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF1

Quant Time: Sep 20 01:54:38 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 20 01:49:56 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	393956	20.00	ng/ul	0.00
18) Naphthalene-d8	10.77	136	1704255	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	1005232	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.34	188	2244551	20.00	ng/ul	0.00
78) Chrysene-d12	21.50	240	2303691	20.00	ng/ul	0.00
86) Perylene-d12	23.87	264	1999750	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.39	96	41727	4.76	ng/uL	0.00
5) Phenol-d5	7.12	99	195789	5.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.29	67	735175	28.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.50	132	626101	21.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.66	113	246472	8.35	ng/ul	0.00
19) Nitrobenzene-d5	9.13	128	396070	30.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.85	143	421390	31.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.39	165	718140	26.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	2257	0.08	ng/ul	0.01
44) Dimethylphthalate-d6	14.00	166	2573124	30.28	ng/ul	0.00
47) Acenaphthylene-d8	14.29	160	2621773	25.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.78	143	68398	4.28	ng/ul	0.00
58) Fluorene-d10	15.59	176	2258630	30.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.70	200	348110	26.65	ng/ul	0.00
71) Anthracene-d10	17.43	188	3517800	31.83	ng/ul	0.00
79) Pyrene-d10	19.72	212	3966231	36.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.72	264	3122636	32.77	ng/ul	0.00

Target Compounds


					Ovalue	
10) 2-Chlorophenol	7.53	128	60453	2.174	ng/ul#	88
11) 2-Methylphenol	8.34	108	219909	7.724	ng/ul	99
32) Caprolactam	11.59	113	8603	1.047	ng/ul#	21
37) 1,2,4,5-Tetrachlorobenzene	12.79	216	194001	6.506	ng/ul#	96
73) 1,2,3,4-Tetrachlorobenzene	13.40	216	926126	30.964	ng/uL	97
74) Pentachlorobenzene	14.91	250	40352	1.330	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM091917\
Data File : BM011610.D
Acq On : 19 Sep 2017 18:37
Operator : SJ/JU
Sample : I5271-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF1

Quant Time: Sep 20 01:54:38 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 20 01:49:56 2017
Response via : Initial Calibration

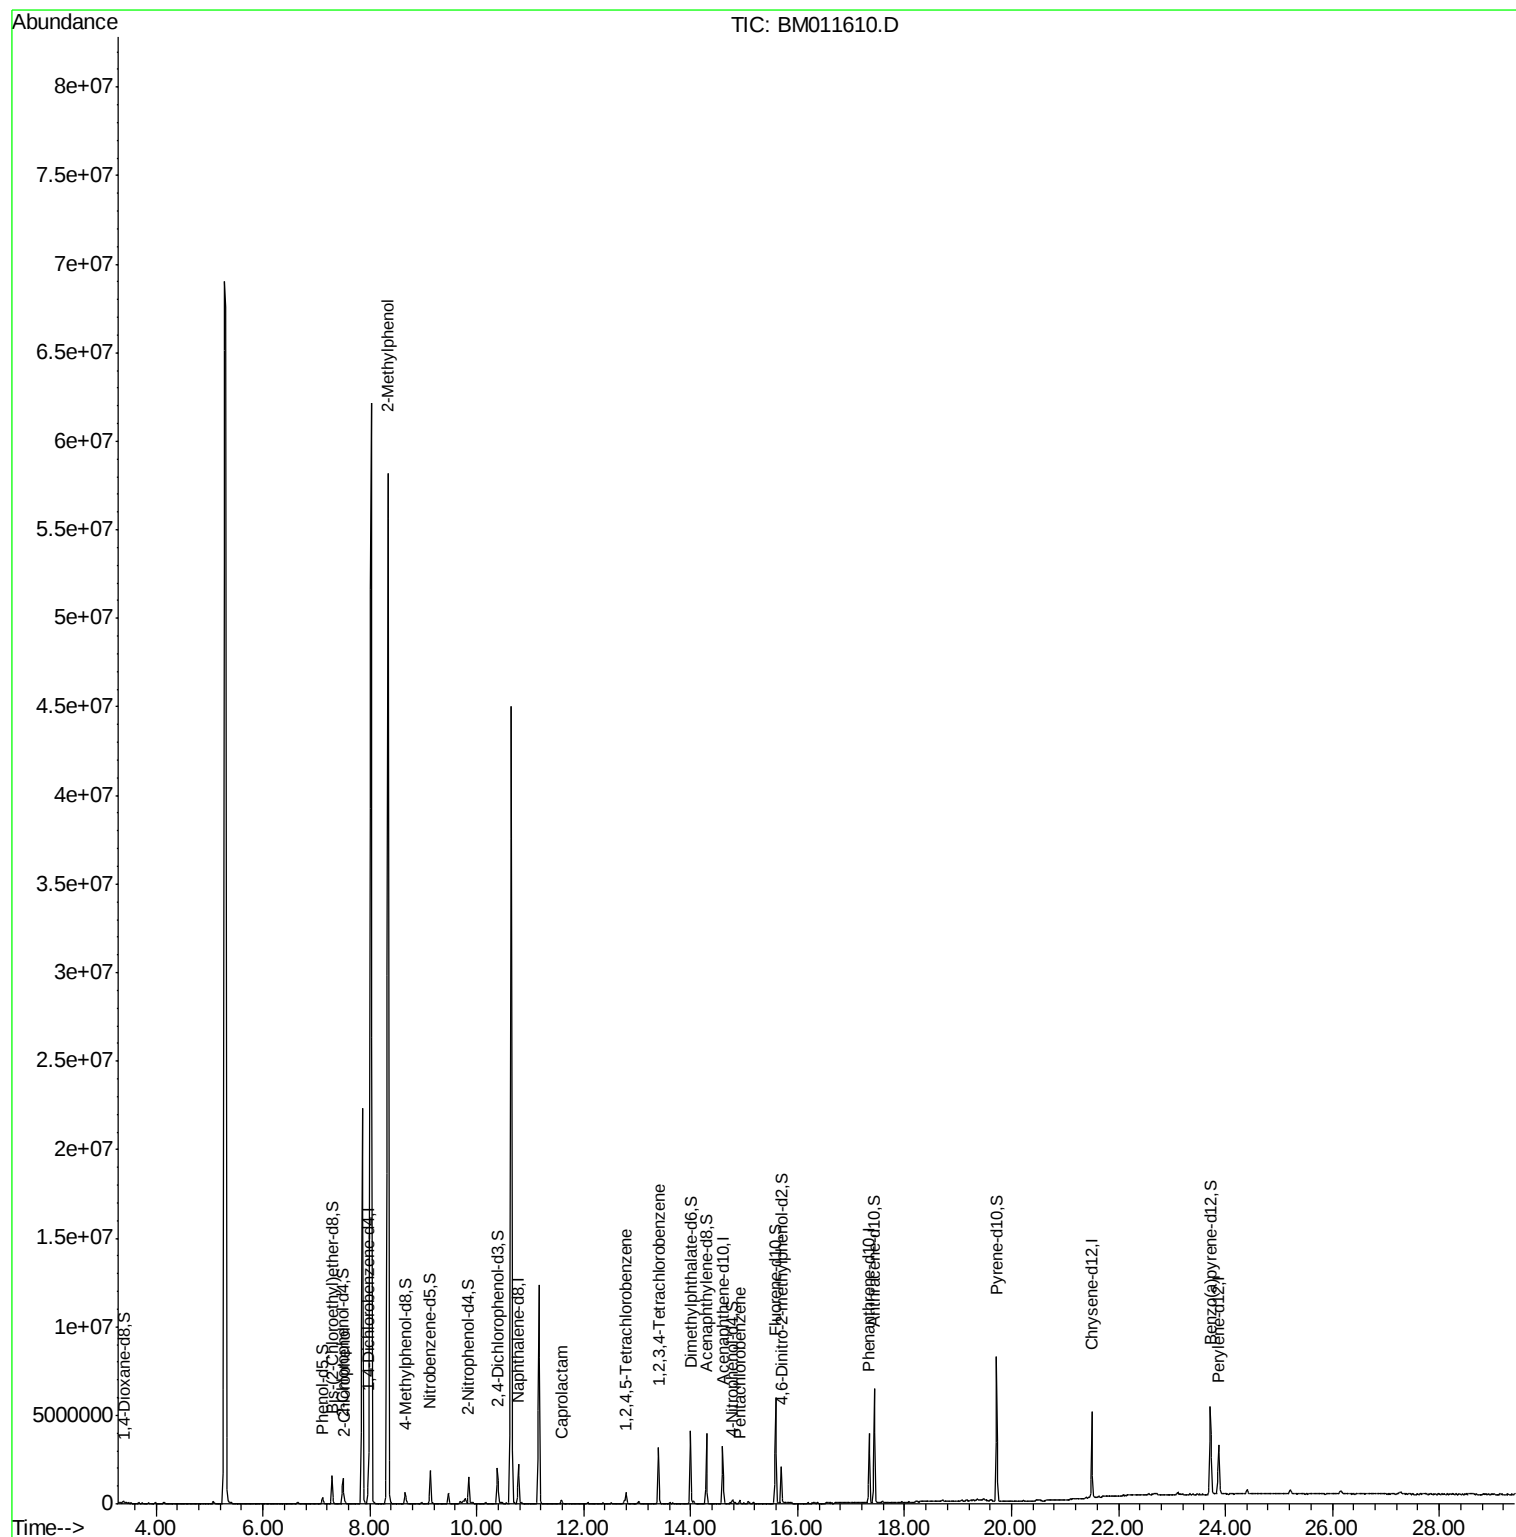

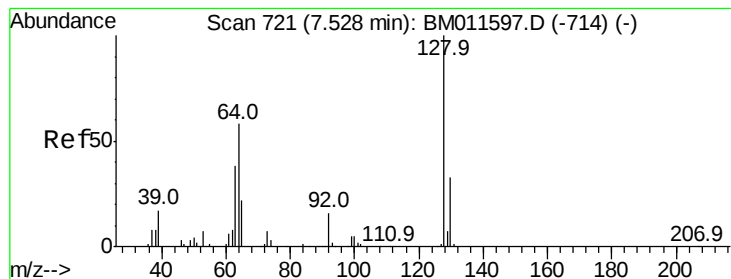

#10

2-Chlorophenol

Concen: 2.174 ng/ul

RT: 7.53 min Scan# 721

Delta R.T. 0.00 min

Lab File: BM011610.D

Acq: 19 Sep 2017 18:37

Instrument :

BNA_M

ClientSampleId :

C0AF1


Tot Ion:128 Resp: 60453

Ion Ratio Lower Upper

128 100

64 60.0 39.8 59.6#




130 27.4 25.8 38.8

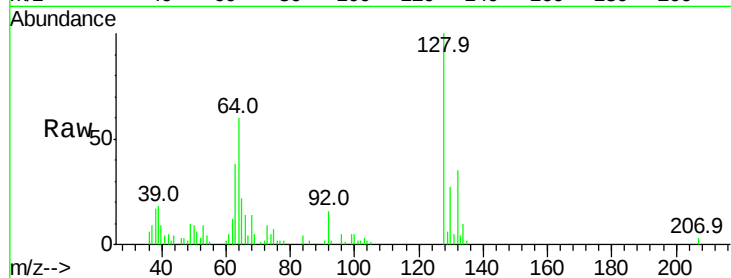

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BM011610.D (-835) (-)

Ion 130.00 (129.70 to 130.70): E

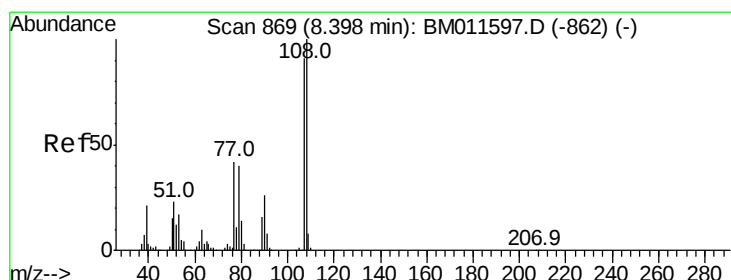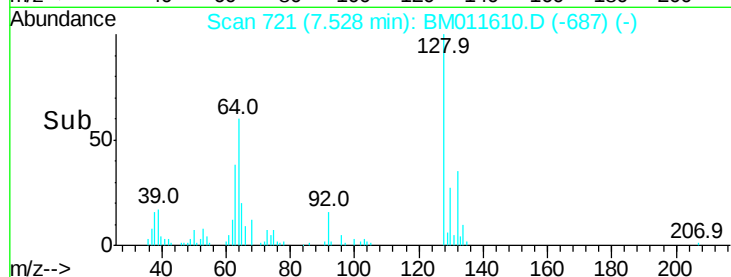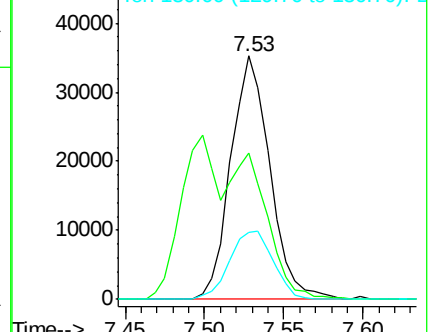

#11

2-Methylphenol

Concen: 7.724 ng/ul

RT: 8.34 min Scan# 859

Delta R.T. -0.06 min

Lab File: BM011610.D


Acq: 19 Sep 2017 18:37

Tgt Ion:108 Resp: 219909

Ion Ratio Lower Upper



108 100


107 91.8 74.1 111.1

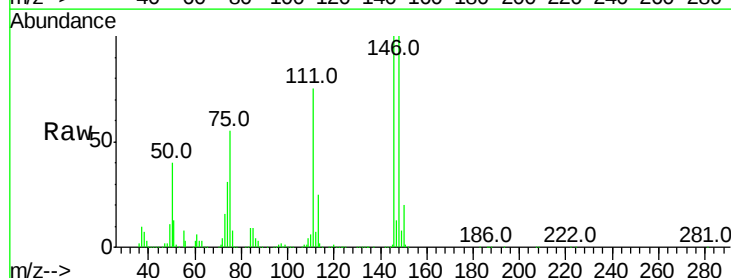

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

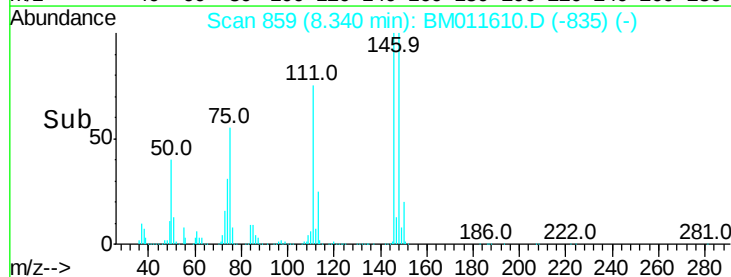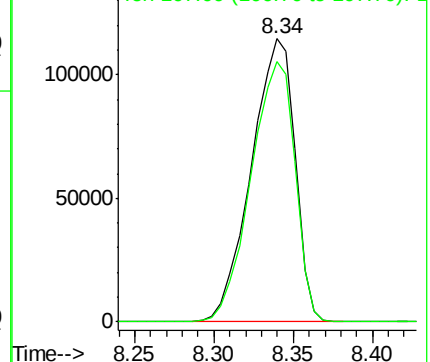

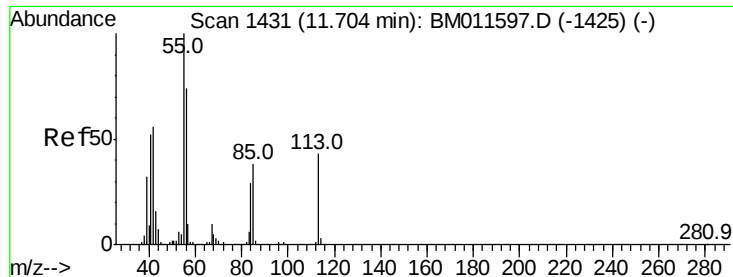

#32

Caprolactam

Concen: 1.047 ng/ul

RT: 11.59 min Scan# 1411

Delta R.T. -0.12 min

Lab File: BM011610.D

Acq: 19 Sep 2017 18:37

Instrument :

BNA_M

ClientSampleId :

C0AF1


Tot Ion:113 Resp: 8603

Ion Ratio Lower Upper

113 100

55 51.4 131.7 197.5#




56 192.5 92.7 139.1#

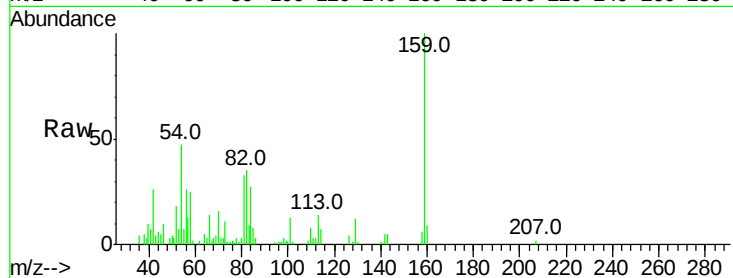

Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM0

Ion 56.00 (55.70 to 56.70): BM0

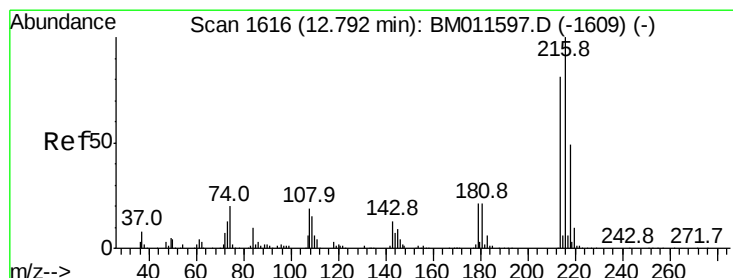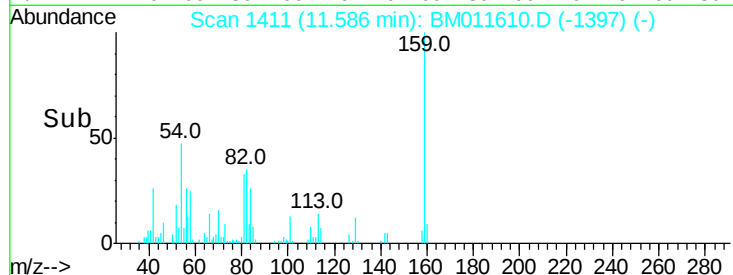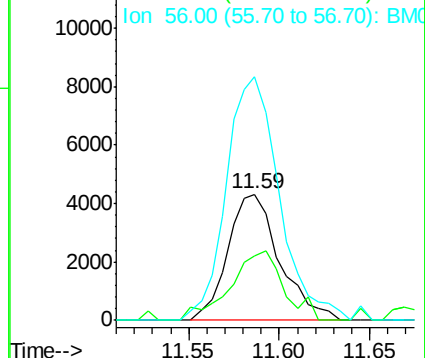

#37

1,2,4,5-Tetrachlorobenzene

Concen: 6.506 ng/ul

RT: 12.79 min Scan# 1616

Delta R.T. 0.00 min

Lab File: BM011610.D

Acq: 19 Sep 2017 18:37

Tgt Ion:216 Resp: 194001


Ion Ratio Lower Upper

216 100

214 78.6 64.1 96.1

179 20.8 14.5 21.7

108 19.1 10.4 15.6#


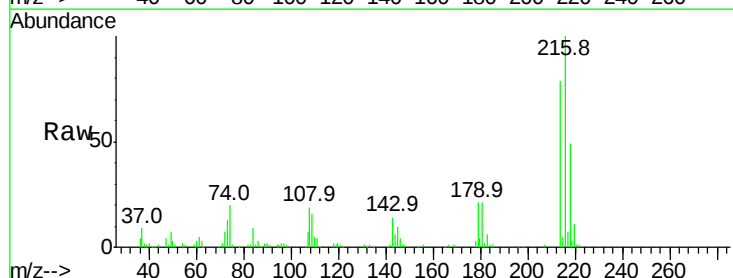



Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

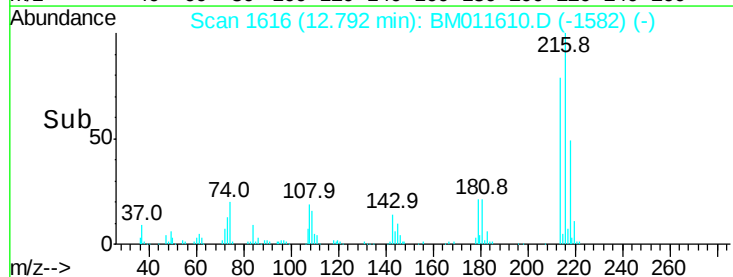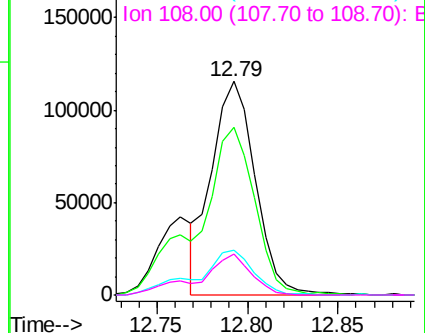

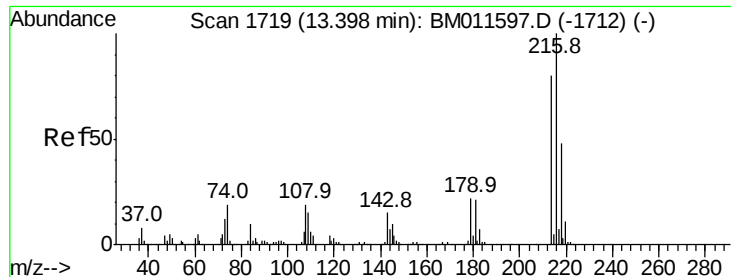

#73

1,2,3,4-Tetrachlorobenzene

Concen: 30.964 ng/uL

RT: 13.40 min Scan# 1719

Delta R.T. 0.00 min

Lab File: BM011610.D

Acq: 19 Sep 2017 18:37

Instrument :

BNA_M

ClientSampleId :

C0AF1


Tot Ion:216 Resp: 926126

Ion Ratio Lower Upper

216 100

214 77.4 64.1 96.1




218 47.1 39.4 59.0

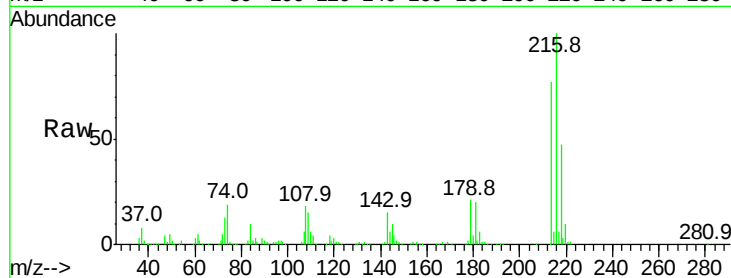

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

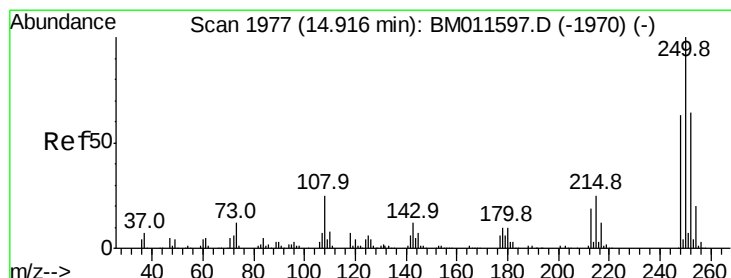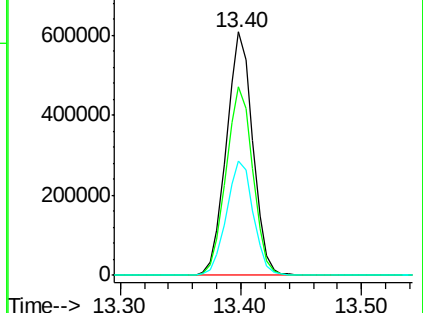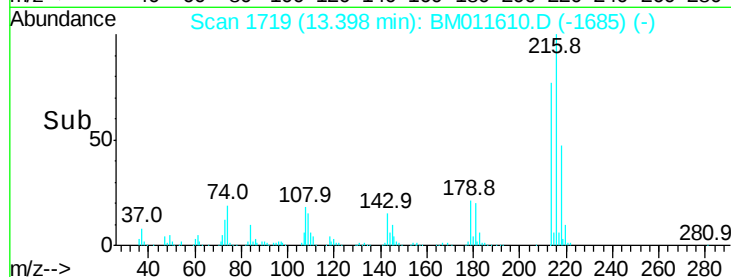

#74

Pentachlorobenzene

Concen: 1.330 ng/uL

RT: 14.91 min Scan# 1976

Delta R.T. -0.01 min

Lab File: BM011610.D

Acq: 19 Sep 2017 18:37


Tgt Ion:250 Resp: 40352

Ion Ratio Lower Upper

250 100

248 51.6 51.4 77.2

252 59.0 49.8 74.6

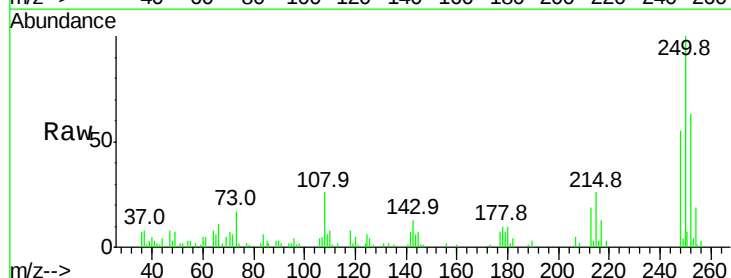

Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

