

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091920\
 Data File : BM027479.D
 Acq On : 19 Sep 2020 02:15
 Operator : JU/CG
 Sample : PB131687BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK87

Quant Time: Sep 19 07:41:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 19 07:00:16 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	132681	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	482114	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	323021	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	695162	20.00	ng/ul	0.00
78) Chrysene-d12	21.10	240	724796	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	775437	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.05	96	23638	7.93	ng/uL	0.00
5) Phenol-d5	6.69	99	324846	29.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	227242	31.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	261530	32.66	ng/ul	0.00
13) 4-Methylphenol-d8	8.21	113	249771	28.00	ng/ul	0.00
19) Nitrobenzene-d5	8.64	128	124335	34.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	140108	35.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	260085	30.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.40	131	318732	31.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	881053	34.28	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	1023036	35.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	96999	21.43	ng/ul	0.00
58) Fluorene-d10	15.14	176	736023	31.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	110849	24.92	ng/ul	0.00
71) Anthracene-d10	16.99	188	1173817	35.71	ng/ul	0.00
79) Pyrene-d10	19.30	212	1328867	41.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	1424337	34.24	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.21	70	8587	1.002 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091920\
Data File : BM027479.D
Acq On : 19 Sep 2020 02:15
Operator : JU/CG
Sample : PB131687BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK87

Quant Time: Sep 19 07:41:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 19 07:00:16 2020
Response via : Initial Calibration

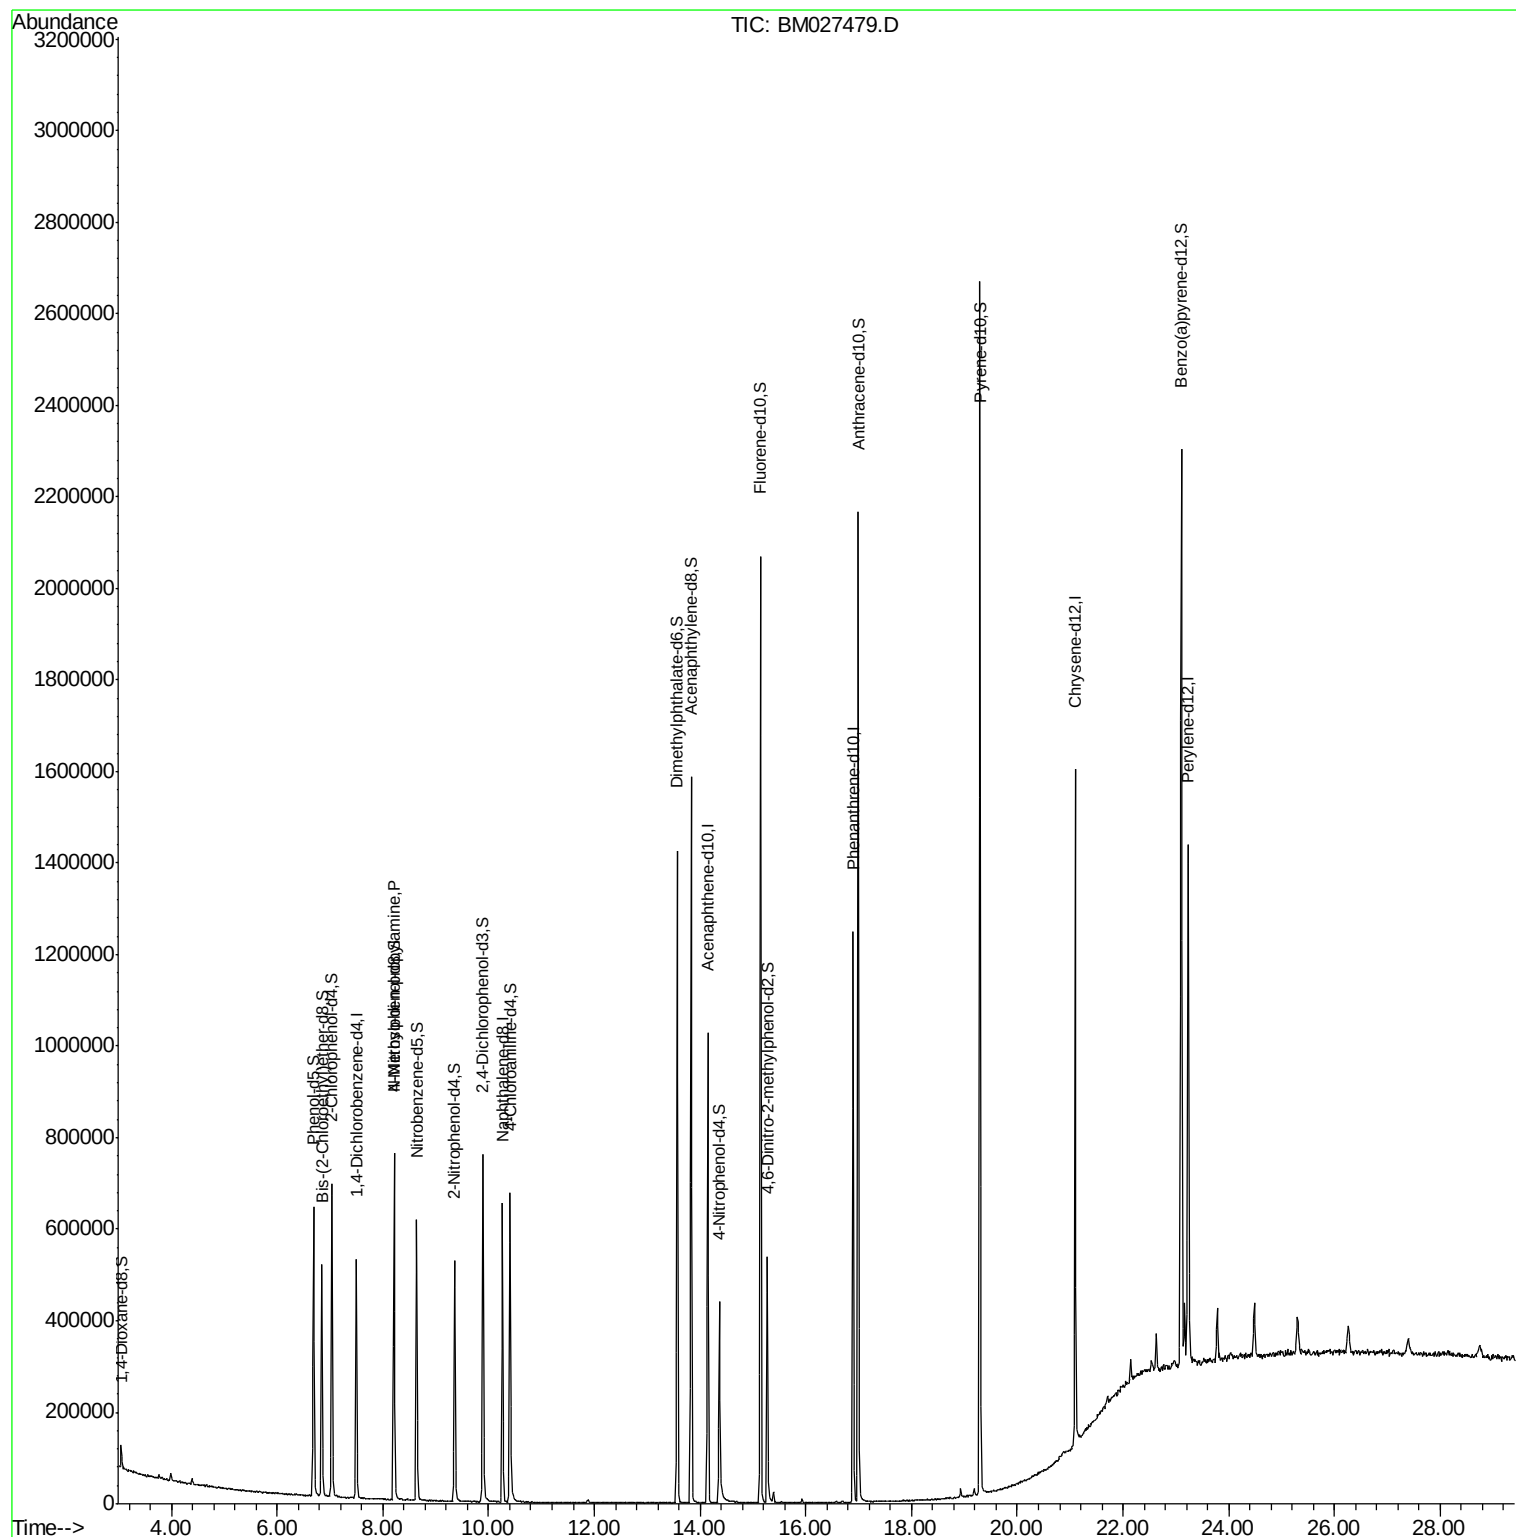

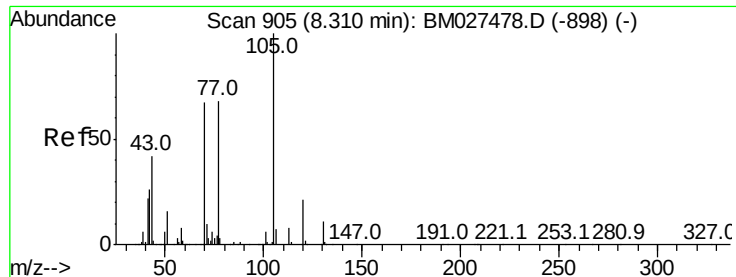

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.002 ng/ul
 RT: 8.21 min Scan# 888
 Delta R.T. -0.10 min
 Lab File: BM027479.D
 Acq: 19 Sep 2020 02:15

Instrument :
 BNA_M
 ClientSampleId :
 SBLK87

Tot Ion: 70 Resp: 8587
 Ion Ratio Lower Upper
 70 100
 42 239.0 31.0 46.4#
 101 0.0 7.0 10.6#
 130 0.0 13.6 20.4#

