

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021798.D
 Acq On : 19 Sep 2022 11:11
 Operator : CG/JU
 Sample : PB147715BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 20 00:23:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4527	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	15220	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.708	164	8877	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	18961	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	11191	0.400	ng/ul #	0.00
23) Perylene-d12	24.155	264	9433	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	32393	5.816	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.473	152	8192	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	14972	0.360	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.855	202	1834	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.995	252	2858	0.082	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021798.D
Acq On : 19 Sep 2022 11:11
Operator : CG/JU
Sample : PB147715BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 20 00:23:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




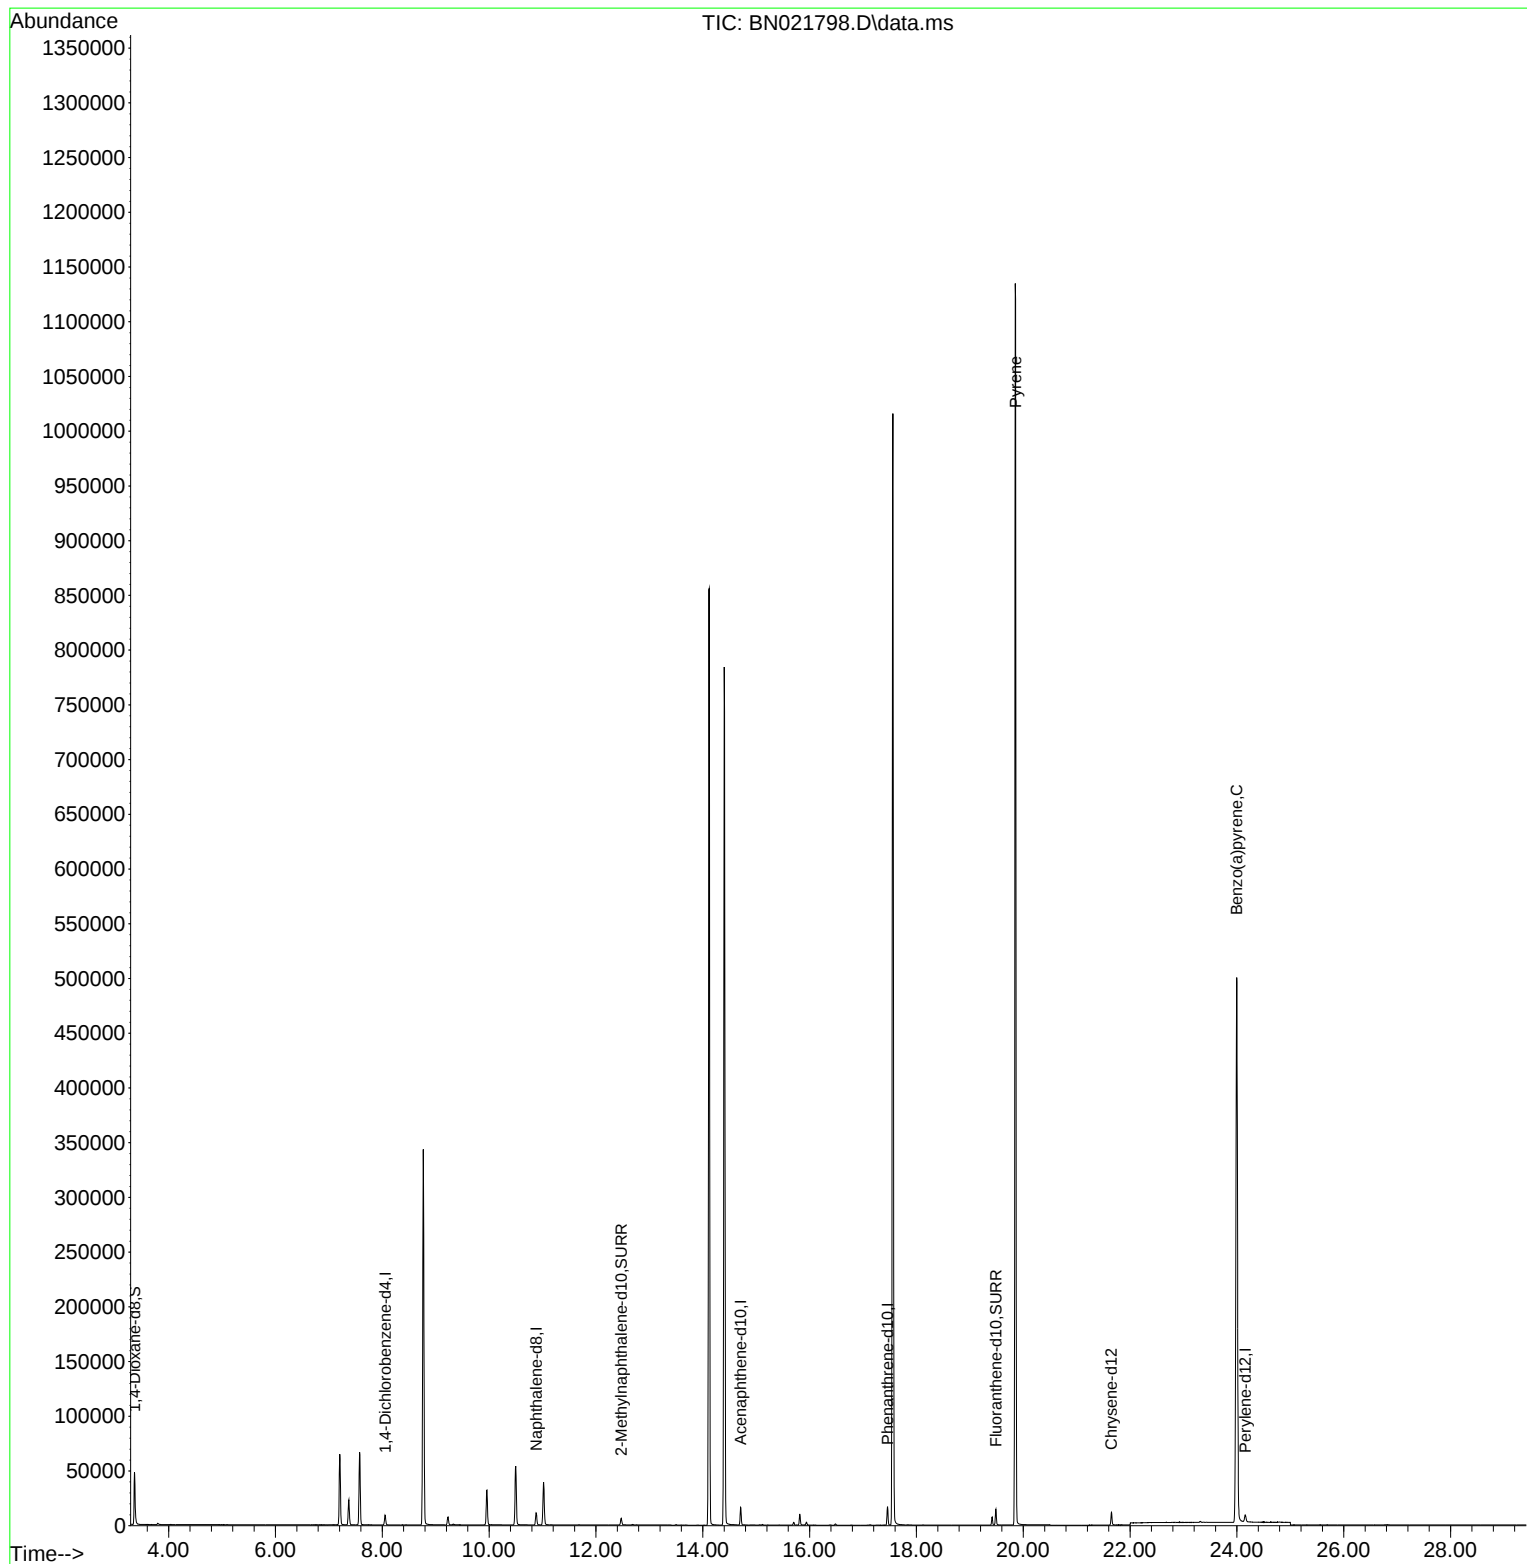


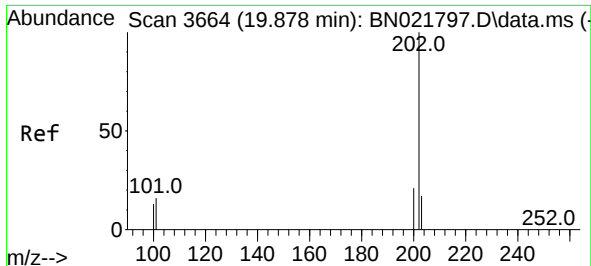

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.855 min Scan# 3659
Delta R.T. -0.023 min
Lab File: BN021798.D
Acq: 19 Sep 2022 11:11

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 1834
Ion Ratio Lower Upper
202 100
101 166.1 11.3 16.9#
100 1182.8 9.0 13.4#

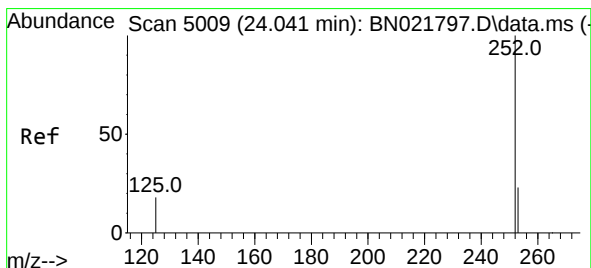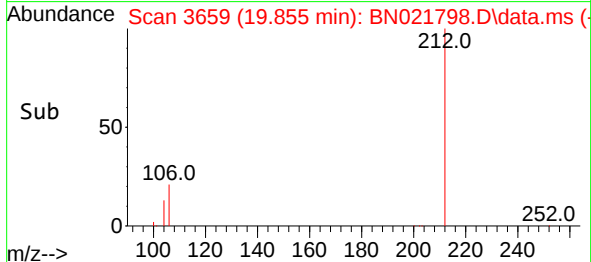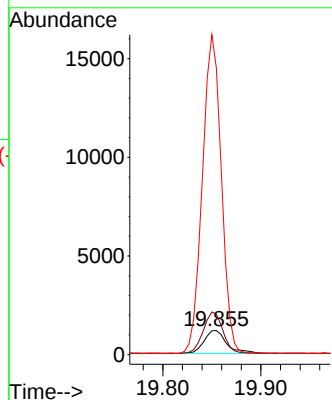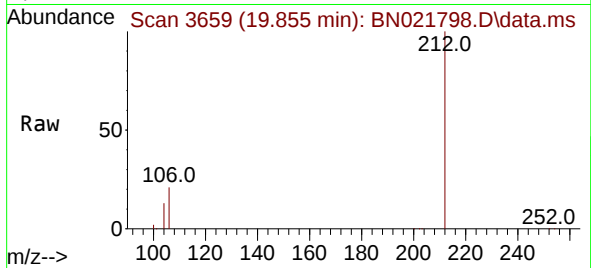

#26
Benzo(a)pyrene
Concen: 0.082 ng/ul
RT: 23.995 min Scan# 4993
Delta R.T. -0.047 min
Lab File: BN021798.D
Acq: 19 Sep 2022 11:11

Tgt Ion:252 Resp: 2858
Ion Ratio Lower Upper
252 100
253 50.9 22.1 33.1#
125 47.9 14.7 22.1#

