

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021799.D
 Acq On : 19 Sep 2022 11:49
 Operator : CG/JU
 Sample : PB147716BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 20 00:23:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4829	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	16242	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.707	164	9539	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.459	188	19992	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	11526	0.400	ng/ul #	0.00
23) Perylene-d12	24.155	264	9612	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	34012	5.725	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.472	152	8546	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	15427	0.360	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.702	166	2352	0.062	ng/ul#	14
20) Pyrene	19.854	202	1847	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.991	252	2872	0.081	ng/ul#	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021799.D
Acq On : 19 Sep 2022 11:49
Operator : CG/JU
Sample : PB147716BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Sep 20 00:23:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

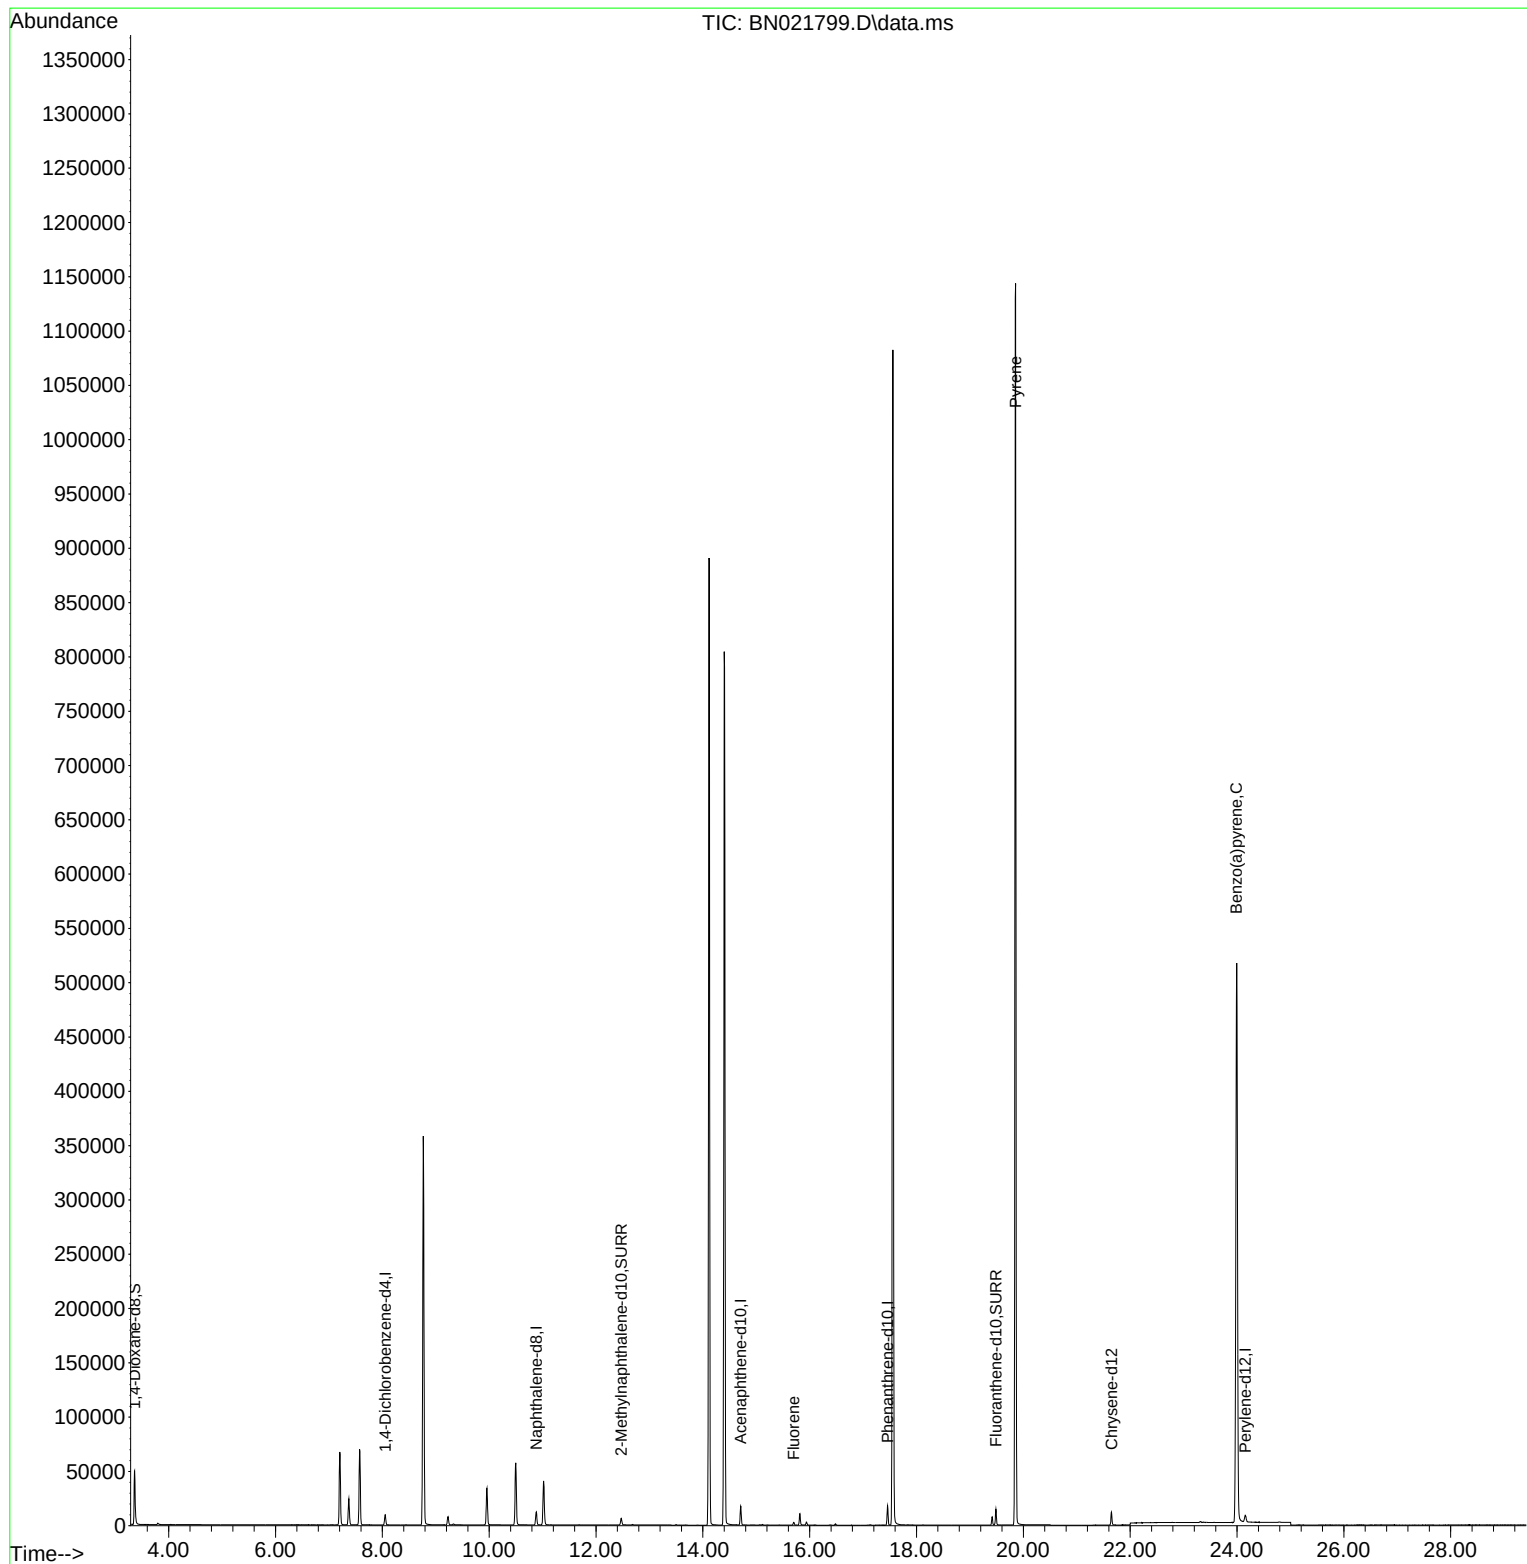



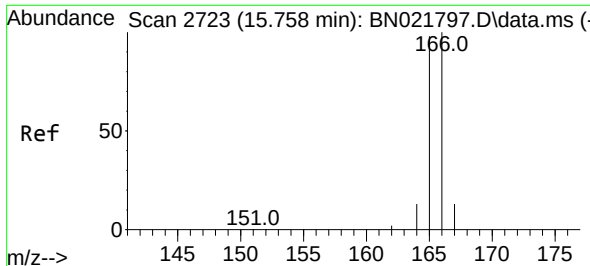


#12
Fluorene
Concen: 0.062 ng/ul
RT: 15.702 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN021799.D
Acq: 19 Sep 2022 11:49


Instrument :
BNA_M
ClientSampleId :

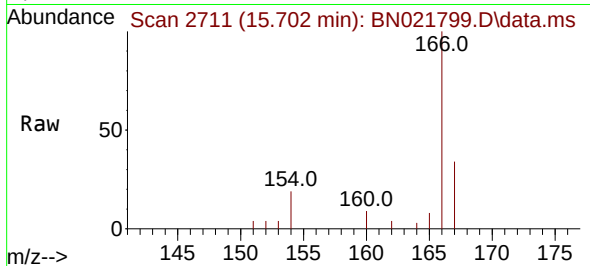



Tgt Ion:166 Resp: 2352
Ion Ratio Lower Upper
166 100
165 7.5 78.6 117.8#
167 33.6 11.8 17.6#

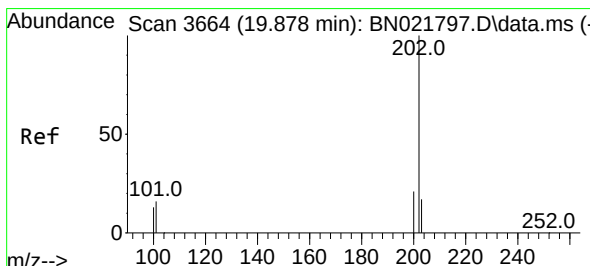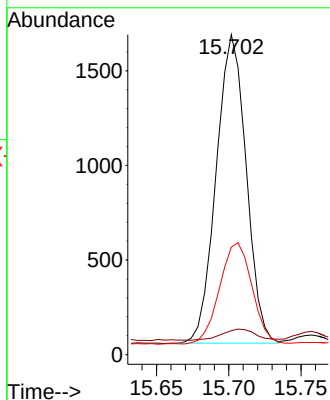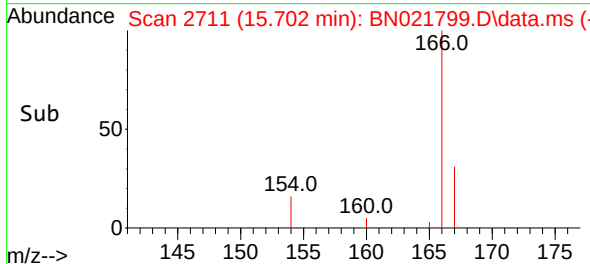


#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.854 min Scan# 3659
Delta R.T. -0.024 min
Lab File: BN021799.D
Acq: 19 Sep 2022 11:49

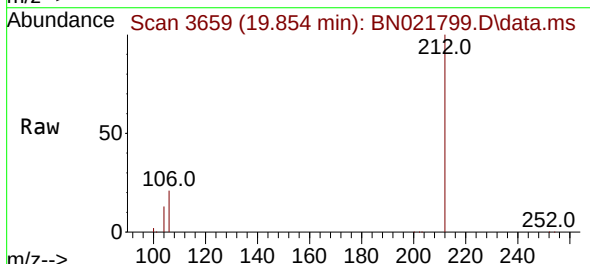


Tgt Ion:202 Resp: 1847
Ion Ratio Lower Upper
202 100
101 167.5 11.3 16.9#
100 1191.1 9.0 13.4#

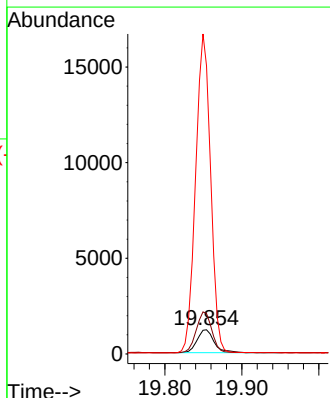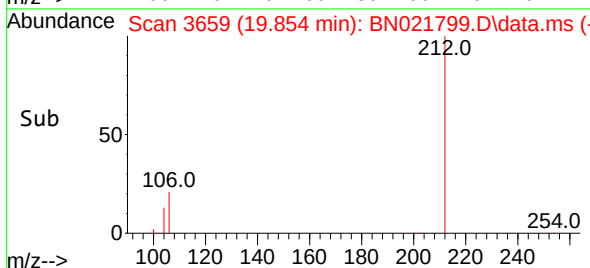

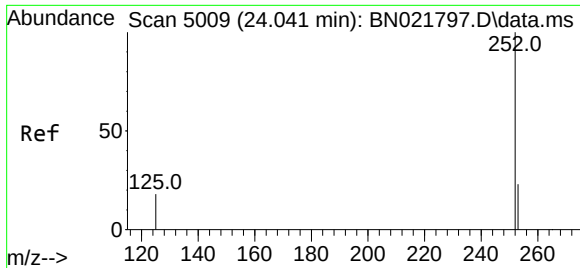

#26
 Benzo(a)pyrene
 Concen: 0.081 ng/ul
 RT: 23.991 min Scan# 49
 Delta R.T. -0.050 min
 Lab File: BN021799.D
 Acq: 19 Sep 2022 11:49

Instrument :
 BNA_M
 ClientSampleId :

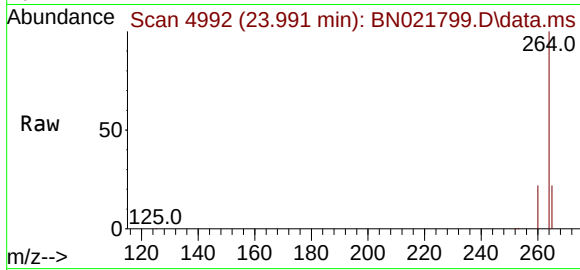

Tgt Ion:	252	Resp:	2872
Ion	Ratio	Lower	Upper
252	100		
253	47.9	22.1	33.1#
125	46.7	14.7	22.1#

