

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021811.D
 Acq On : 19 Sep 2022 19:25
 Operator : CG/JU
 Sample : PB147716BS
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 20 00:26:33 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	3898	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	13309	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.712	164	7794	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.464	188	15401	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	9533	0.400	ng/ul	# 0.00
23) Perylene-d12	24.158	264	7932	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	3418	0.713	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.473	152	8594	0.408	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	16369	0.462	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	9383	1.908	ng/ul#	88
5) Naphthalene	10.933	128	14847	0.396	ng/ul	98
7) 2-Methylnaphthalene	12.544	142	9815	0.402	ng/ul	98
8) 1-Methylnaphthalene	12.764	142	10161	0.406	ng/ul	100
10) Acenaphthylene	14.435	152	14399	0.440	ng/ul	99
11) Acenaphthene	14.772	153	10697	0.386	ng/ul	100
12) Fluorene	15.762	166	12330	0.396	ng/ul	99
14) Pentachlorophenol	17.114	266	1676	0.562	ng/ul	98
15) Phenanthrene	17.502	178	19228	0.396	ng/ul	100
16) Anthracene	17.595	178	17460	0.433	ng/ul	99
19) Fluoranthene	19.520	202	20265	0.455	ng/ul	99
20) Pyrene	19.882	202	20315	0.463	ng/ul	96
21) Benzo(a)anthracene	21.633	228	15167	0.475	ng/ul	99
22) Chrysene	21.685	228	15221	0.437	ng/ul	99
24) Benzo(b)fluoranthene	23.384	252	14215	0.369	ng/ul	89
25) Benzo(k)fluoranthene	23.433	252	13378	0.359	ng/ul#	90
26) Benzo(a)pyrene	24.041	252	13514	0.464	ng/ul#	89
27) Indeno(1,2,3-cd)pyrene	26.798	276	14946	0.456	ng/ul#	98
28) Dibenzo(a,h)anthracene	26.824	278	12248	0.440	ng/ul#	94
29) Benzo(g,h,i)perylene	27.619	276	12959	0.429	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021811.D
Acq On : 19 Sep 2022 19:25
Operator : CG/JU
Sample : PB147716BS
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Sep 20 00:26:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

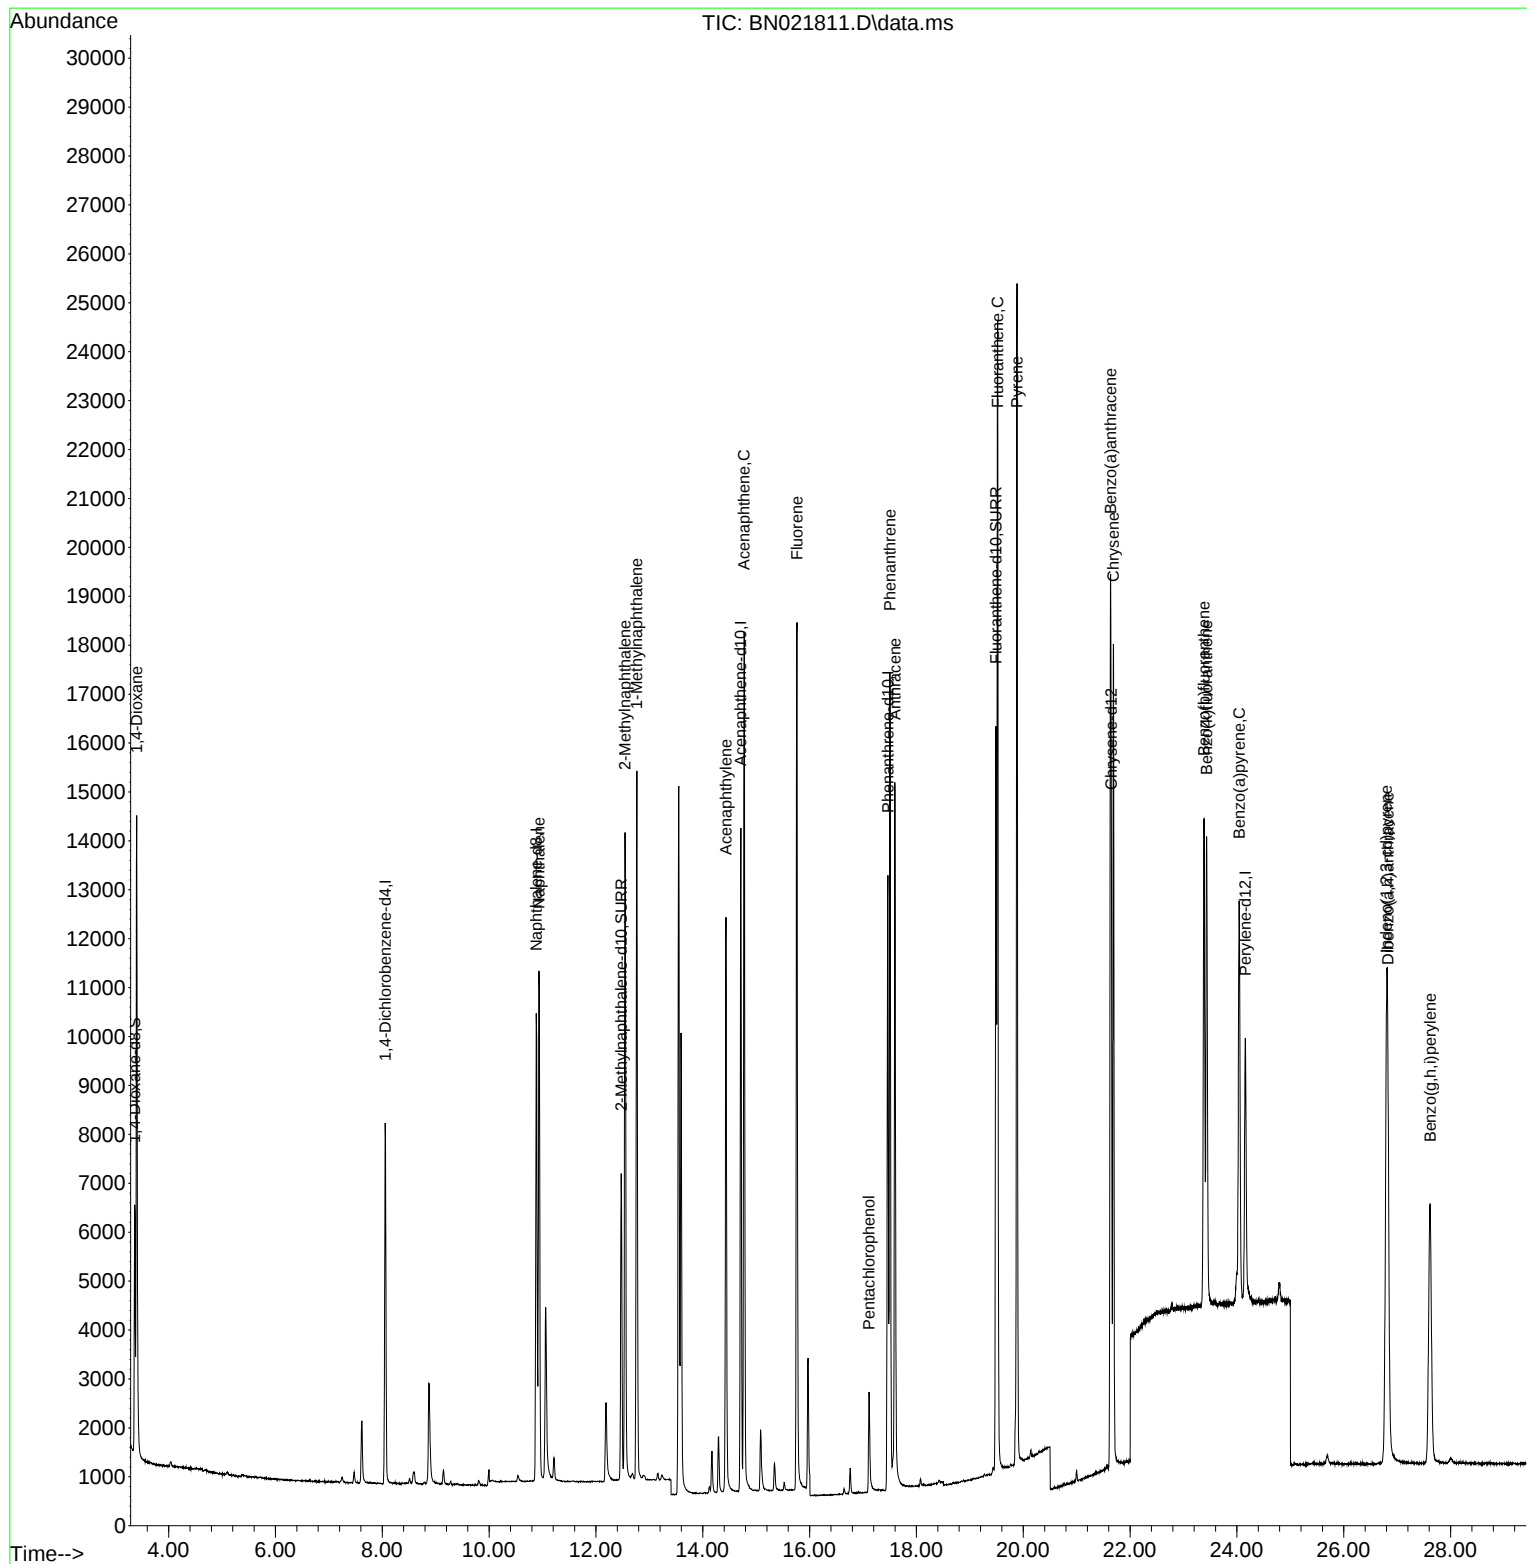



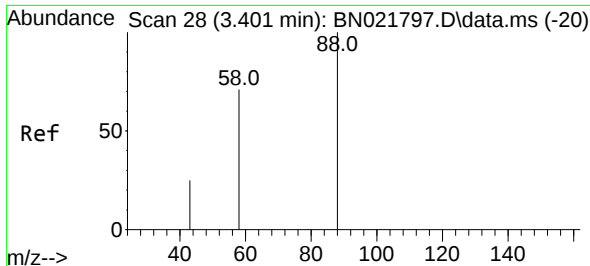


#2
 1,4-Dioxane
 Concen: 1.908 ng/ul
 RT: 3.401 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN021811.D
 Acq: 19 Sep 2022 19:25

Instrument :
 BNA_M
 ClientSampleId :



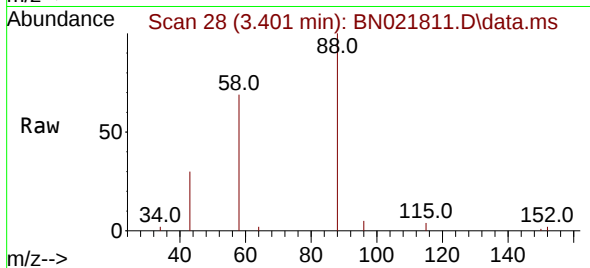



Tgt Ion: 88 Resp: 9383
 Ion Ratio Lower Upper
 88 100
 43 29.5 31.4 47.0#
 58 68.7 49.0 73.6

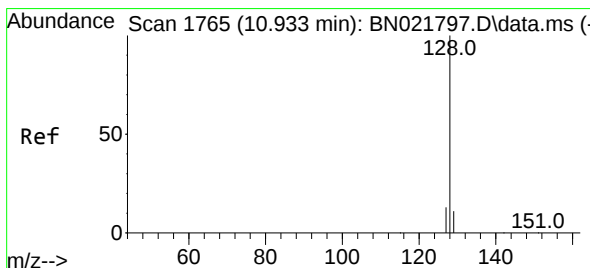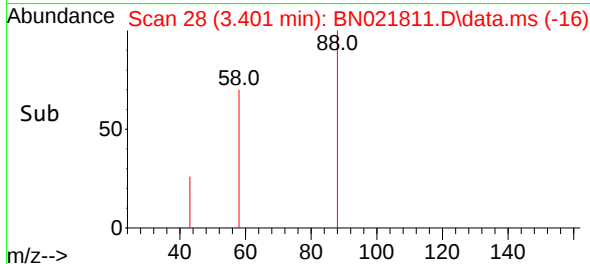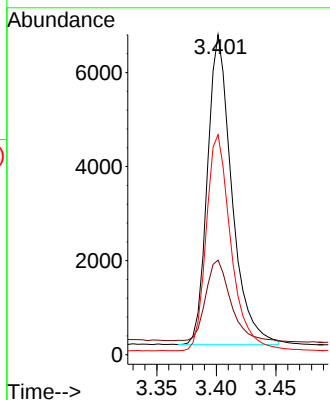

#5
 Naphthalene
 Concen: 0.396 ng/ul
 RT: 10.933 min Scan# 1765
 Delta R.T. 0.000 min
 Lab File: BN021811.D
 Acq: 19 Sep 2022 19:25

Tgt Ion: 128 Resp: 14847
 Ion Ratio Lower Upper
 128 100
 129 11.7 9.8 14.6
 127 13.6 11.6 17.4


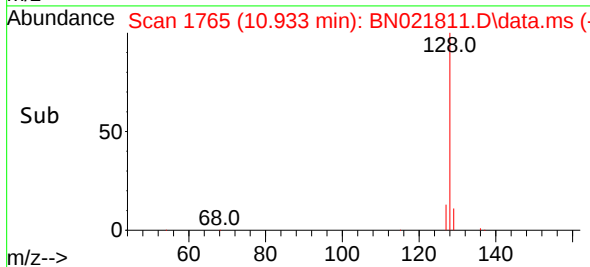
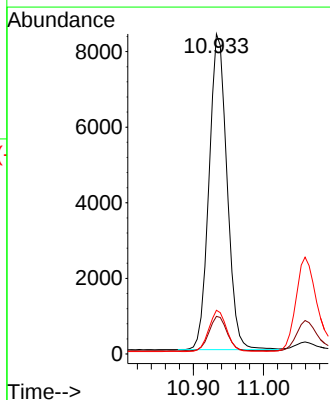
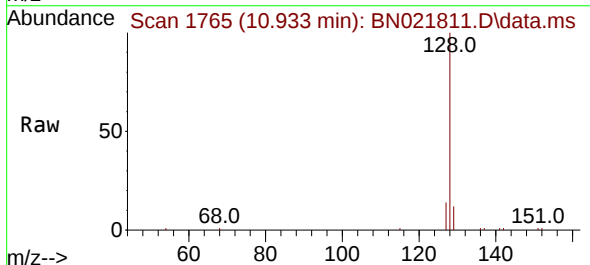




#7
2-Methylnaphthalene
Concen: 0.402 ng/ul
RT: 12.544 min Scan# 2058
Delta R.T. 0.000 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:142 Resp: 9815
Ion Ratio Lower Upper
142 100
141 88.6 72.2 108.2

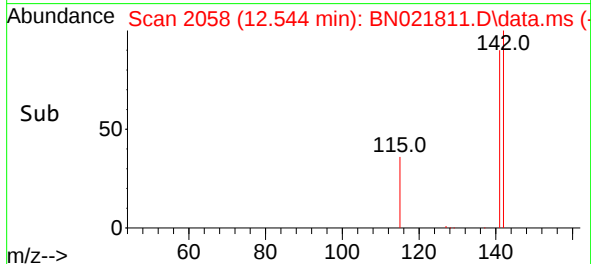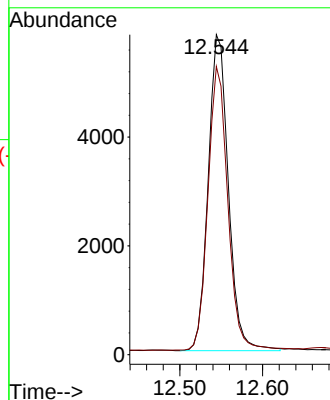

#8
1-Methylnaphthalene
Concen: 0.406 ng/ul
RT: 12.764 min Scan# 2098
Delta R.T. 0.006 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:142 Resp: 10161
Ion Ratio Lower Upper
142 100
141 92.1 73.9 110.9


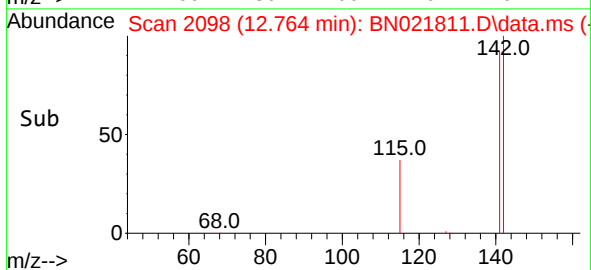
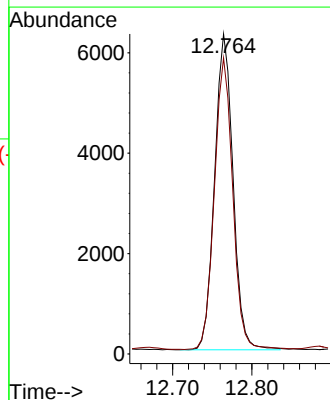
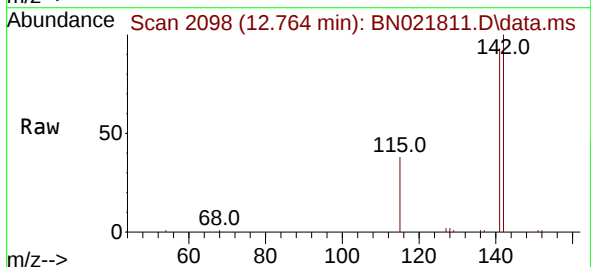




#10
Acenaphthylene
Concen: 0.440 ng/ul
RT: 14.435 min Scan# 2436
Delta R.T. 0.005 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:152 Resp: 14399
Ion Ratio Lower Upper
152 100
151 20.3 16.9 25.3
153 13.8 11.2 16.8

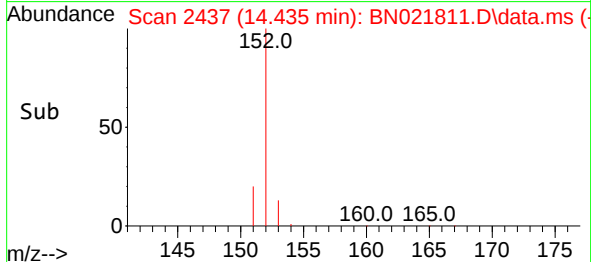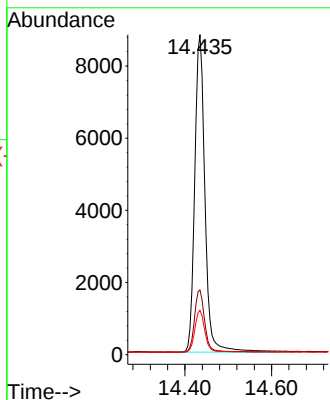

#11
Acenaphthene
Concen: 0.386 ng/ul
RT: 14.772 min Scan# 2510
Delta R.T. 0.000 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:153 Resp: 10697
Ion Ratio Lower Upper
153 100
152 50.4 40.2 60.4
154 88.1 70.7 106.1


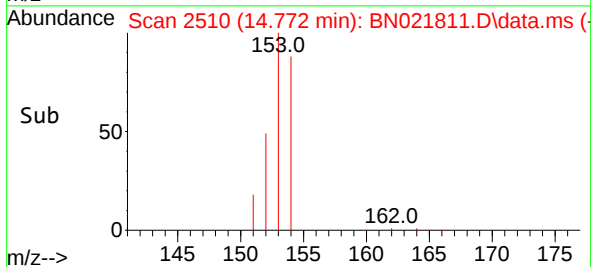
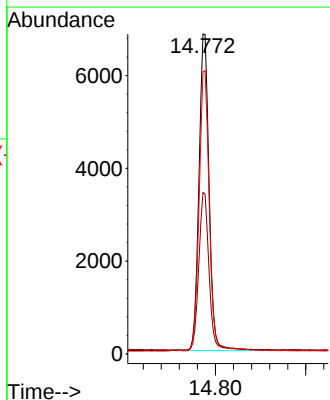
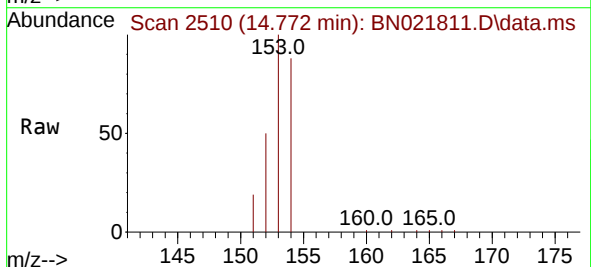




#12
Fluorene
Concen: 0.396 ng/ul
RT: 15.762 min Scan# 21
Delta R.T. 0.005 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:166 Resp: 12330
Ion Ratio Lower Upper
166 100
165 96.9 78.6 117.8
167 13.9 11.8 17.6

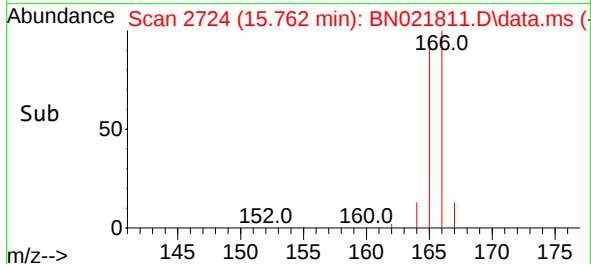

#14
Pentachlorophenol
Concen: 0.562 ng/ul
RT: 17.114 min Scan# 3039
Delta R.T. 0.004 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:266 Resp: 1676
Ion Ratio Lower Upper
266 100
264 63.2 49.8 74.8
268 64.9 50.6 75.8


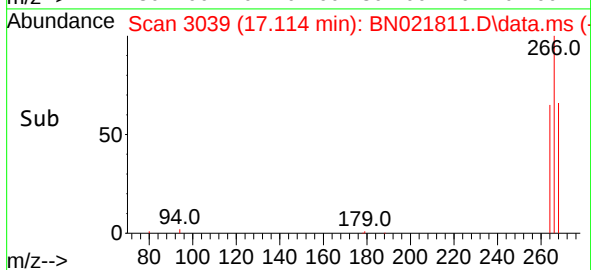

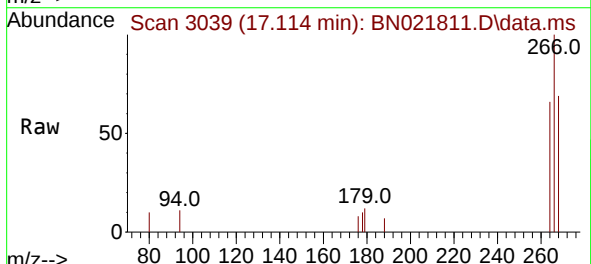




#15
Phenanthrene
Concen: 0.396 ng/u1
RT: 17.502 min Scan# 3131
Delta R.T. 0.000 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:178 Resp: 19228
Ion Ratio Lower Upper
178 100
179 16.0 12.8 19.2
176 19.8 15.9 23.9

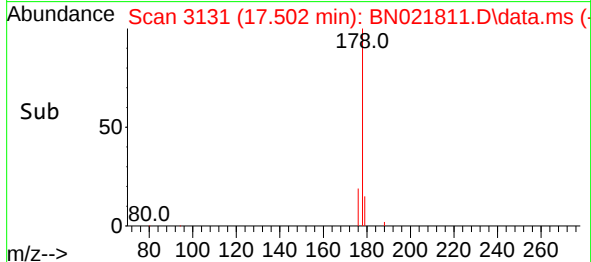

#16
Anthracene
Concen: 0.433 ng/u1
RT: 17.595 min Scan# 3153
Delta R.T. 0.000 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:178 Resp: 17460
Ion Ratio Lower Upper
178 100
179 16.2 12.9 19.3
176 19.3 15.9 23.9


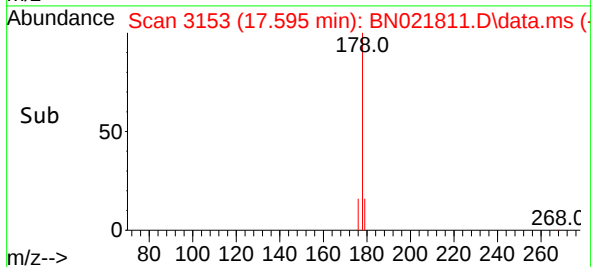

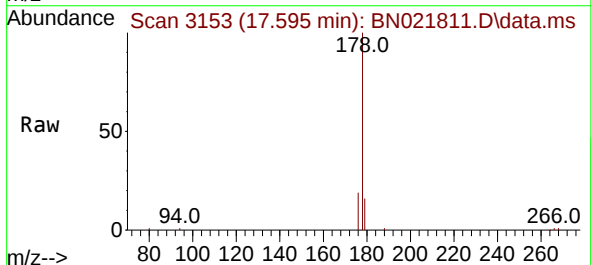




#19
Fluoranthene
Concen: 0.455 ng/u1
RT: 19.520 min Scan# 31
Delta R.T. 0.005 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:202 Resp: 20265
Ion Ratio Lower Upper
202 100
101 13.2 10.0 15.0
100 9.6 8.0 12.0

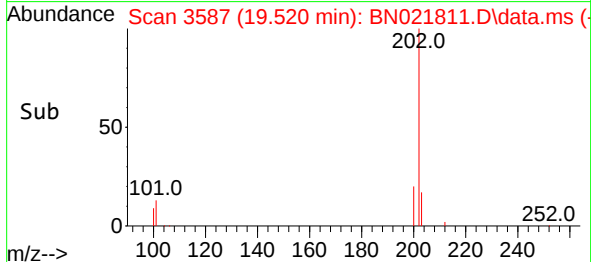

#20
Pyrene
Concen: 0.463 ng/u1
RT: 19.882 min Scan# 3665
Delta R.T. 0.005 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:202 Resp: 20315
Ion Ratio Lower Upper
202 100
101 15.9 11.3 16.9
100 12.4 9.0 13.4


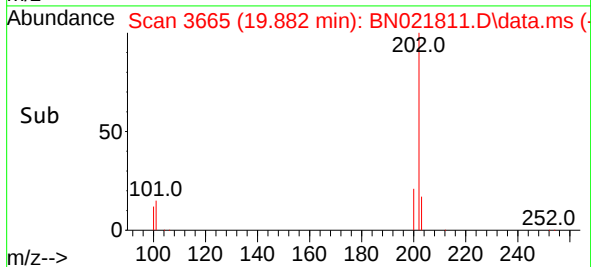

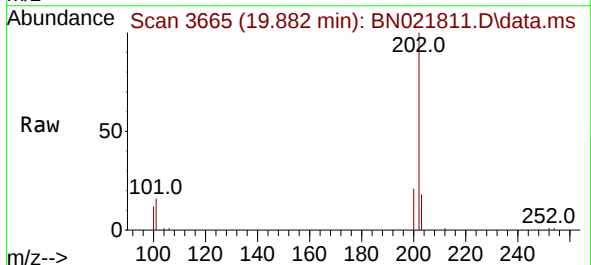


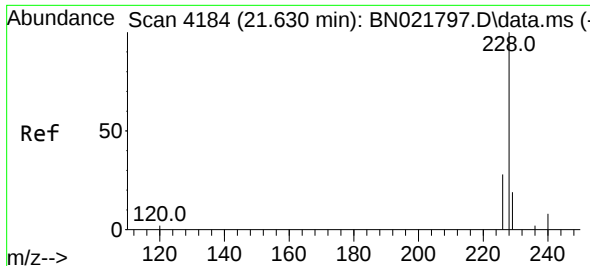

#21
Benzo(a)anthracene
Concen: 0.475 ng/ul
RT: 21.633 min Scan# 4184
Delta R.T. 0.003 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:228 Resp: 15167
Ion Ratio Lower Upper
228 100
229 20.6 16.0 24.0
226 28.2 21.9 32.9

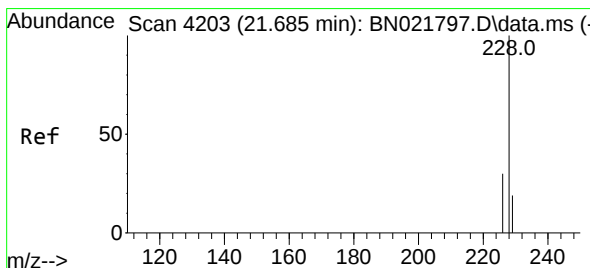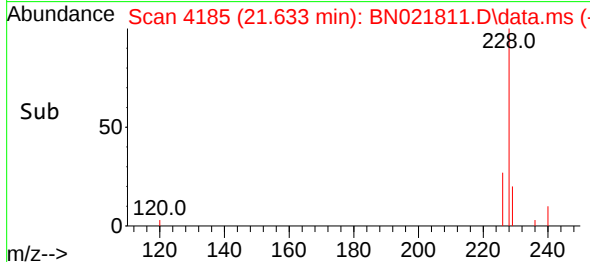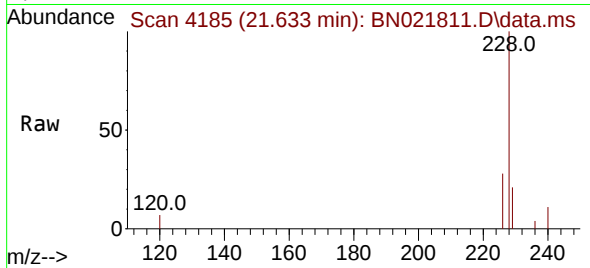

#22
Chrysene
Concen: 0.437 ng/ul
RT: 21.685 min Scan# 4203
Delta R.T. 0.000 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:228 Resp: 15221
Ion Ratio Lower Upper
228 100
226 31.3 24.6 37.0
229 20.4 15.8 23.8


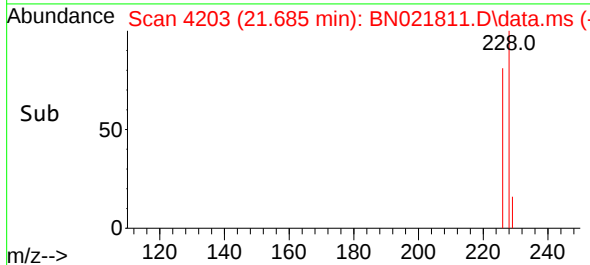

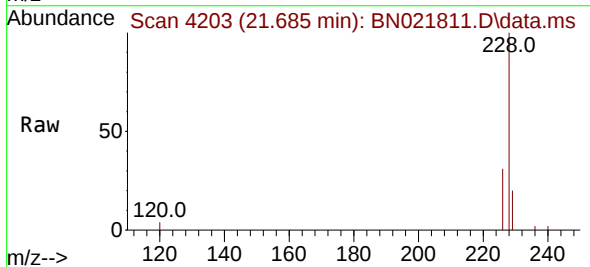




#24
Benzo(b)fluoranthene
Concen: 0.369 ng/ul
RT: 23.384 min Scan# 4783
Delta R.T. 0.003 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:252 Resp: 14215
Ion Ratio Lower Upper
252 100
253 29.5 0.0 50.8
125 21.7 0.0 30.0

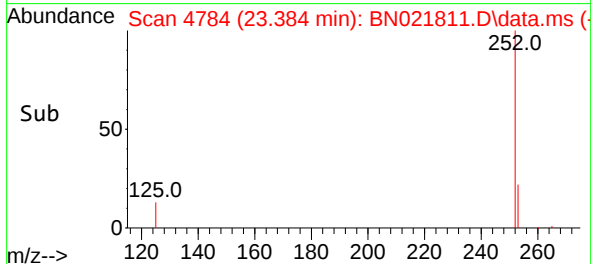

#25
Benzo(k)fluoranthene
Concen: 0.359 ng/ul
RT: 23.433 min Scan# 4801
Delta R.T. 0.003 min
Lab File: BN021811.D
Acq: 19 Sep 2022 19:25

Tgt Ion:252 Resp: 13378
Ion Ratio Lower Upper
252 100
253 29.4 20.6 31.0
125 21.4 11.8 17.6#

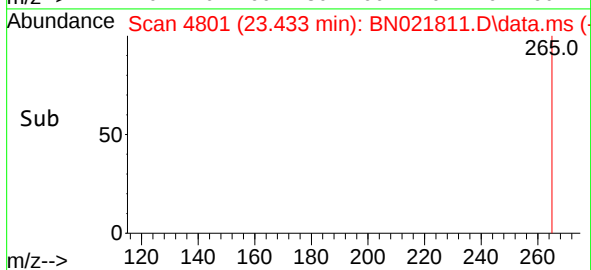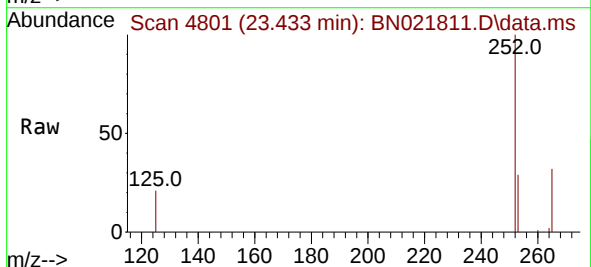



#26

Benzo(a)pyrene

Concen: 0.464 ng/ul

RT: 24.041 min Scan# 5009

Delta R.T. 0.000 min


Lab File: BN021811.D

Acq: 19 Sep 2022 19:25




Instrument :

BNA_M

ClientSampleId :

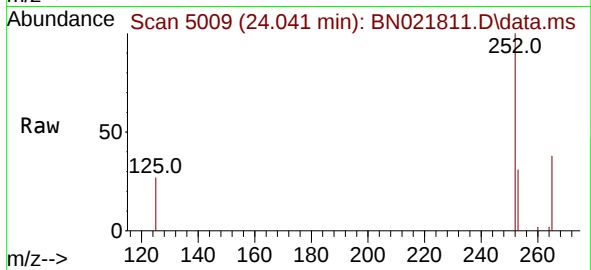

Tgt Ion:	252	Resp:	13514
Ion Ratio	Lower	Upper	
252	100		
253	31.0	22.1	33.1
125	26.5	14.7	22.1#

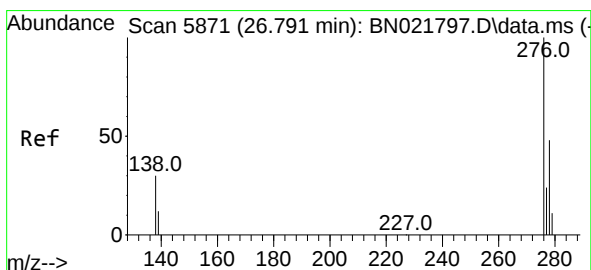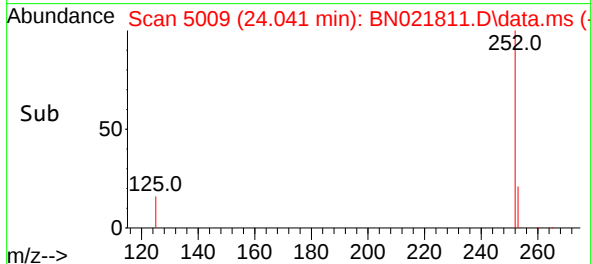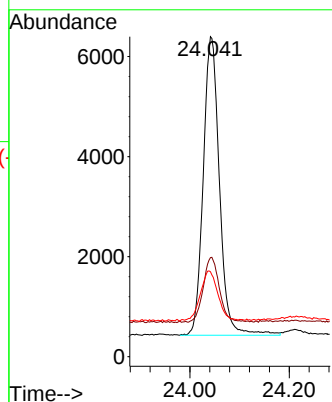

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.456 ng/ul




RT: 26.798 min Scan# 5873


Delta R.T. 0.007 min

Lab File: BN021811.D

Acq: 19 Sep 2022 19:25


Tgt Ion:	276	Resp:	14946
Ion Ratio	Lower	Upper	
276	100		
138	33.9	26.1	39.1
227	0.1	0.1	0.1#

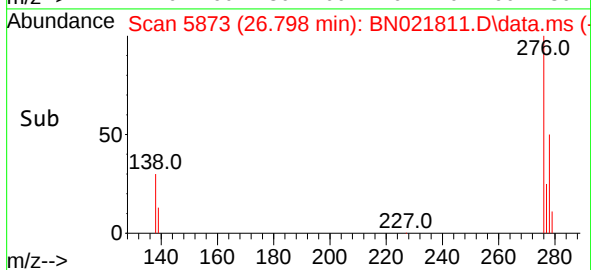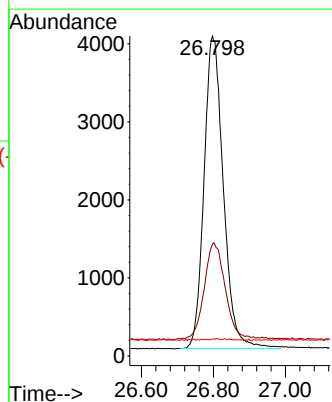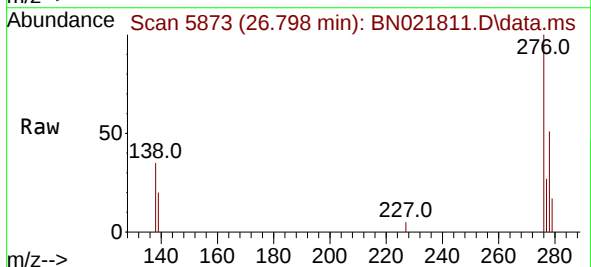






#28
 Dibenzo(a,h)anthracene
 Concen: 0.440 ng/ul
 RT: 26.824 min Scan# 5881
 Delta R.T. 0.007 min
 Lab File: BN021811.D
 Acq: 19 Sep 2022 19:25

Instrument :
 BNA_M
 ClientSampleId :



Tgt Ion:278 Resp: 12248
 Ion Ratio Lower Upper
 278 100
 139 28.2 18.3 27.5#
 279 29.0 23.9 35.9

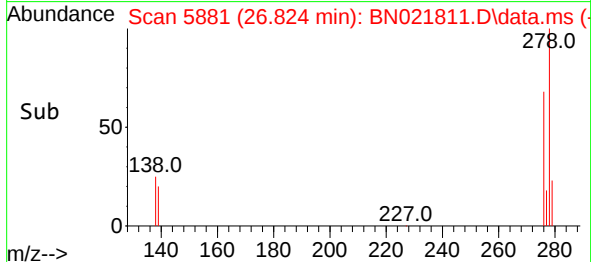

#29
 Benzo(g,h,i)perylene
 Concen: 0.429 ng/ul
 RT: 27.619 min Scan# 6118
 Delta R.T. 0.010 min
 Lab File: BN021811.D
 Acq: 19 Sep 2022 19:25

Tgt Ion:276 Resp: 12959
 Ion Ratio Lower Upper
 276 100
 138 32.0 22.6 34.0
 277 26.0 20.2 30.2

