

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021814.D
 Acq On : 19 Sep 2022 21:57
 Operator : CG/JU
 Sample : PB147719BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 20 00:27:19 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	5161	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	17449	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.712	164	10031	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	20015	0.400	ng/ul	0.00
17) Chrysene-d12	21.647	240	11590	0.400	ng/ul #	0.00
23) Perylene-d12	24.152	264	9739	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	33584	5.289	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.473	152	8794	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	16018	0.372	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.850	202	1797	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.989	252	2841	0.079	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021814.D
Acq On : 19 Sep 2022 21:57
Operator : CG/JU
Sample : PB147719BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 20 00:27:19 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration




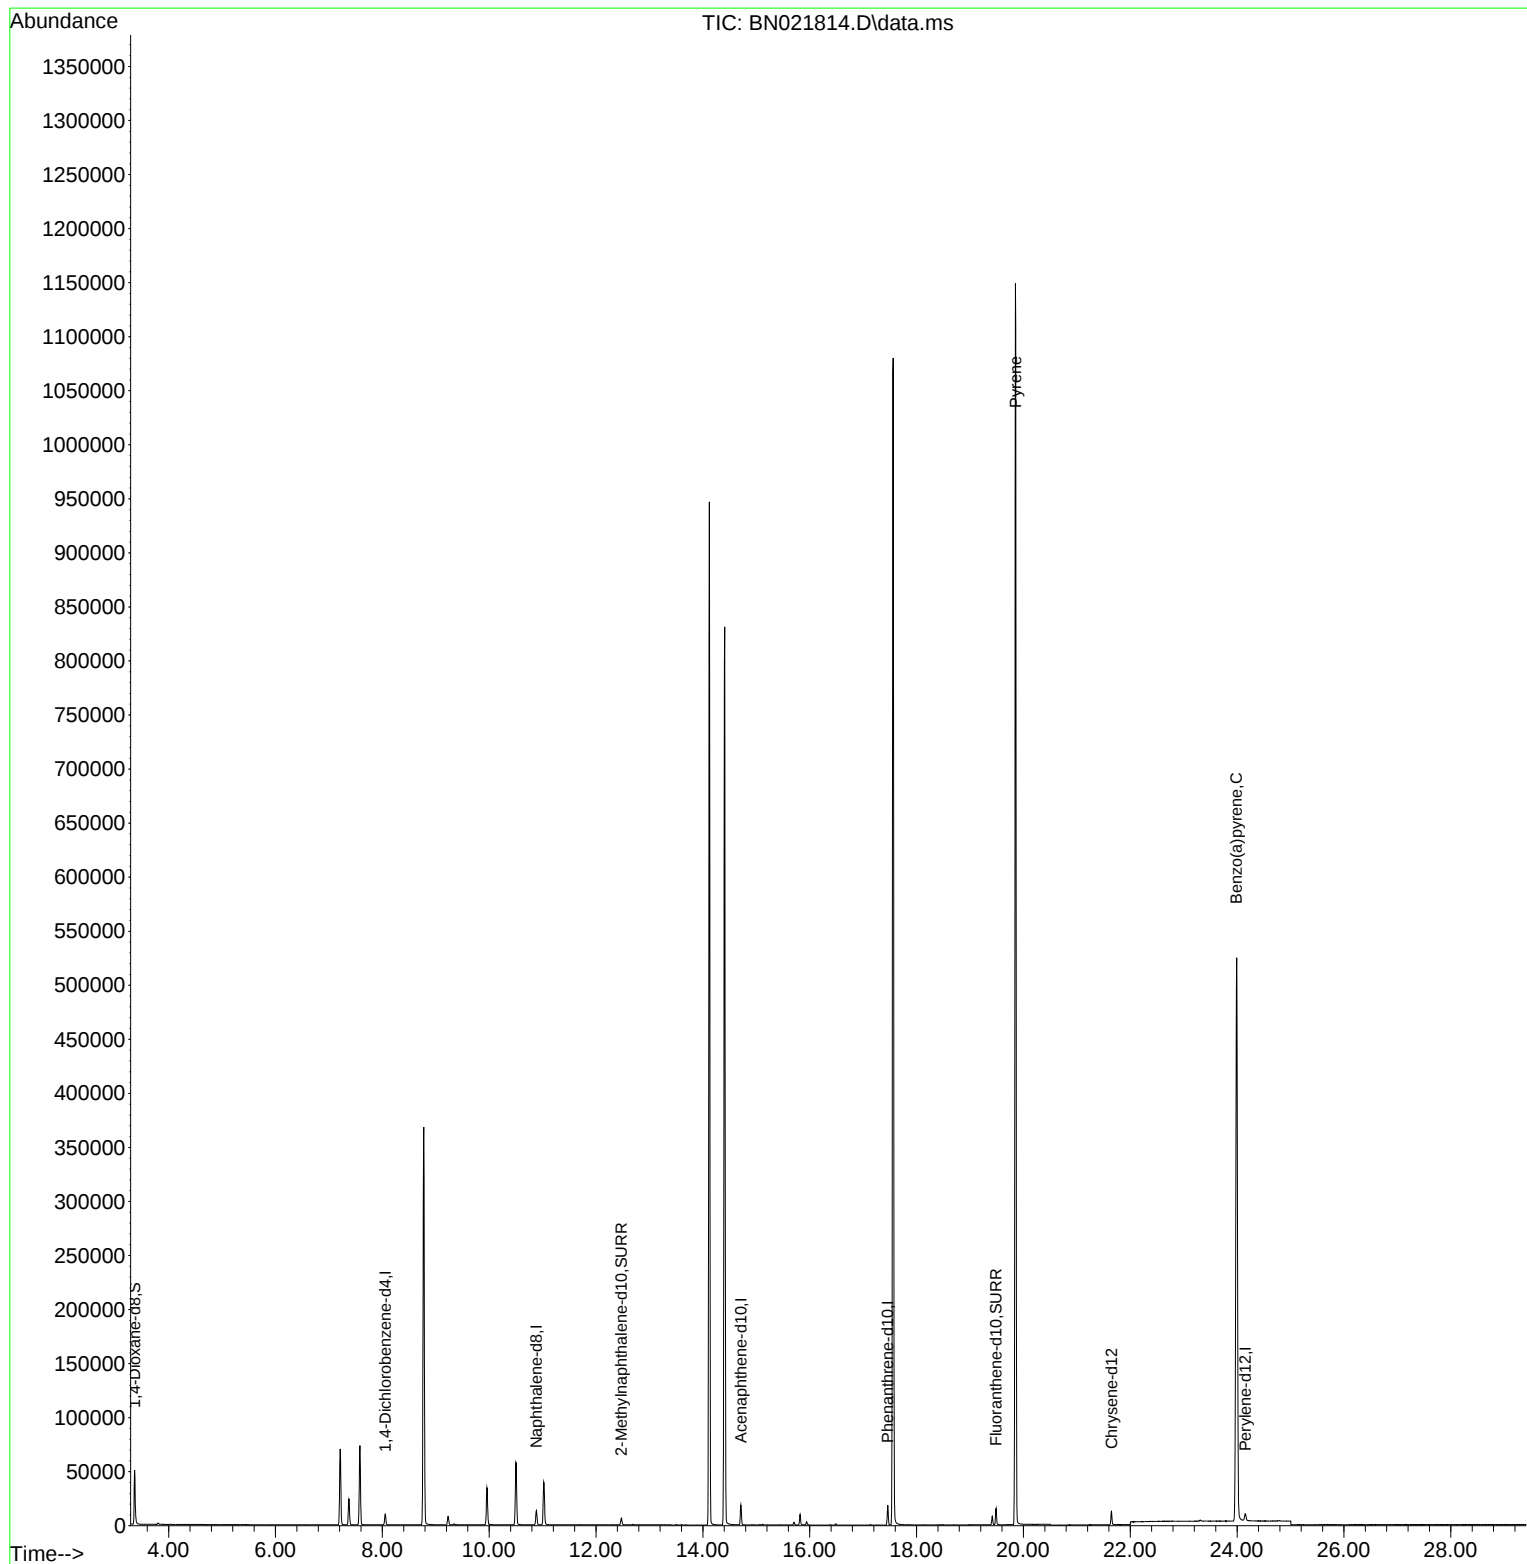


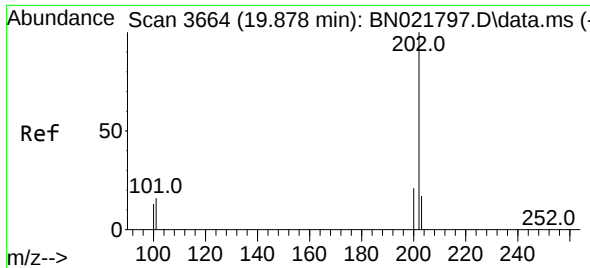

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.850 min Scan# 30
Delta R.T. -0.028 min
Lab File: BN021814.D
Acq: 19 Sep 2022 21:57

Instrument :
BNA_M
ClientSampleId :

Tgt Ion:202 Resp: 1797
Ion Ratio Lower Upper
202 100
101 176.7 11.3 16.9#
100 1324.2 9.0 13.4#

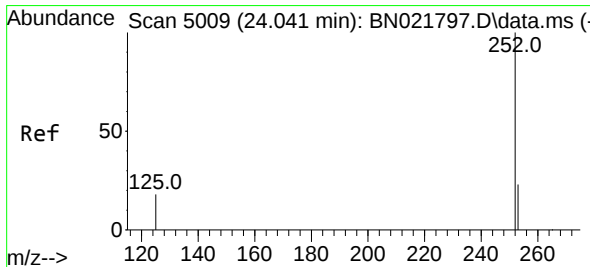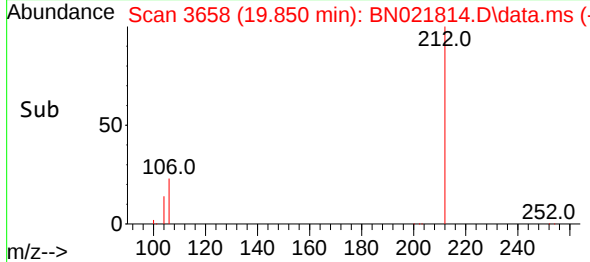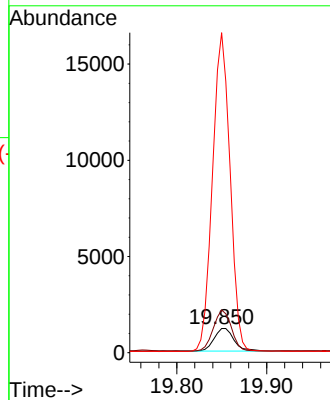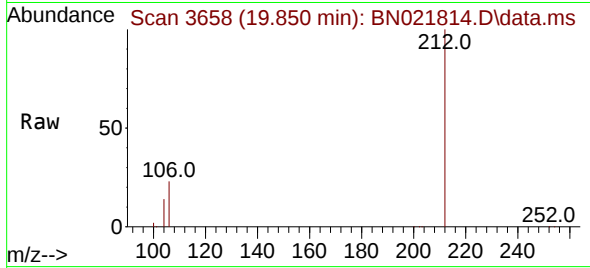

#26
Benzo(a)pyrene
Concen: 0.079 ng/ul
RT: 23.989 min Scan# 4991
Delta R.T. -0.053 min
Lab File: BN021814.D
Acq: 19 Sep 2022 21:57

Tgt Ion:252 Resp: 2841
Ion Ratio Lower Upper
252 100
253 56.7 22.1 33.1#
125 53.7 14.7 22.1#

