

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091922\
 Data File : BM036590.D
 Acq On : 19 Sep 2022 21:12
 Operator : CG/JU
 Sample : N4604-22
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5782

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/20/2022
 Supervised By :mohammad ahmed 09/21/2022

Quant Time: Sep 19 22:35:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 16 02:39:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	397599	20.000	ng/u1	0.00
20) Naphthalene-d8	10.839	136	1809025	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.651	164	1161654	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	2383382	20.000	ng/u1	0.00
79) Chrysene-d12	21.550	240	2255282	20.000	ng/u1	0.00
88) Perylene-d12	23.991	264	2037392	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	42895	4.044	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.175	99	831949	23.415	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.351	67	544473	25.233	ng/u1	0.00
11) 2-Chlorophenol-d4	7.551	132	674581	26.371	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	546696	20.823	ng/u1	0.00
21) Nitrobenzene-d5	9.192	128	340874	27.839	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	335500	30.590	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	641005	25.219	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	223000	5.277	ng/u1	0.00
46) Dimethylphthalate-d6	14.062	166	2112797	26.967	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	2543579	27.370	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	298179	19.622	ng/u1	0.00
60) Fluorene-d10	15.639	176	1903914	27.117	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	228680	24.251	ng/u1	0.00
73) Anthracene-d10	17.486	188	2737416	25.120	ng/u1	0.00
81) Pyrene-d10	19.768	212	3375142	30.420	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.838	264	2755169	27.679	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.892	128	132729	1.347	ng/u1	100
36) 2-Methylnaphthalene	12.492	142	82891	1.262	ng/u1	100
37) 1-Methylnaphthalene	12.710	142	70721	1.071	ng/u1	99
71) Pentachlorophenol	17.033	266	174870	10.595	ng/u1	99
72) Phenanthrene	17.427	178	787335	5.997	ng/u1	99
80) Fluoranthene	19.433	202	868345	6.387	ng/u1	99
82) Pyrene	19.792	202	638331	4.435	ng/u1	96
85) Benzo(a)anthracene	21.533	228	462636m	3.274	ng/u1	
87) Chrysene	21.586	228	960287	7.160	ng/u1	97
90) Benzo(b)fluoranthene	23.244	252	695045	5.380	ng/u1	97
91) Benzo(k)fluoranthene	23.291	252	193625m	1.500	ng/u1	
93) Benzo(a)pyrene	23.885	252	286017	2.518	ng/u1	96
94) Indeno(1,2,3-cd)pyrene	26.538	276	187570	1.414	ng/u1	99
96) Benzo(g,h,i)perylene	27.315	276	146187	1.271	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091922\
Data File : BM036590.D
Acq On : 19 Sep 2022 21:12
Operator : CG/JU
Sample : N4604-22
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A5782

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022


Quant Time: Sep 19 22:35:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 16 02:39:54 2022
Response via : Initial Calibration

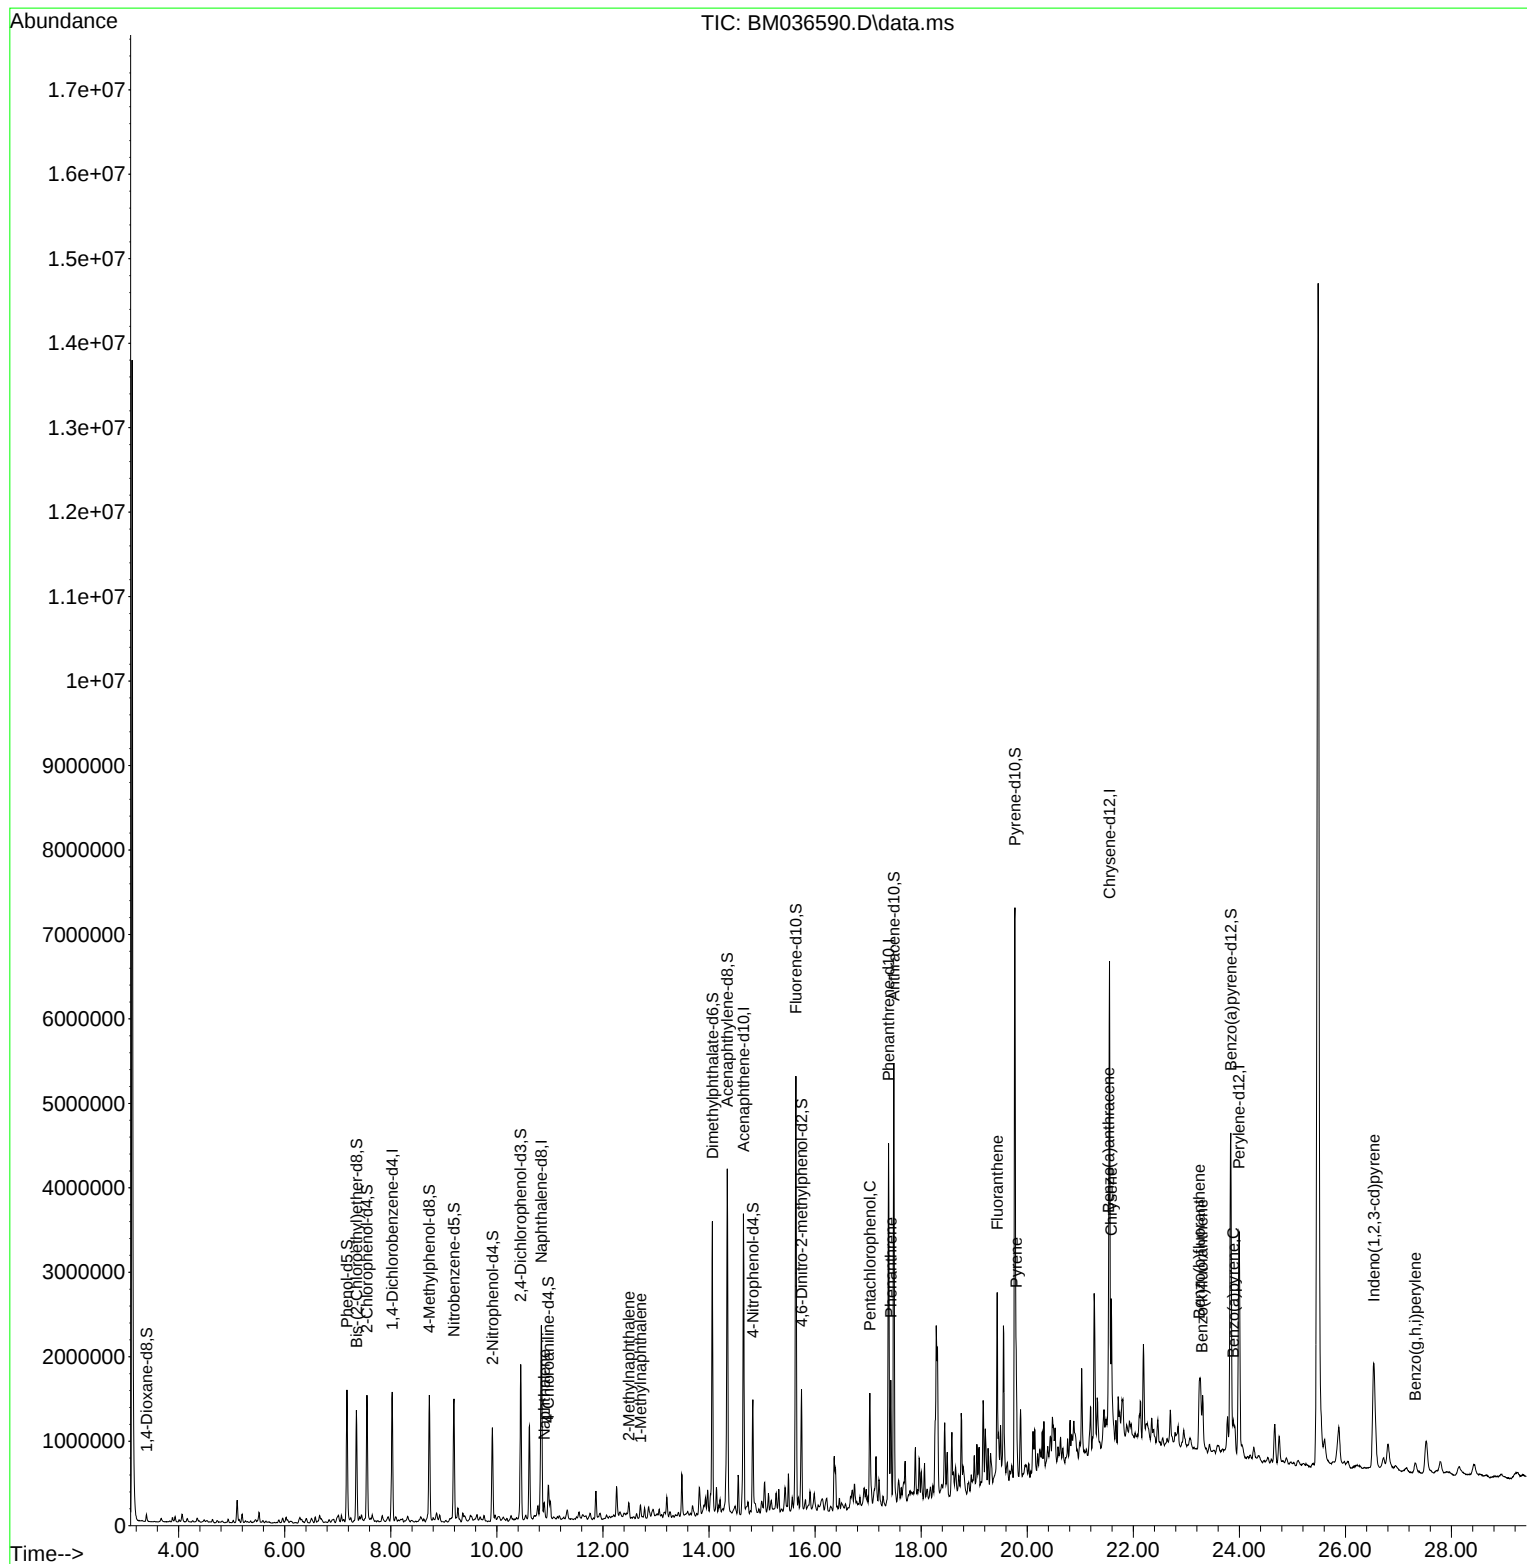

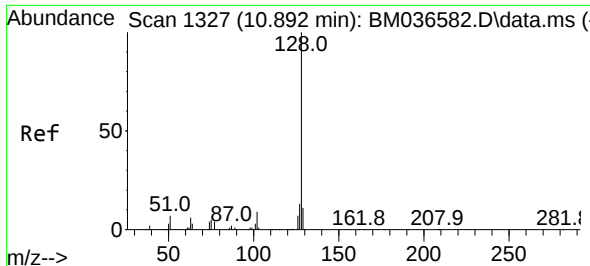

#30
Naphthalene
Concen: 1.347 ng/ul
RT: 10.892 min Scan# 1327
Delta R.T. -0.000 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12




Instrument :
BNA_M
ClientSampleId :
A5782

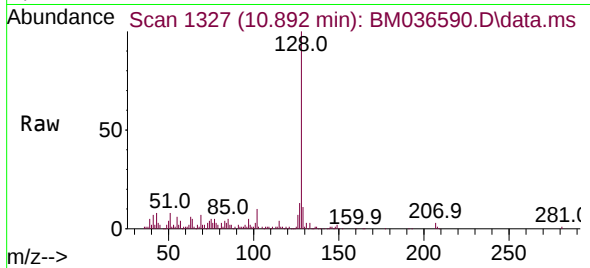

Tgt Ion:128 Resp: 132729
Ion Ratio Lower Upper
128 100
129 11.2 8.7 13.1
127 12.9 10.3 15.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

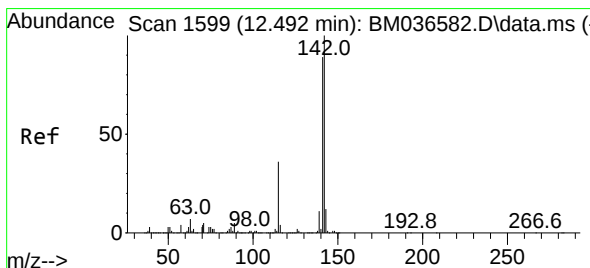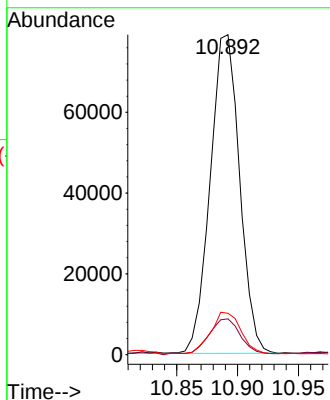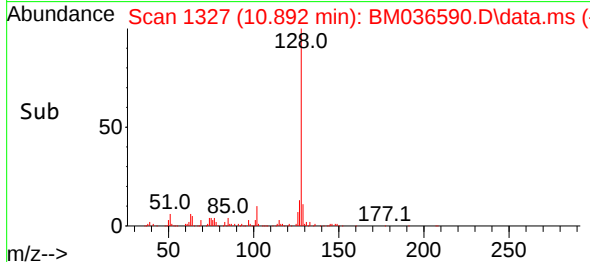

#36
2-Methylnaphthalene
Concen: 1.262 ng/ul
RT: 12.492 min Scan# 1599
Delta R.T. -0.000 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12

Tgt Ion:142 Resp: 82891
Ion Ratio Lower Upper
142 100
141 88.2 70.7 106.1

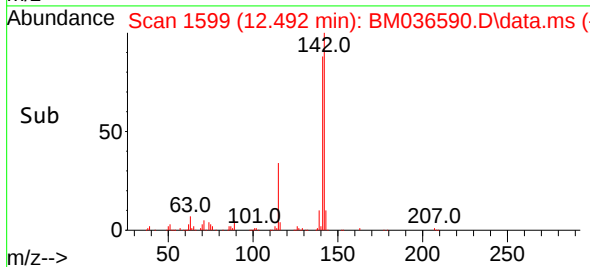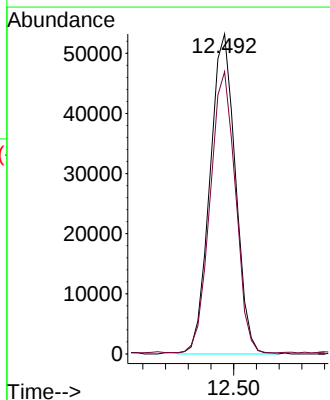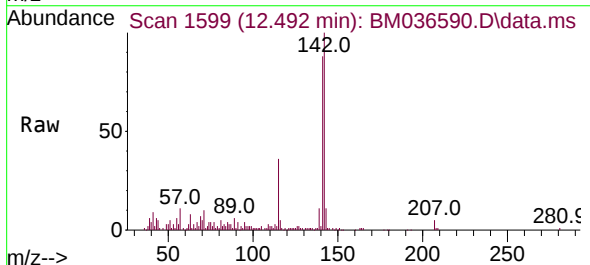

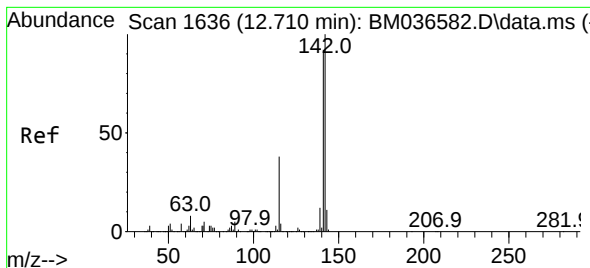

#37

1-Methylnaphthalene

Concen: 1.071 ng/ul

RT: 12.710 min Scan# 1636

Delta R.T. -0.000 min

Lab File: BM036590.D

Acq: 19 Sep 2022 21:12

Instrument :

BNA_M

ClientSampleId :





A5782

Tgt Ion:	142	Resp:	7072
Ion Ratio	Lower	Upper	
142	100		
141	93.1	73.4	110.2
116	3.9	3.1	4.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

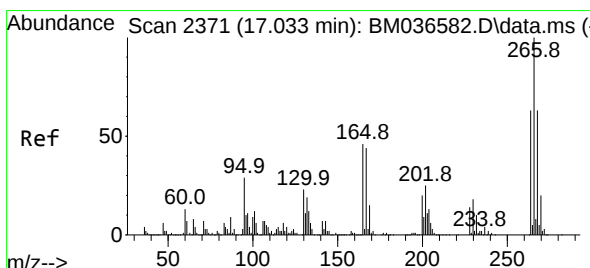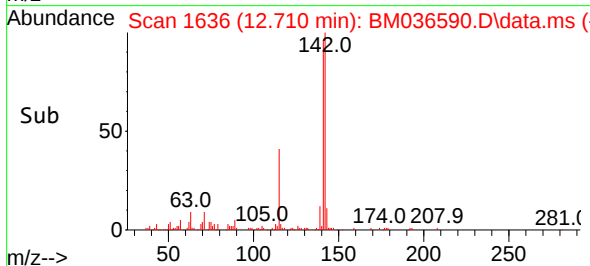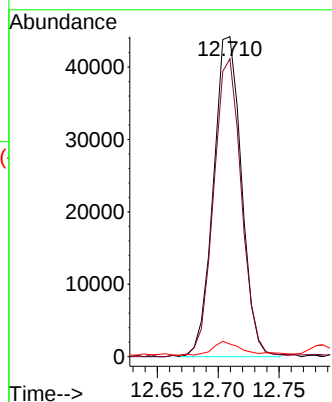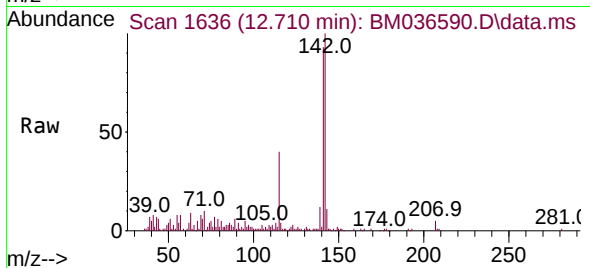

#71

Pentachlorophenol

Concen: 10.595 ng/ul




RT: 17.033 min Scan# 2371


Delta R.T. -0.000 min

Lab File: BM036590.D

Acq: 19 Sep 2022 21:12


Tgt Ion:	266	Resp:	174870
Ion Ratio	Lower	Upper	
266	100		
264	61.7	49.7	74.5
268	65.3	51.8	77.6

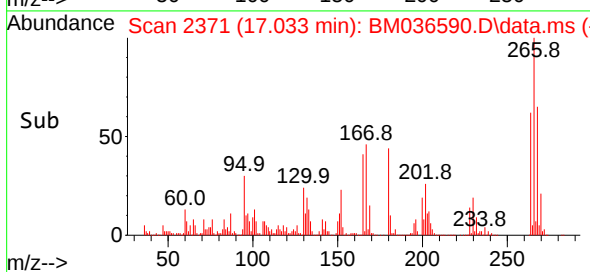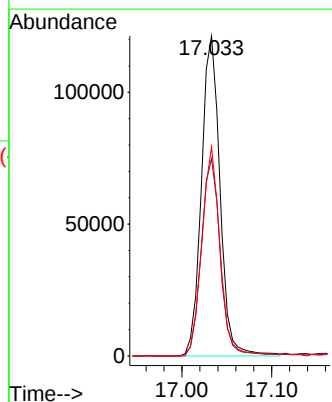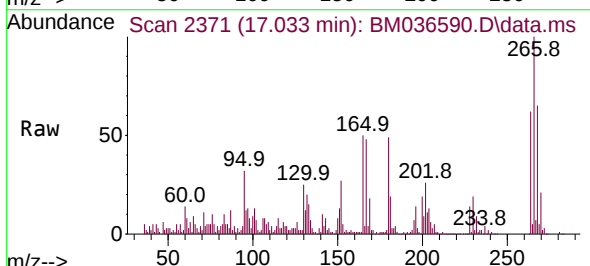

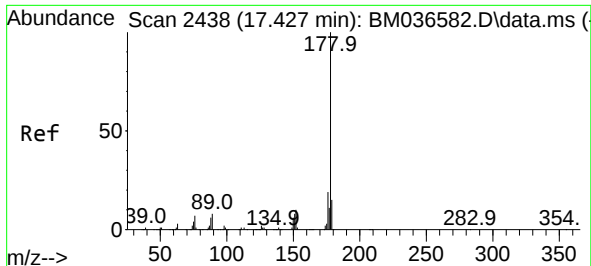

#72
Phenanthrene
Concen: 5.997 ng/ul
RT: 17.427 min Scan# 2438
Delta R.T. -0.006 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12




Instrument :
BNA_M
ClientSampleId :
A5782

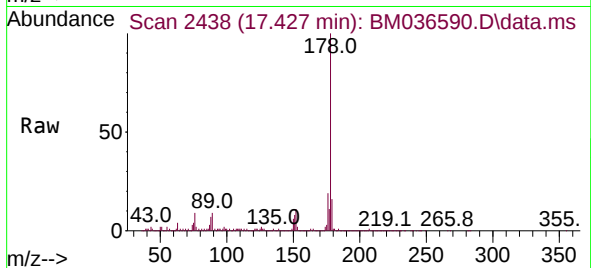

Tgt Ion:178 Resp: 787335
Ion Ratio Lower Upper
178 100
179 15.9 12.2 18.2
176 19.3 15.7 23.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

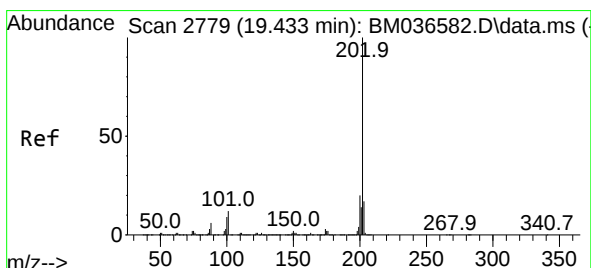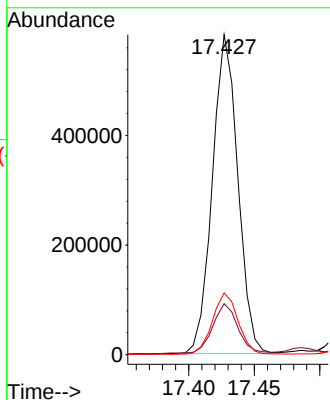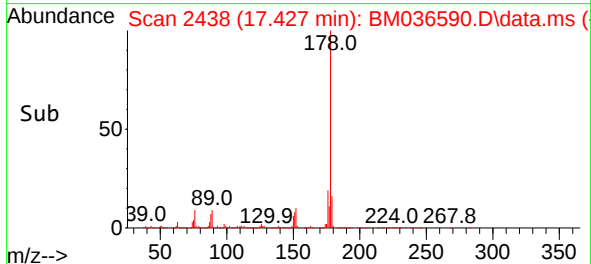

#80
Fluoranthene
Concen: 6.387 ng/ul
RT: 19.433 min Scan# 2779
Delta R.T. -0.000 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12


Tgt Ion:202 Resp: 868345
Ion Ratio Lower Upper
202 100
101 12.7 9.8 14.6
100 9.3 7.4 11.2

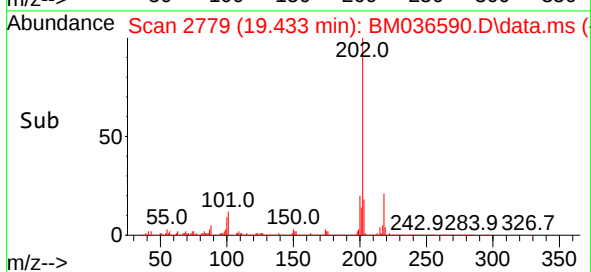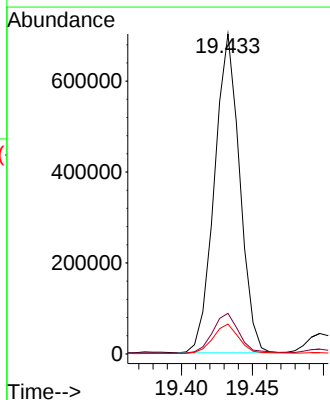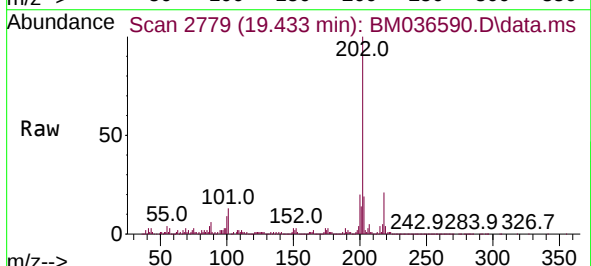

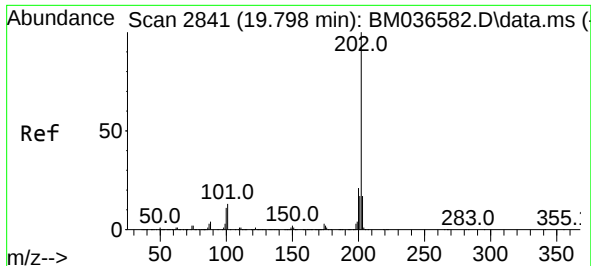

#82
Pyrene
Concen: 4.435 ng/ul
RT: 19.792 min Scan# 2841
Delta R.T. -0.006 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12




Instrument :
BNA_M
ClientSampleId :
A5782

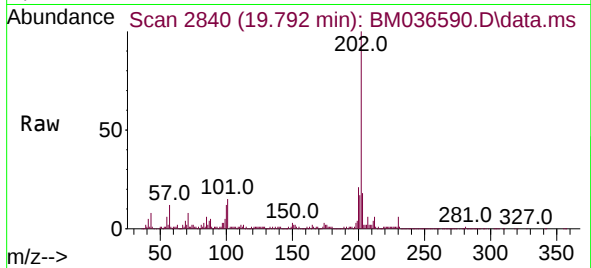


Tgt Ion:202 Resp: 63833
Ion Ratio Lower Upper
202 100
101 15.4 10.9 16.3
100 11.9 8.7 13.1

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

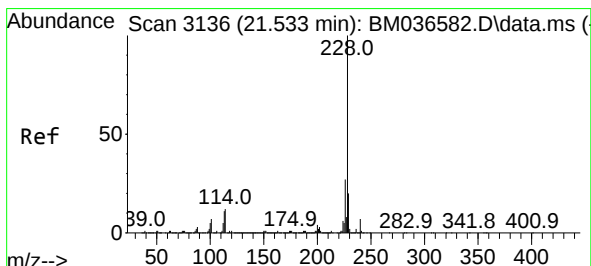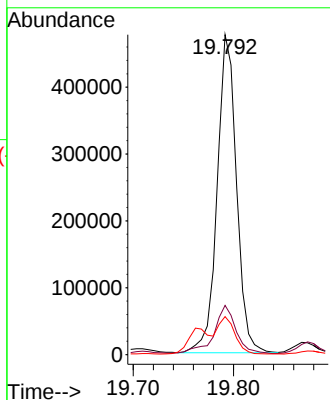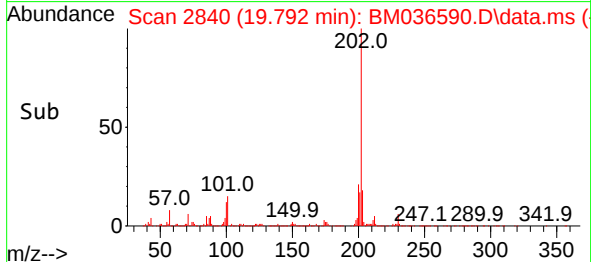


#85
Benzo(a)anthracene
Concen: 3.274 ng/ul m
RT: 21.533 min Scan# 3136
Delta R.T. -0.006 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12

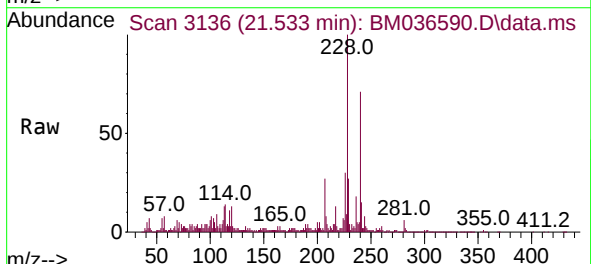


Tgt Ion:228 Resp: 462636
Ion Ratio Lower Upper
228 100
229 26.6 15.8 23.8#
226 29.8 21.9 32.9

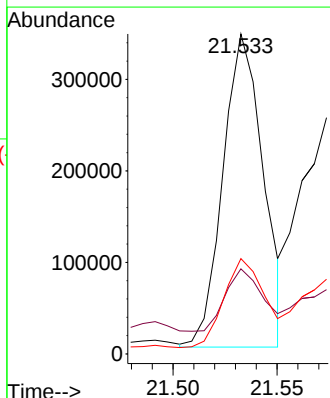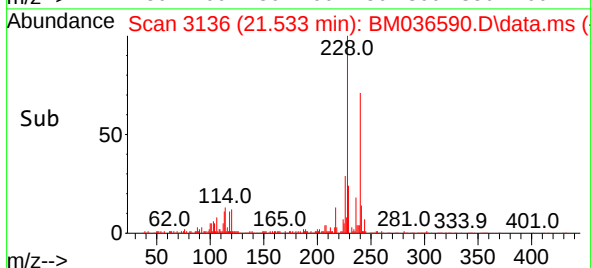

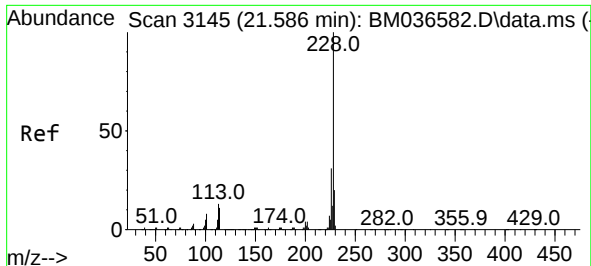

#87
Chrysene
Concen: 7.160 ng/ul
RT: 21.586 min Scan# 3145
Delta R.T. -0.006 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12




Instrument :
BNA_M
ClientSampleId :
A5782

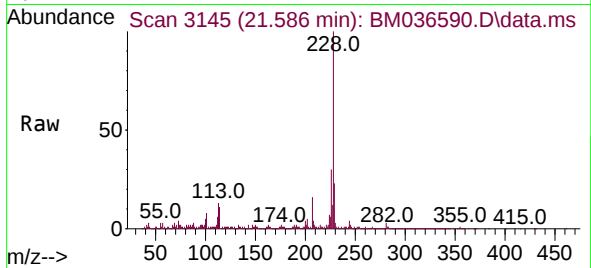


Tgt Ion:228 Resp: 960287
Ion Ratio Lower Upper
228 100
226 30.3 24.4 36.6
229 22.6 15.6 23.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

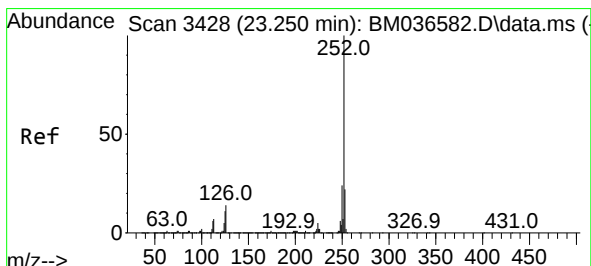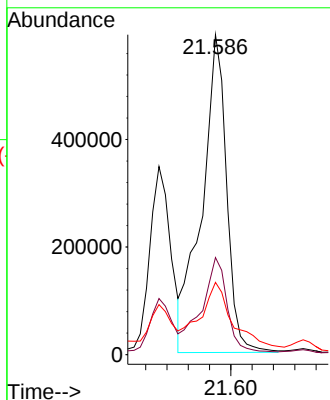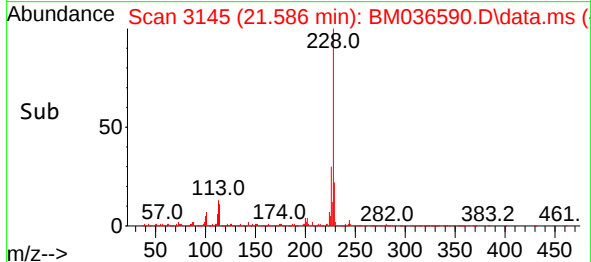


#90
Benzo(b)fluoranthene
Concen: 5.380 ng/ul
RT: 23.244 min Scan# 3427
Delta R.T. -0.006 min
Lab File: BM036590.D
Acq: 19 Sep 2022 21:12

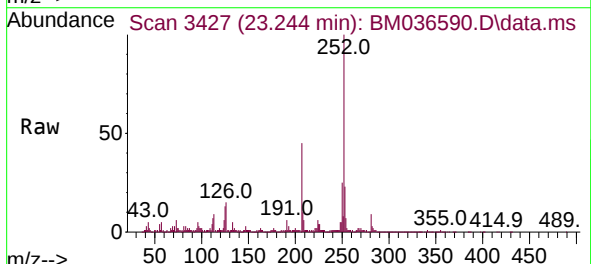

Tgt Ion:252 Resp: 695045
Ion Ratio Lower Upper
252 100
253 22.9 17.6 26.4
125 12.8 9.1 13.7

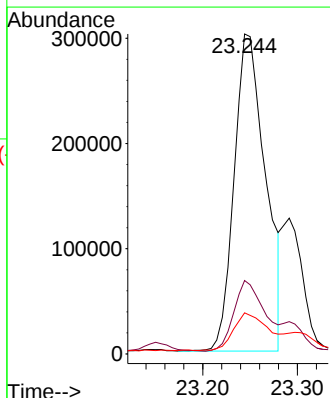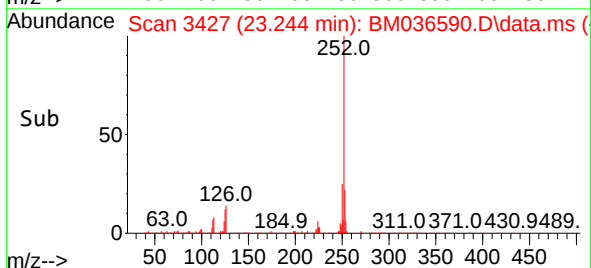

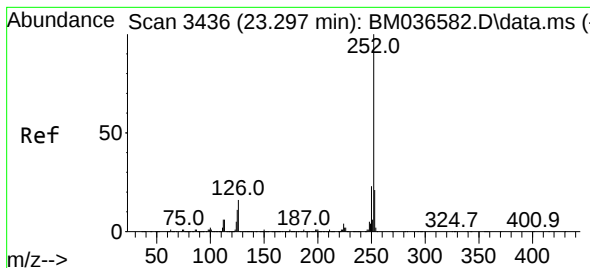

#91

Benzo(k)fluoranthene

Concen: 1.500 ng/ul m

RT: 23.291 min Scan# 3436

Delta R.T. -0.012 min

Lab File: BM036590.D

Acq: 19 Sep 2022 21:12

Instrument :

BNA_M

ClientSampleId :





A5782

Tgt Ion:252 Resp: 193625
 Ion Ratio Lower Upper
 252 100
 253 23.8 17.8 26.8
 125 15.2 8.2 12.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/20/2022
 Supervised By :mohammad ahmed 09/21/2022

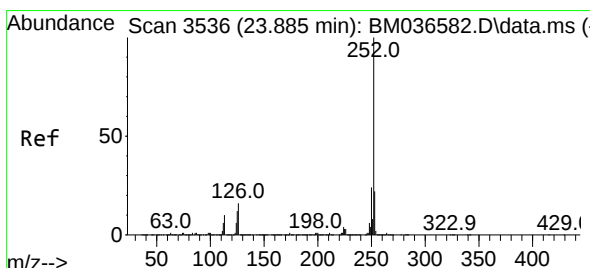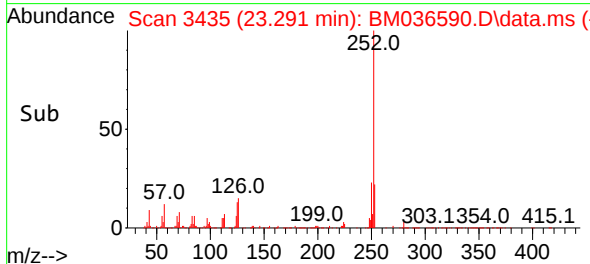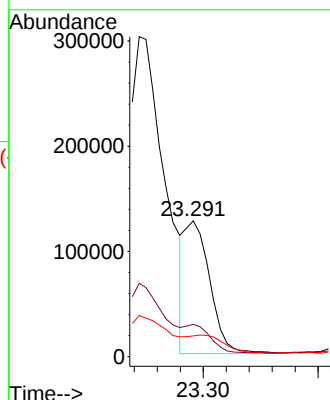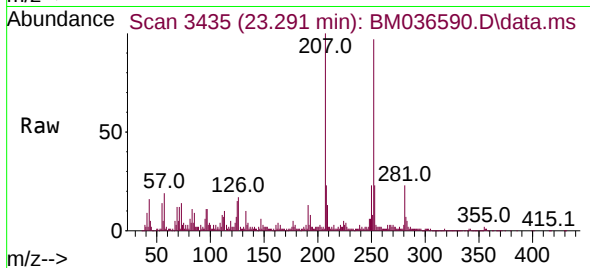

#93

Benzo(a)pyrene

Concen: 2.518 ng/ul




RT: 23.885 min Scan# 3536


Delta R.T. -0.006 min

Lab File: BM036590.D

Acq: 19 Sep 2022 21:12

Tgt Ion:252 Resp: 286017
 Ion Ratio Lower Upper
 252 100
 253 24.0 17.5 26.3
 125 13.5 9.5 14.3

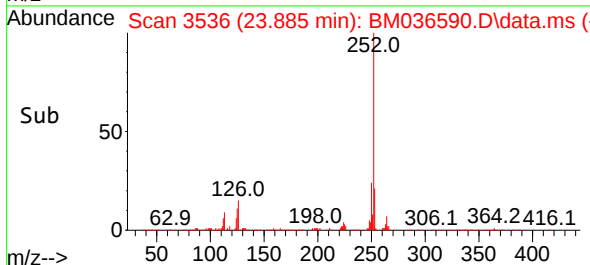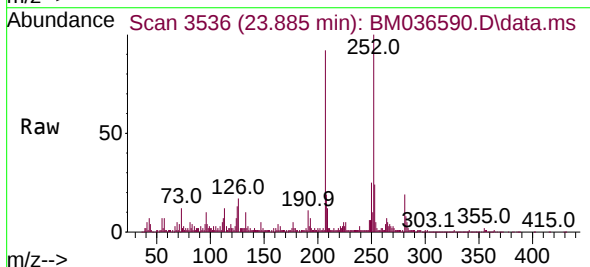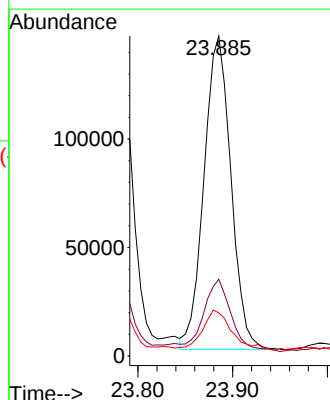

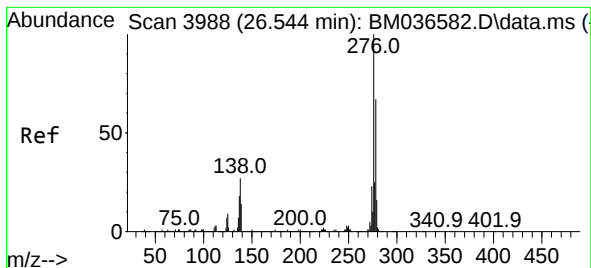

#94

Indeno(1,2,3-cd)pyrene

Concen: 1.414 ng/ul

RT: 26.538 min Scan# 3988

Delta R.T. -0.012 min

Lab File: BM036590.D

Acq: 19 Sep 2022 21:12

Instrument :

BNA_M

ClientSampleId :

A5782





Tgt Ion: 276 Resp: 187576

Ion	Ratio	Lower	Upper
276	100		
138	25.8	20.2	30.4
277	23.8	19.7	29.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

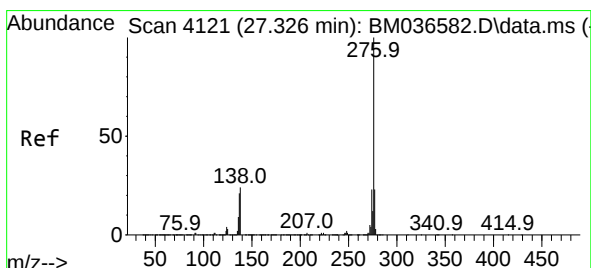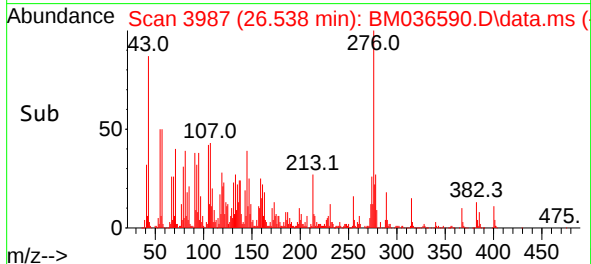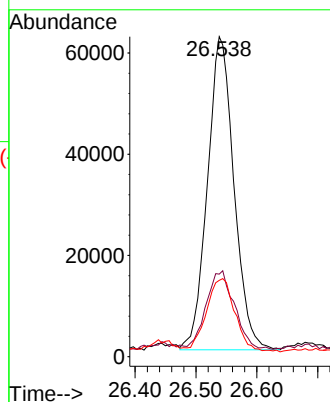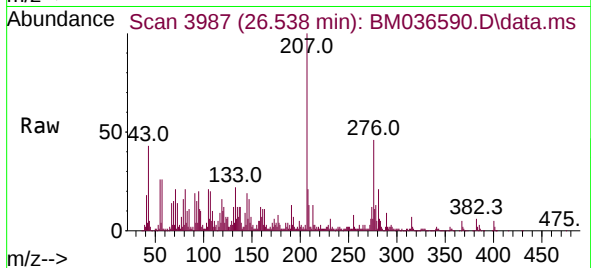

#96

Benzo(g,h,i)perylene

Concen: 1.271 ng/ul

RT: 27.315 min Scan# 4119

Delta R.T. -0.018 min

Lab File: BM036590.D

Acq: 19 Sep 2022 21:12

Tgt Ion: 276 Resp: 146187

Ion	Ratio	Lower	Upper
276	100		
138	24.5	18.7	28.1
277	25.1	19.2	28.8

