

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
 Data File : BM047570.D
 Acq On : 19 Sep 2024 14:34
 Operator : RC/JU
 Sample : P3845-22
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 RR-TRIAZINE-WP

Quant Time: Sep 19 15:29:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 08:56:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	294611	20.000	ng	-0.01
21) Naphthalene-d8	10.634	136	1113898	20.000	ng	-0.01
39) Acenaphthene-d10	14.469	164	542943	20.000	ng	-0.01
64) Phenanthrene-d10	17.204	188	990223	20.000	ng	-0.01
76) Chrysene-d12	21.433	240	743798	20.000	ng	-0.01
86) Perylene-d12	24.456	264	838933	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	2967957	160.402	ng	0.00
7) Phenol-d6	7.004	99	3801297	145.880	ng	0.00
23) Nitrobenzene-d5	8.993	82	2327347	104.565	ng	-0.01
42) 2,4,6-Tribromophenol	15.951	330	787399	150.037	ng	-0.01
45) 2-Fluorobiphenyl	13.098	172	4185573	106.194	ng	-0.01
79) Terphenyl-d14	19.821	244	5441080	131.085	ng	-0.01
Target Compounds						Qvalue
69) Atrazine	16.669	200	160710	19.194	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
Data File : BM047570.D
Acq On : 19 Sep 2024 14:34
Operator : RC/JU
Sample : P3845-22
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RR-TRIAZINE-WP

Quant Time: Sep 19 15:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

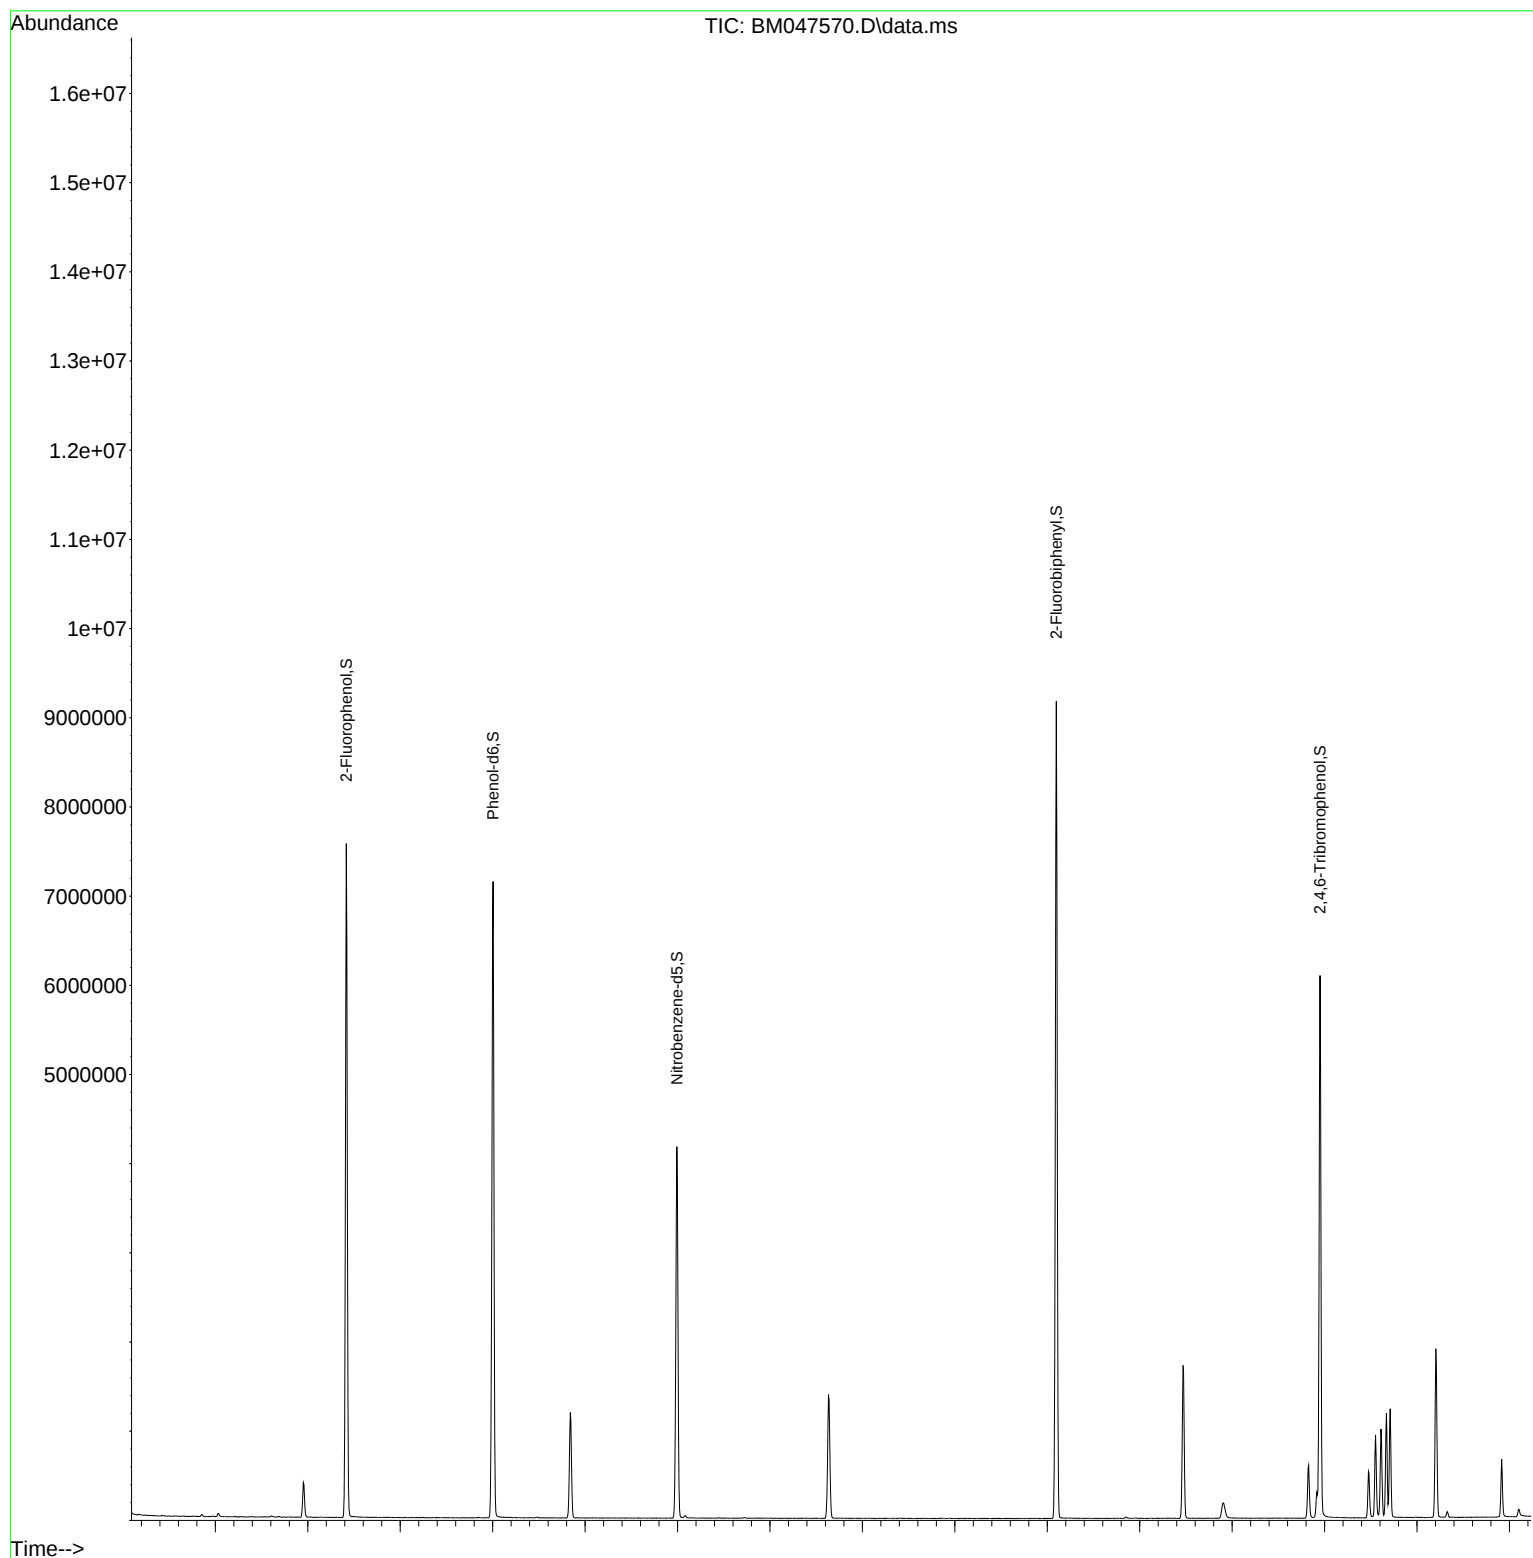

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
Data File : BM047570.D
Acq On : 19 Sep 2024 14:34
Operator : RC/JU
Sample : P3845-22
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
RR-TRIAZINE-WP

Quant Time: Sep 19 15:29:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

