
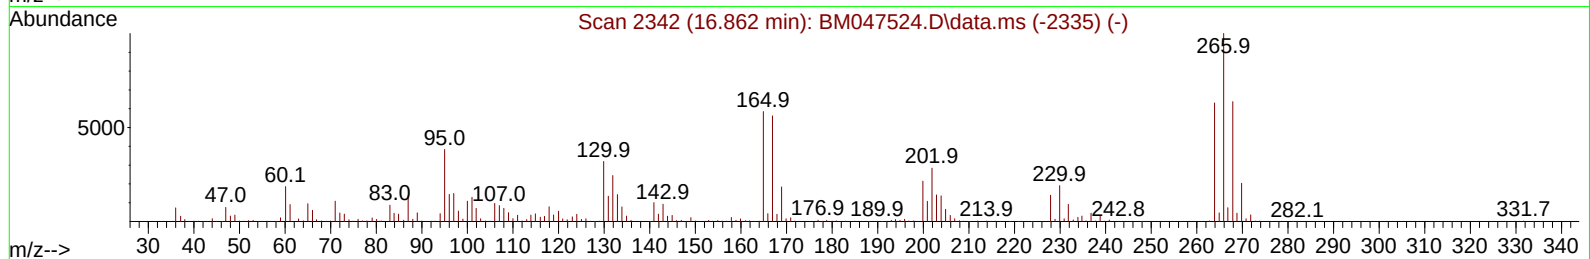
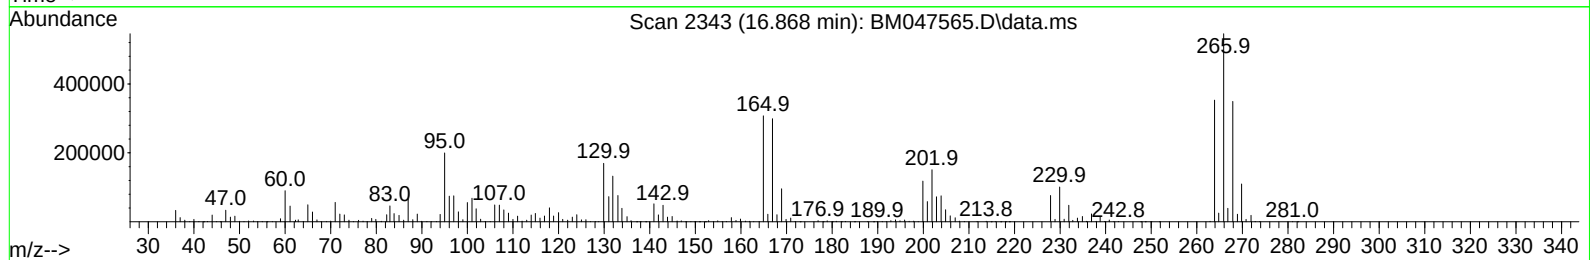


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
Data File : BM047565.D
Acq On : 19 Sep 2024 08:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 12:50:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

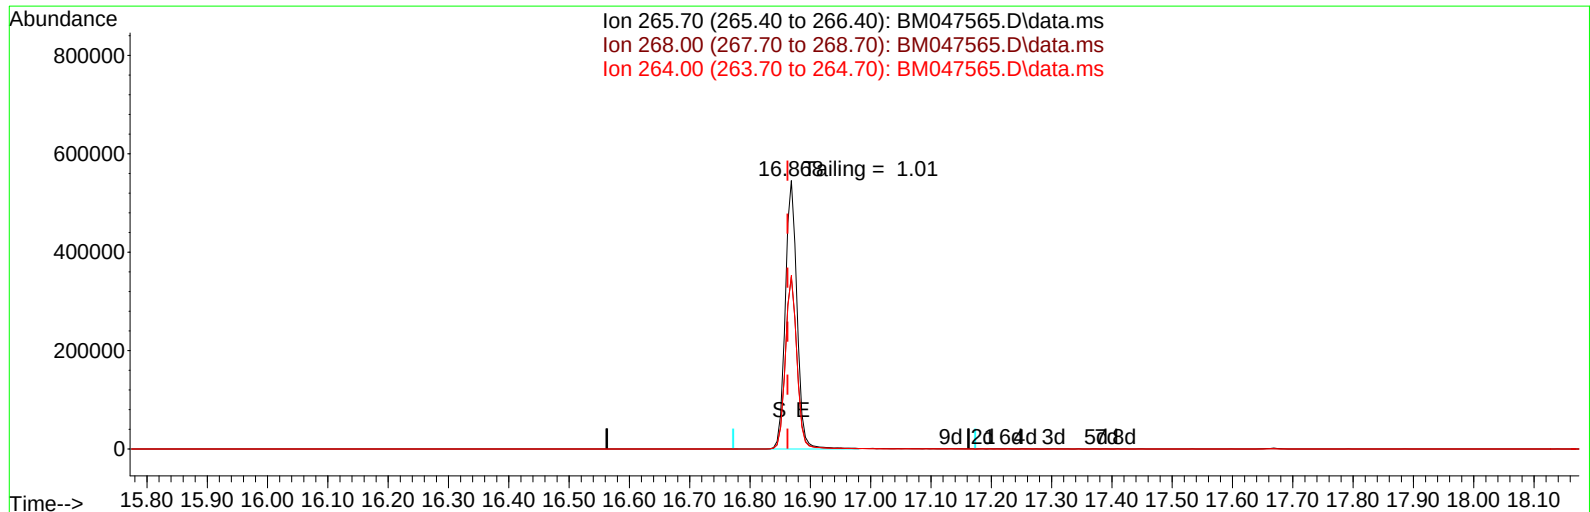

TIC: BM047565.D\data.ms

(70) Pentachlorophenol (C)




16.868min (+ 0.006) 28826.43 ng m

response 749732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.05
264.00	63.00	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091924\
Data File : BM047565.D
Acq On : 19 Sep 2024 08:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 12:50:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 08:56:37 2024
Response via : Initial Calibration

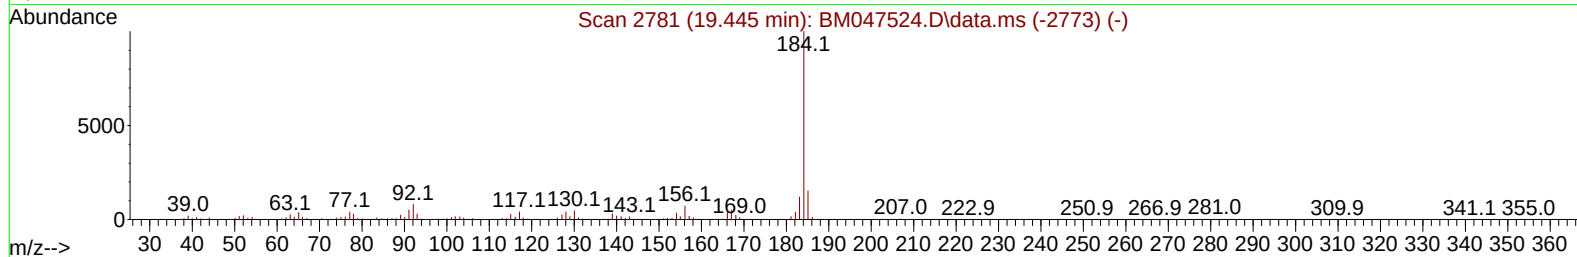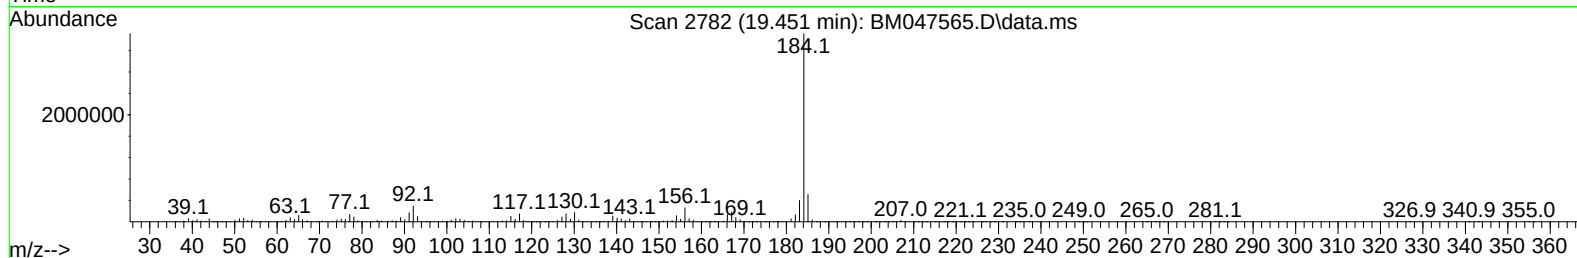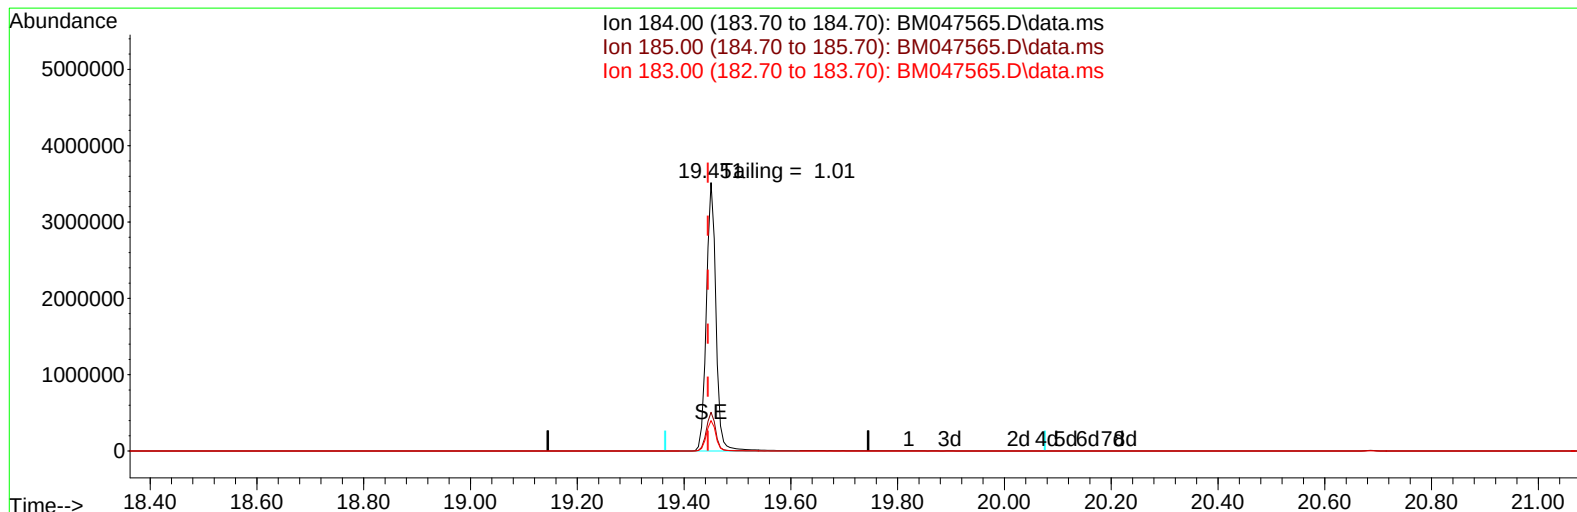

TIC: BM047565.D\data.ms

(77) Benzidine

19.451min (+ 0.006) 2160538.53 ng m

response 4472986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.44
183.00	12.00	11.35
0.00	0.00	0.00