

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM092017\
 Data File : BM011631.D
 Acq On : 20 Sep 2017 11:12
 Operator : SJ/JU
 Sample : I5271-14DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AH5DL

Manual Integrations
 APPROVED

Sohil
 9/22/2017 4:05:07 PM

Quant Time: Sep 21 02:15:22 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 21 01:44:48 2017
 Response via : Initial Calibration

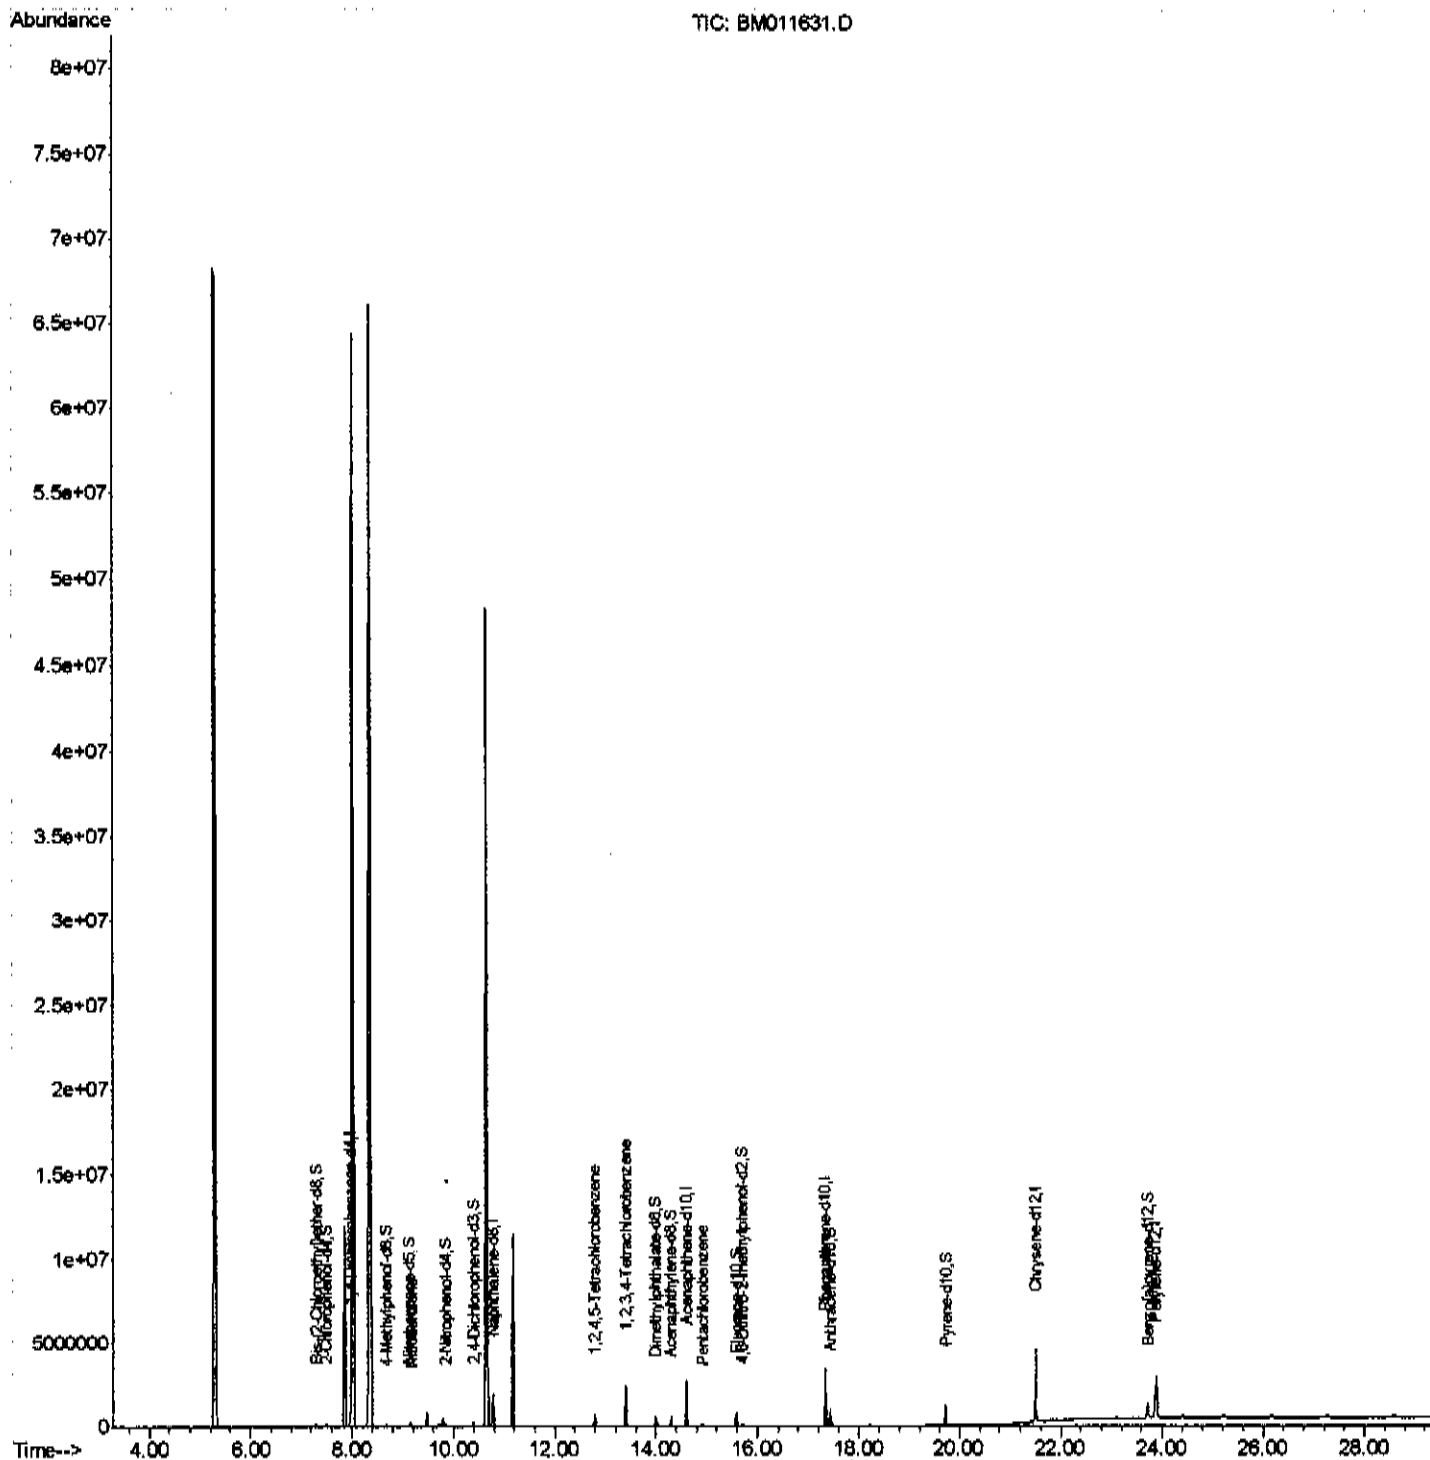

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM092017\
 Data File : BM011631.D
 Acq On : 20 Sep 2017 11:12
 Operator : SJ/JU
 Sample : I5271-14DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AH5DL

Manual Integrations
 APPROVED

Sohil
 9/22/2017 4:05:07 PM

Quant Time: Sep 21 01:47:05 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 21 01:44:48 2017
 Response via : Initial Calibration

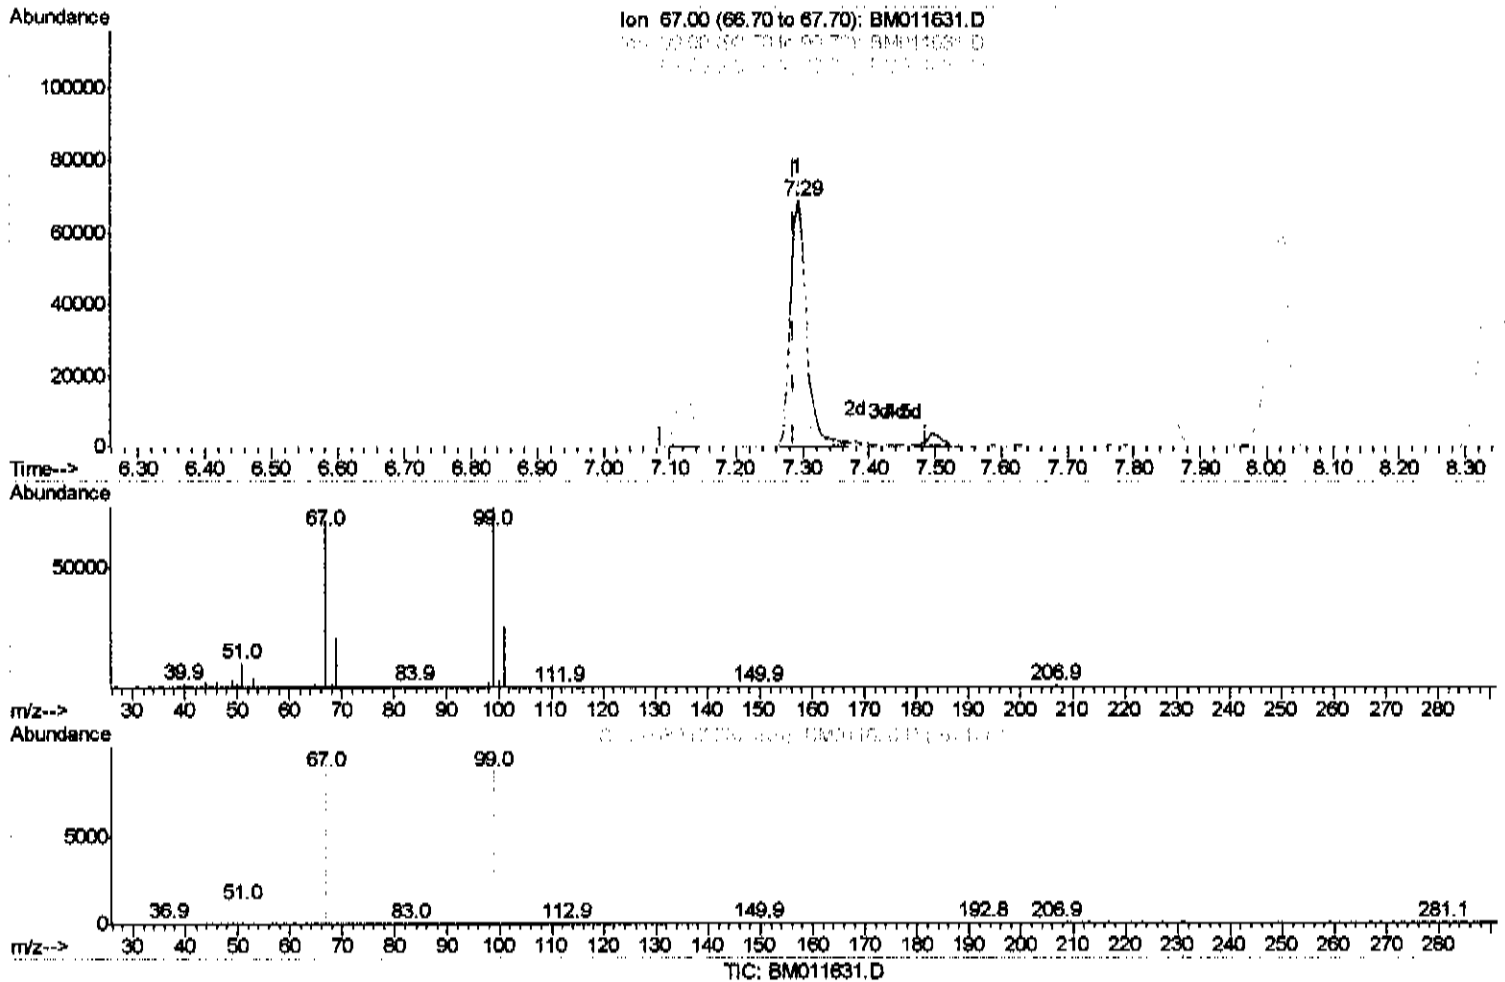

(7) Bis-(2-Chloroethyl)ether-d8 (S)

7.293min (+0.006) 4.97ng/ul

response 116405

Ion	Exp%	Act%
67.00	100	100
99.00	117.60	108.41
69.00	33.70	30.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM092017\
 Data File : BM011631.D
 Acq On : 20 Sep 2017 11:12
 Operator : SJ/JU
 Sample : I5271-14DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH5DL

Quant Time: Sep 21 02:15:22 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 Last Update : Thu Sep 21 01:44:48 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 9/22/2017 4:05:07 PM

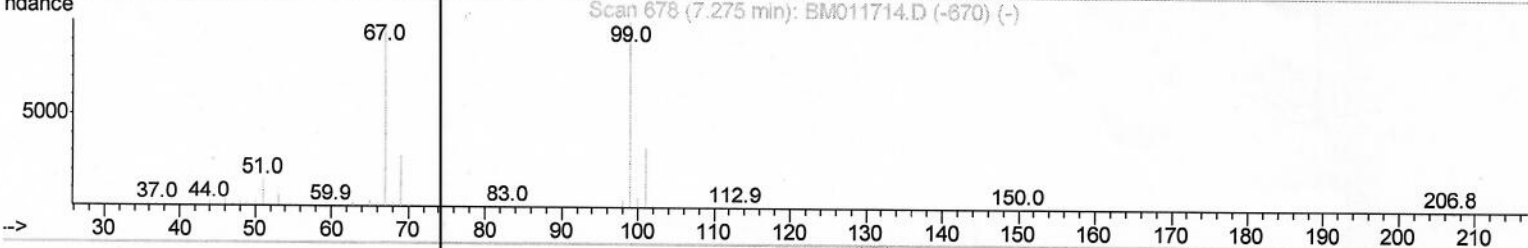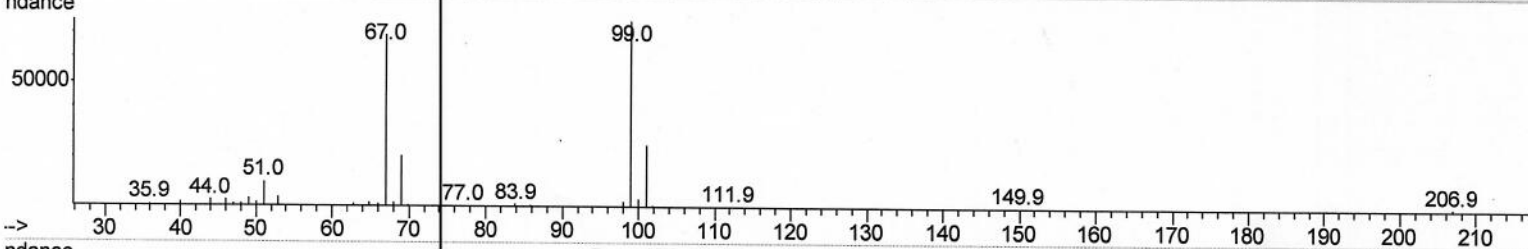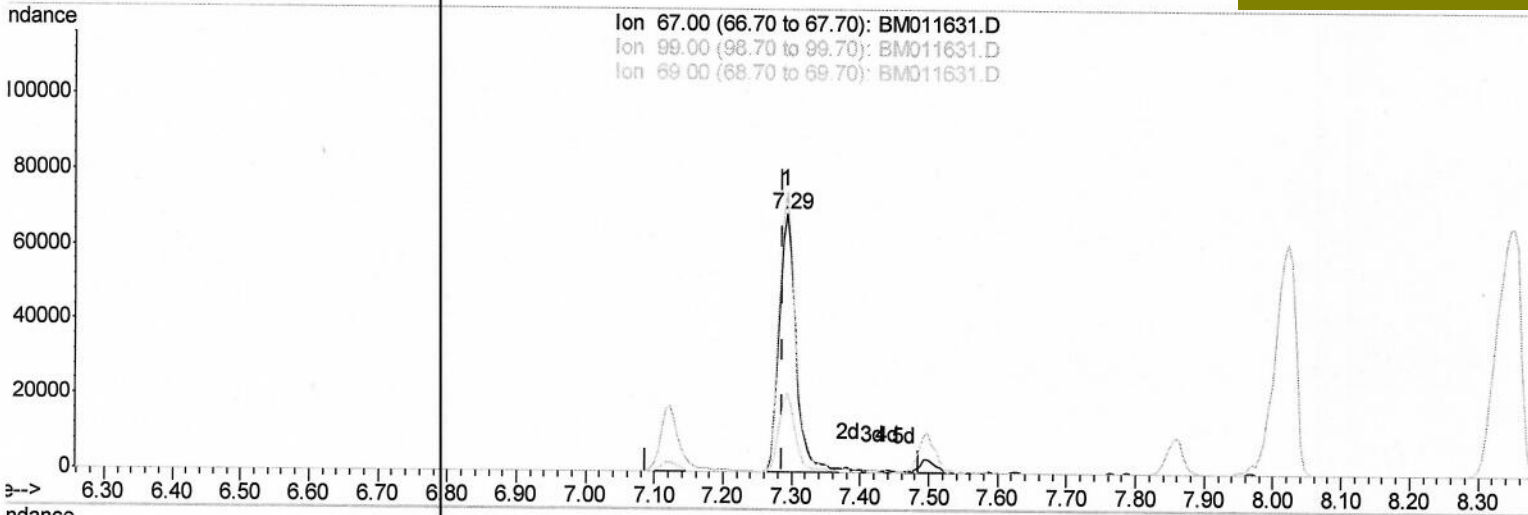

TIC: BM011631.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

7.293min (+0.006) 5.09ng/ul m >

response 119211

Ion	Exp%	Act%
67.00	100	100
99.00	117.60	108.41
69.00	33.70	30.19
0.00	0.00	0.00

JU
 09/25/17

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM092017\
 Data File : BM011631.D
 Acq On : 20 Sep 2017 11:12
 Operator : SJ/JU
 Sample : I5271-14DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AH5DL

Manual Integrations
 APPROVED

Sohil
 9/22/2017 4:05:07 PM

Quant Time: Sep 21 01:47:05 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 OLast Update : Thu Sep 21 01:44:48 2017
 Response via : Initial Calibration

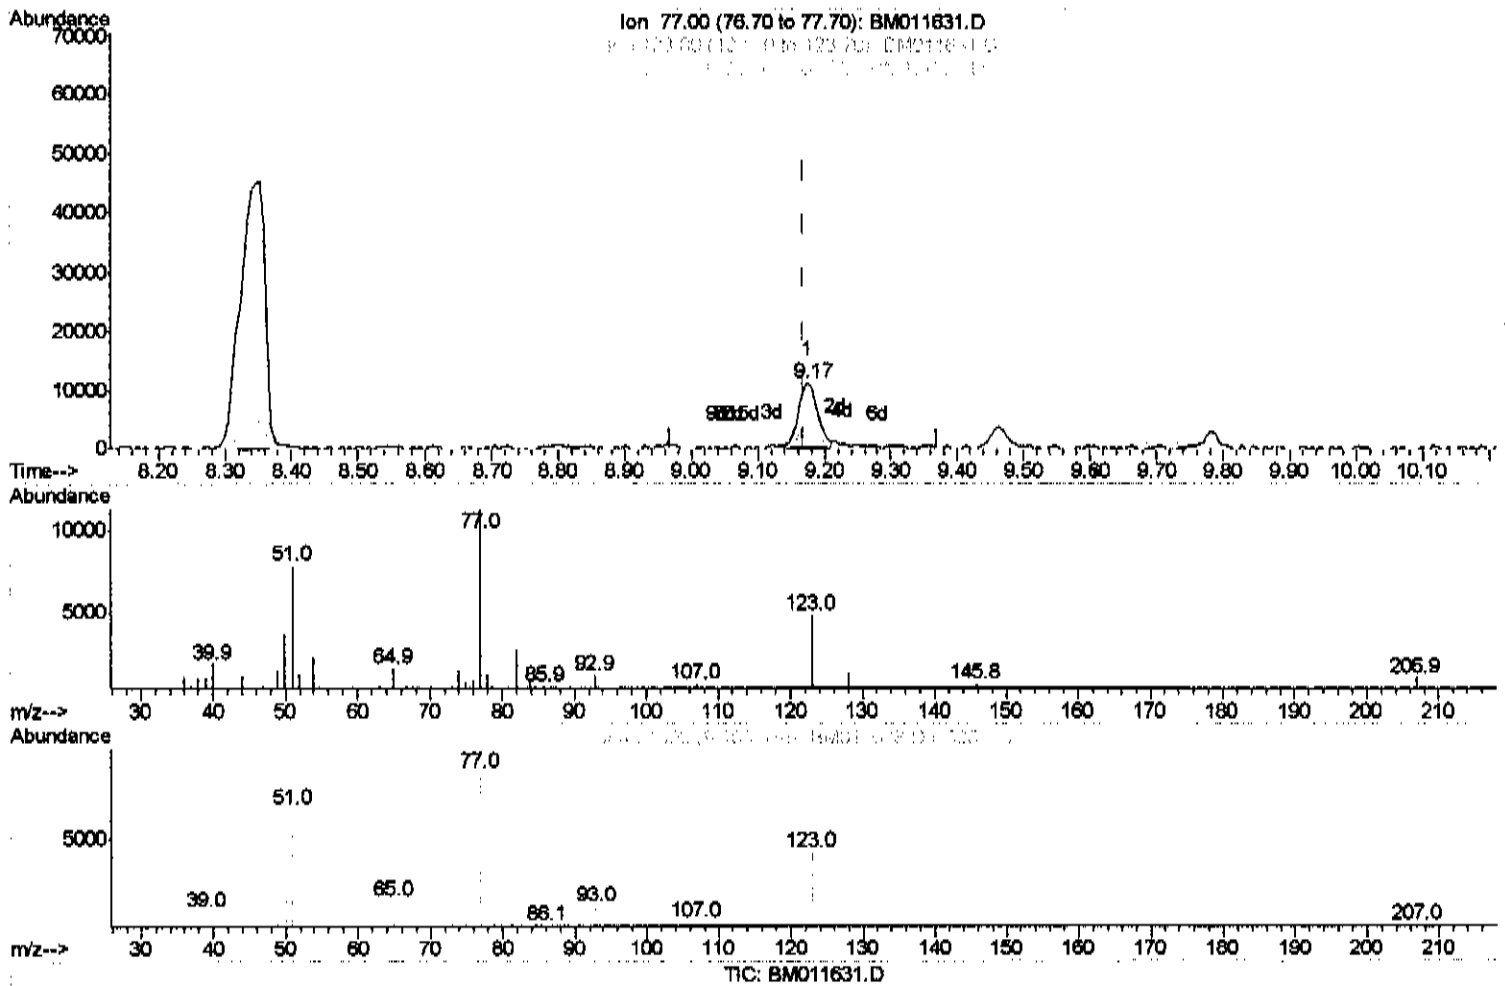

(20) Nitrobenzene

9.175min (+0.006) 0.85ng/ul

response 22112

Ion	Exp%	Act%
77.00	100	100
123.00	39.80	42.04
65.00	13.30	13.66
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM092017\
 Data File : BM011631.D
 Acq On : 20 Sep 2017 11:12
 Operator : SJ/JU
 Sample : I5271-14DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH5DL

Manual Integrations
 APPROVED

Sohil
 9/22/2017 4:05:07 PM

Quant Time: Sep 21 01:47:05 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 21 01:44:48 2017
 Response via : Initial Calibration

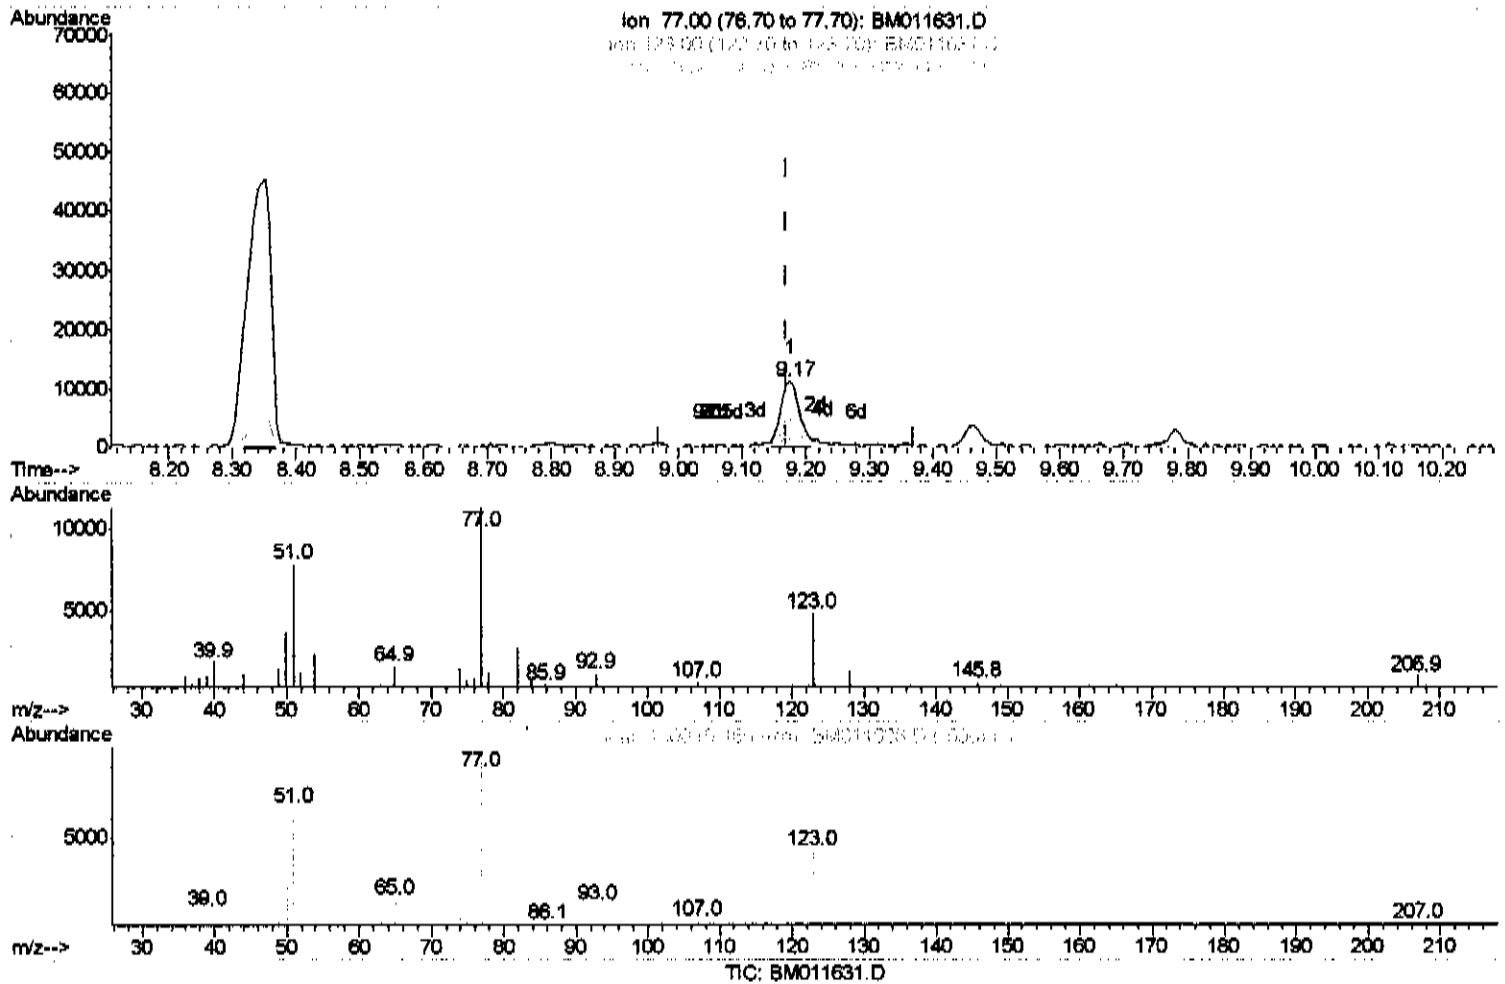

(20) Nitrobenzene

9.175min (+0.006) 1.03ng/ul m

response 26800

Ion	Exp%	Act%
77.00	100	100
123.00	39.80	42.04
65.00	13.30	13.86
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_M
ClientSampled :
COAH5DL

Manual Integrations
APPROVED

Sohil
9/22/2017 4:05:07 PM

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092017\
Data File : BM011631.D
Acq On : 20 Sep 2017 11:12
Operator : SJ/JU
Sample : I5271-14DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Sep 21 02:15:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION
OLast Update : Thu Sep 21 01:44:48 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	361656	20.00	ng/ul	0.01
18) Naphthalene-d8	10.77	136	1463024	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	863466	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.33	188	1919418	20.00	ng/ul	0.00
78) Chrysene-d12	21.50	240	1933507	20.00	ng/ul	0.00
86) Perylene-d12	23.87	264	1705700	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.39	96	2424	0.30	ng/uL	0.00
5) Phenol-d5	7.12	99	32748	0.94	ng/ul	0.01
7) Bis-(2-Chloroethyl) ether-d	7.29	67	119211m	5.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.50	132	101127	3.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.66	113	58586	2.16	ng/ul	0.00
19) Nitrobenzene-d5	9.13	128	58926	5.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.85	143	57601	4.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.39	165	113419	4.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	719	0.03	ng/ul	0.04
44) Dimethylphthalate-d6	14.00	166	406414	5.57	ng/ul	0.00
47) Acenaphthylene-d8	14.29	160	444478	5.03	ng/ul	0.00
52) 4-Nitrophenol-d4	14.81	143	1046	0.08	ng/ul	0.03
58) Fluorene-d10	15.59	176	356214	5.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.70	200	34131	3.06	ng/ul	0.00
71) Anthracene-d10	17.43	188	544973	5.77	ng/ul	0.00
79) Pvrene-d10	19.72	212	611030	6.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.72	264	472030	5.81	ng/ul	0.00

Target Compounds

20) Nitrobenzene	9.17	77	26800m	1.026	ng/ul	98
37) 1,2,4,5-Tetrachlorobenzene	12.79	216	294268	11.489	ng/ul	99
73) 1,2,3,4-Tetrachlorobenzene	13.40	216	690889	27.012	ng/uL	99
74) Pentachlorobenzene	14.92	250	35216	1.358	ng/uL	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed