

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
 Data File : BM047581.D
 Acq On : 20 Sep 2024 09:40
 Operator : RC/JU
 Sample : SSTDICC2.5
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC2.5

Quant Time: Sep 20 16:18:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 14:56:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	315099	20.000	ng	0.00
21) Naphthalene-d8	10.645	136	1223771	20.000	ng	0.00
39) Acenaphthene-d10	14.474	164	638196	20.000	ng	0.00
64) Phenanthrene-d10	17.209	188	1188407	20.000	ng	0.00
76) Chrysene-d12	21.439	240	1031871	20.000	ng	0.00
86) Perylene-d12	24.462	264	1155247	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	0.000	112	0d	0.000	ng	
7) Phenol-d6	0.000	99	0d	0.000	ng	
23) Nitrobenzene-d5	0.000	82	0d	0.000	ng	
42) 2,4,6-Tribromophenol	0.000	330	0d	0.000	ng	
45) 2-Fluorobiphenyl	0.000	172	0d	0.000	ng	
79) Terphenyl-d14	0.000	244	0d	0.000	ng	
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	8.651	70	37552	2.263	ng	# 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047581.D
Acq On : 20 Sep 2024 09:40
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Sep 20 16:18:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 14:56:16 2024
Response via : Initial Calibration

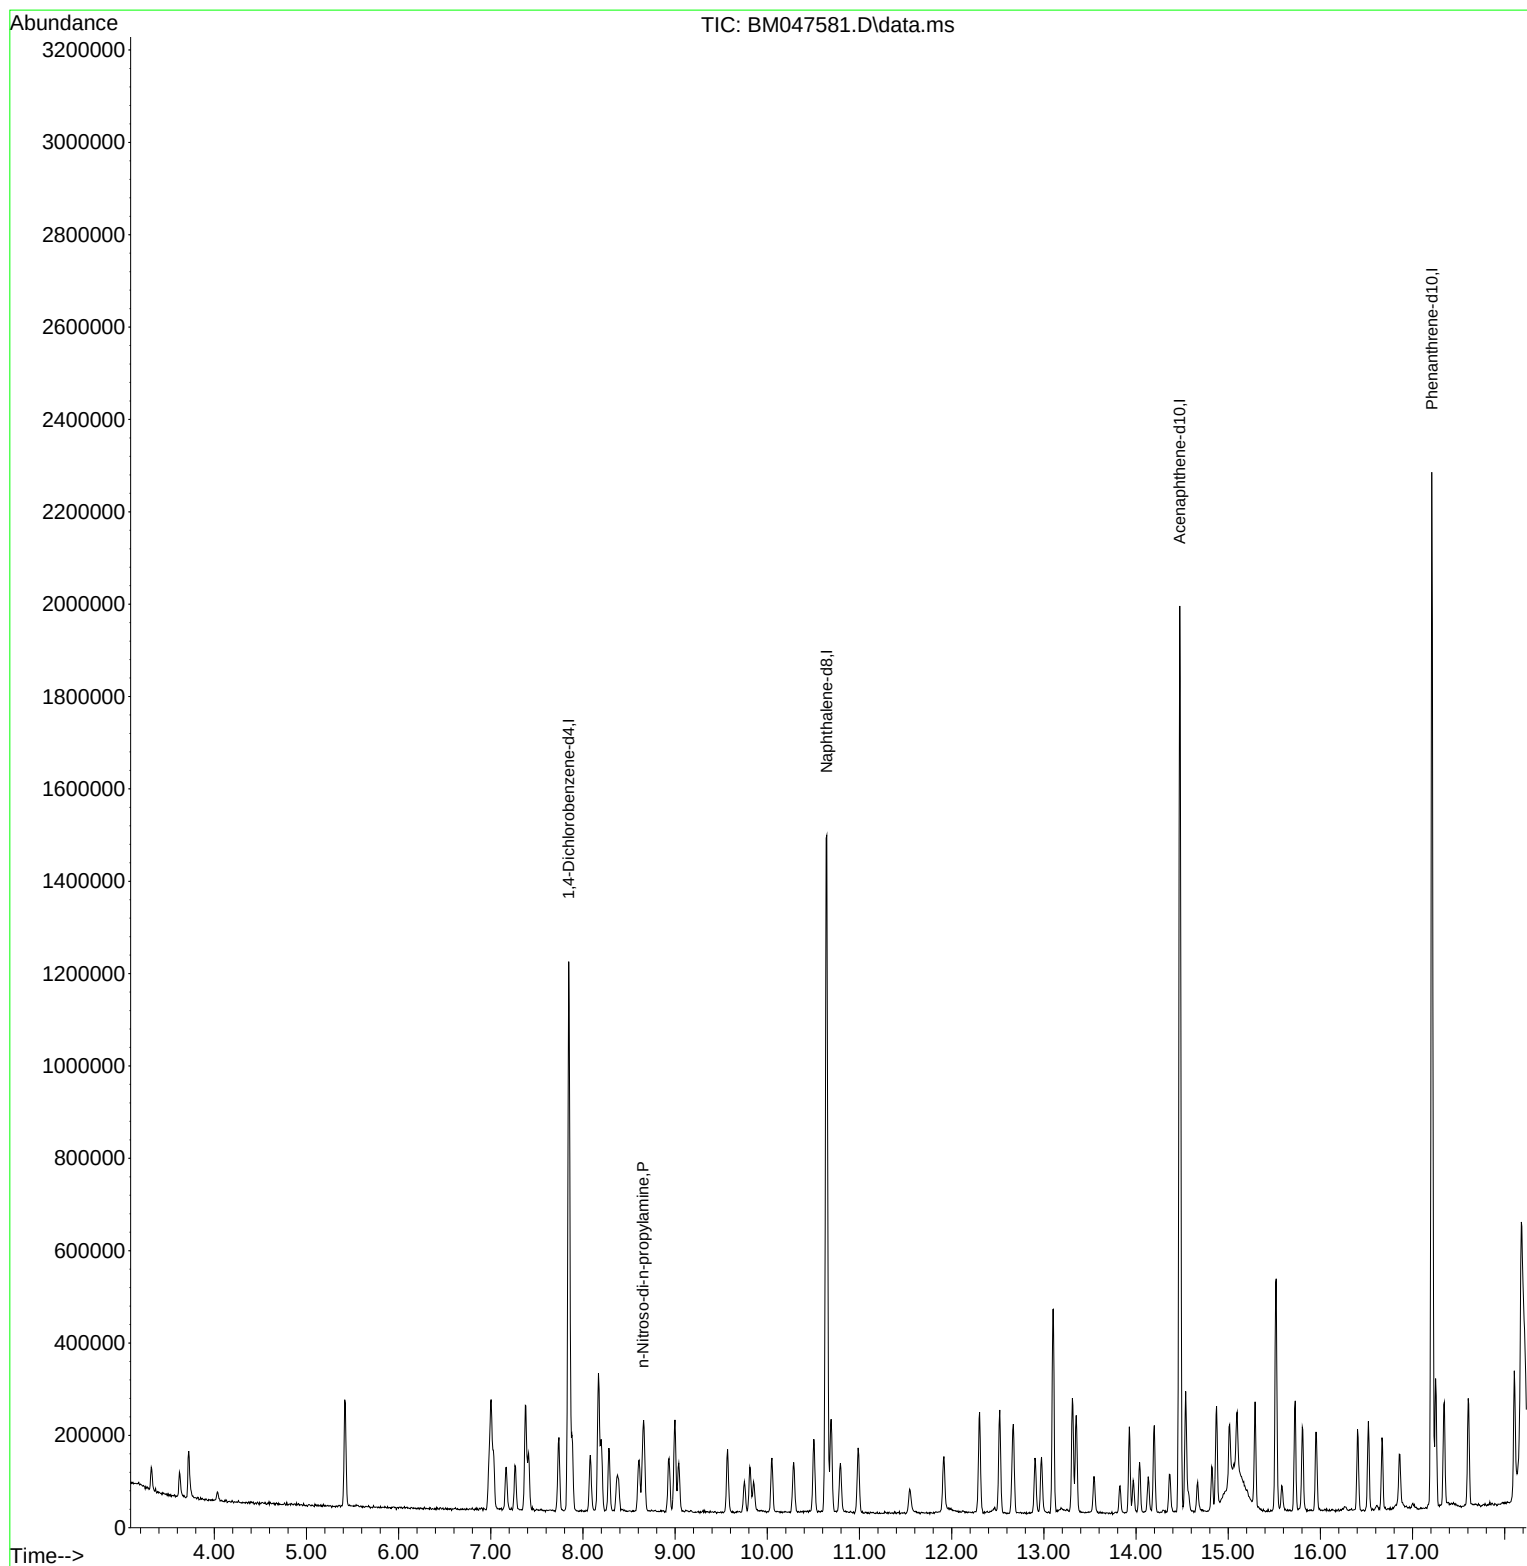

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047581.D
Acq On : 20 Sep 2024 09:40
Operator : RC/JU
Sample : SSTDICC2.5
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC2.5

Quant Time: Sep 20 16:18:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 14:56:16 2024
Response via : Initial Calibration

